

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121923\
 Data File : PD080170.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2023 18:40
 Operator : AR\AJ
 Sample : 05794-17
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGRG0

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/18/2023
 Supervised By :Ankita Jodhani 12/18/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 20:59:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 03:10:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.818	35564716	41557707	27.855	18.690 #
2)	SA Decachlor...	9.102	7.956	34496078	40472081	21.456	16.862m
Target Compounds							
12)	B 4,4'-DDE	6.230	5.277	9042.7E6	6262.5E6	4681.045	1993.776 #
14)	MA Endrin	6.609	5.650	1180.4E6	1868.7E6	753.631	710.224m
16)	A 4,4'-DDD	6.743	5.829	8354.5E6	8923.4E6	6023.114m	3881.005m#
17)	MA 4,4'-DDT	7.057	6.079	2452.3E6	4185.7E6	1659.499m	1735.955m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121923\
Data File : PD080170.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2023 18:40
Operator : AR\AJ
Sample : 05794-17
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 20:59:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 03:10:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

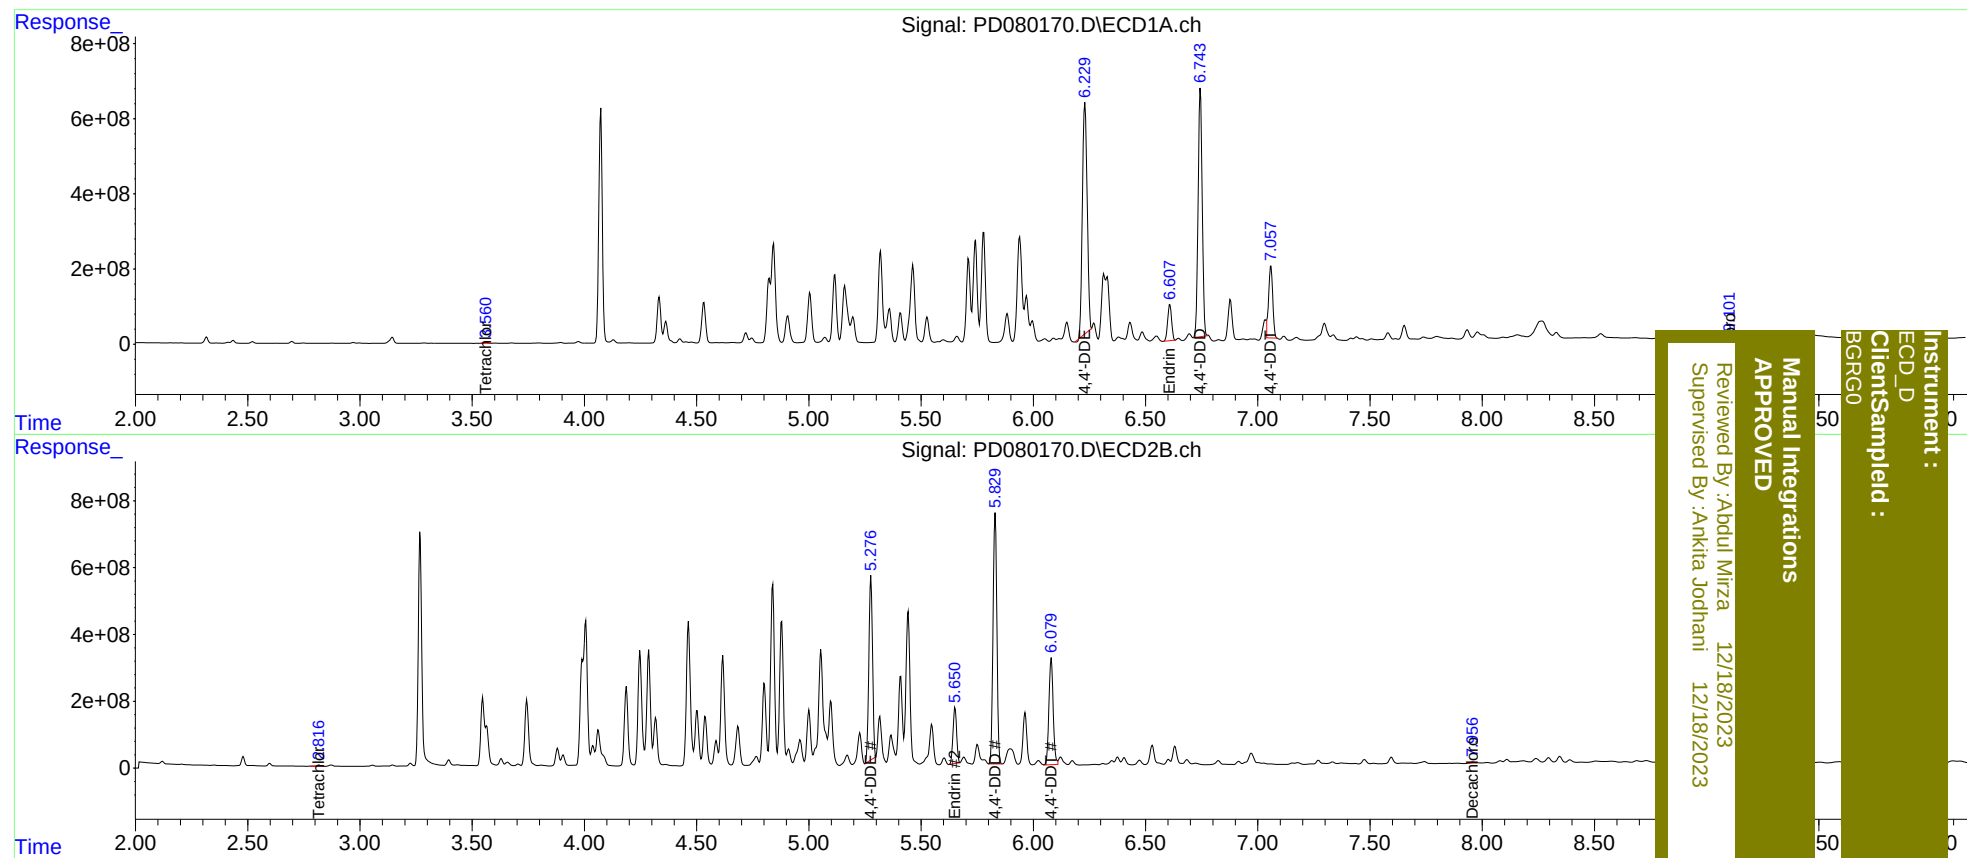

Reviewed By: Abdul Mirza 12/18/2023
Supervised By: Ankita Jodhani 12/18/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
BGRG0