

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121923\
 Data File : PD080177.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Dec 2023 20:13
 Operator : AR\AJ
 Sample : 05794-24
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGRG5

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/19/2023
 Supervised By : Ankita Jodhani 12/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 21:01:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 03:10:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.568	2.801	12564265	29950289	9.841	13.470 #
2)	SA Decachlor...	9.099	7.941	44986250	49980187	27.981	20.823 #
Target Compounds							
9)	A Endosulfan I	6.138	5.152	56959721	140.1E6	31.975m	51.089m#
12)	B 4,4'-DDE	6.226	5.259	22307466	57038048	11.548m	18.159m#
16)	A 4,4'-DDD	6.737	5.811	37826742	32290516	27.271	14.044m#
17)	MA 4,4'-DDT	7.060	6.063	78059744	114.4E6	52.823	47.450m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121923\
Data File : PD080177.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Dec 2023 20:13
Operator : AR\AJ
Sample : 05794-24
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 21:01:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 03:10:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

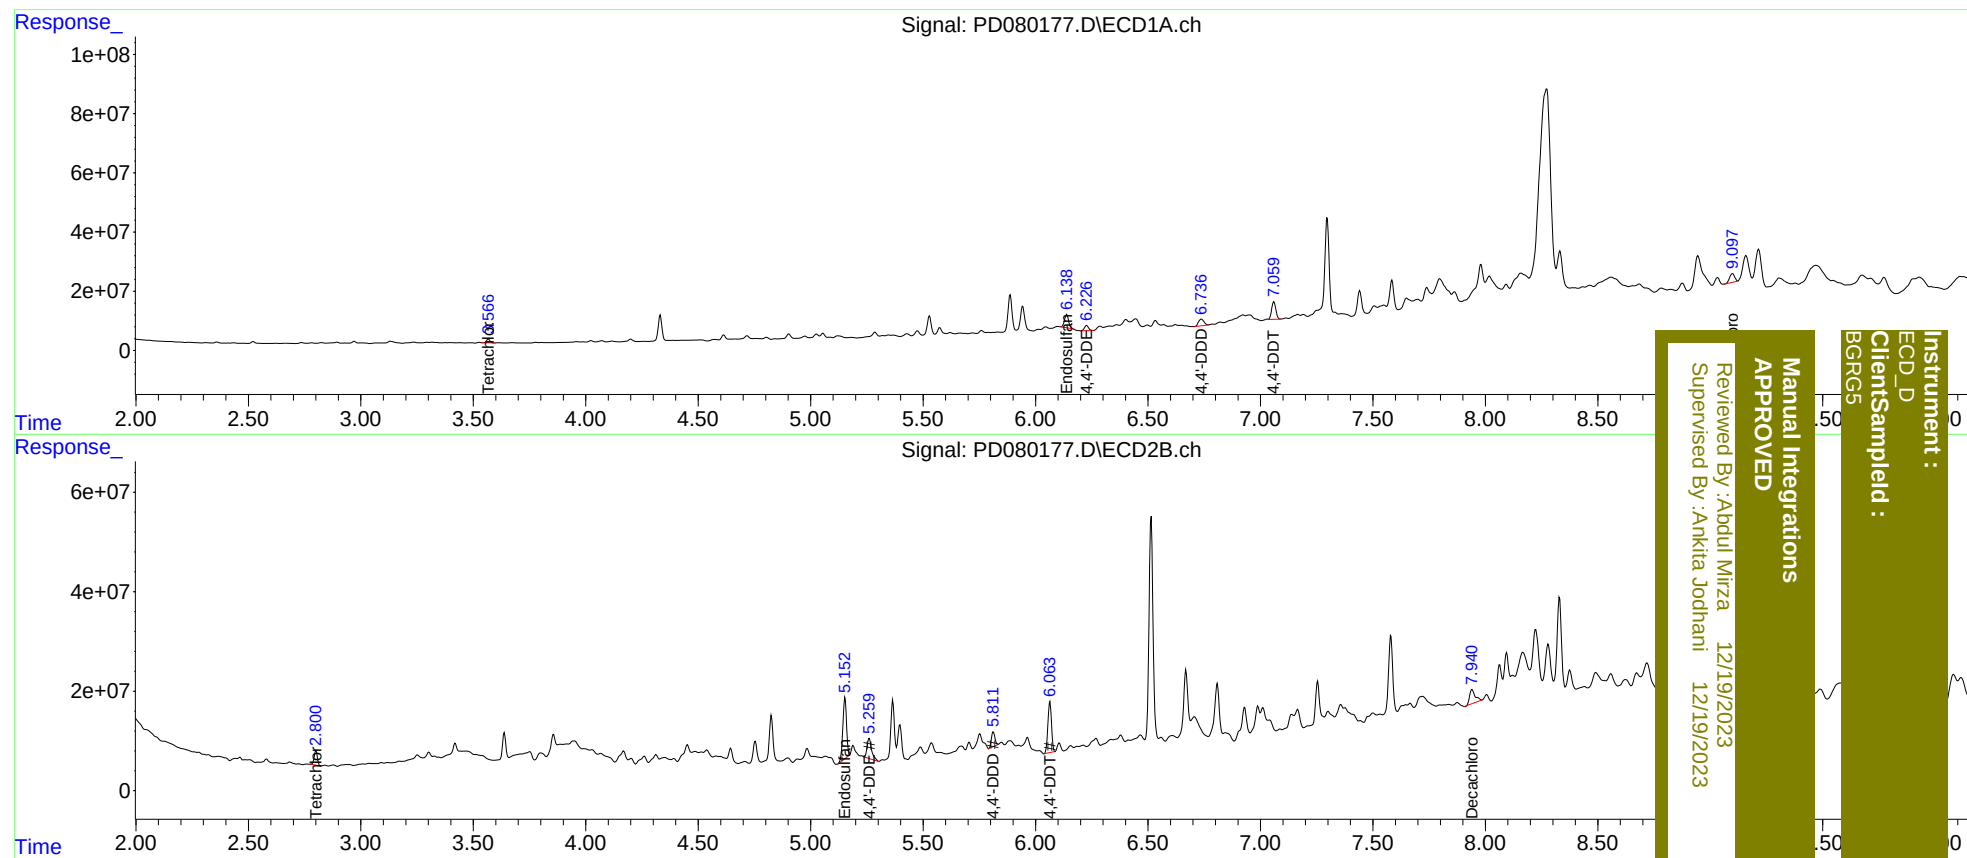

Instrument :
ECD_D
ClientSampled :
BGRGS

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/19/2023
Supervised By :Ankita Jodhani 12/19/2023