

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121924\
 Data File : PD087191.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2024 14:24
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA2043

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 05:40:51 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121924CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 20 05:39:10 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.556	2.883	20855281	119.7E6	10.495	10.837
27)	SA Decachlor...	9.083	8.085	62488575	270.3E6	21.439	21.844
Target Compounds							
2)	A alpha-BHC	4.005	3.397	37863987	182.2E6	9.824	10.472
3)	MA gamma-BHC...	4.336	3.734	37645493	171.6E6	10.048	10.656
4)	MA Heptachlor	4.936	4.089	38771149	177.9E6	10.204	10.766
9)	A Endosulfan I	6.081	5.254	33411178	150.0E6	10.422	10.804
13)	MA Dieldrin	6.354	5.520	69472057	315.4E6	20.040	21.460
14)	MA Endrin	6.582	5.797	58009502	292.7E6	20.104	21.849
16)	A 4,4'-DDD	6.712	5.938	49687008	250.4E6	19.988	21.426
17)	MA 4,4'-DDT	7.028	6.192	51763557	256.4E6	19.993	20.954
20)	A Methoxychlor	7.500	6.764	150.3E6	633.1E6	103.548	111.266


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121924\
Data File : PD087191.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2024 14:24
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 05:40:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121924CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 05:39:10 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

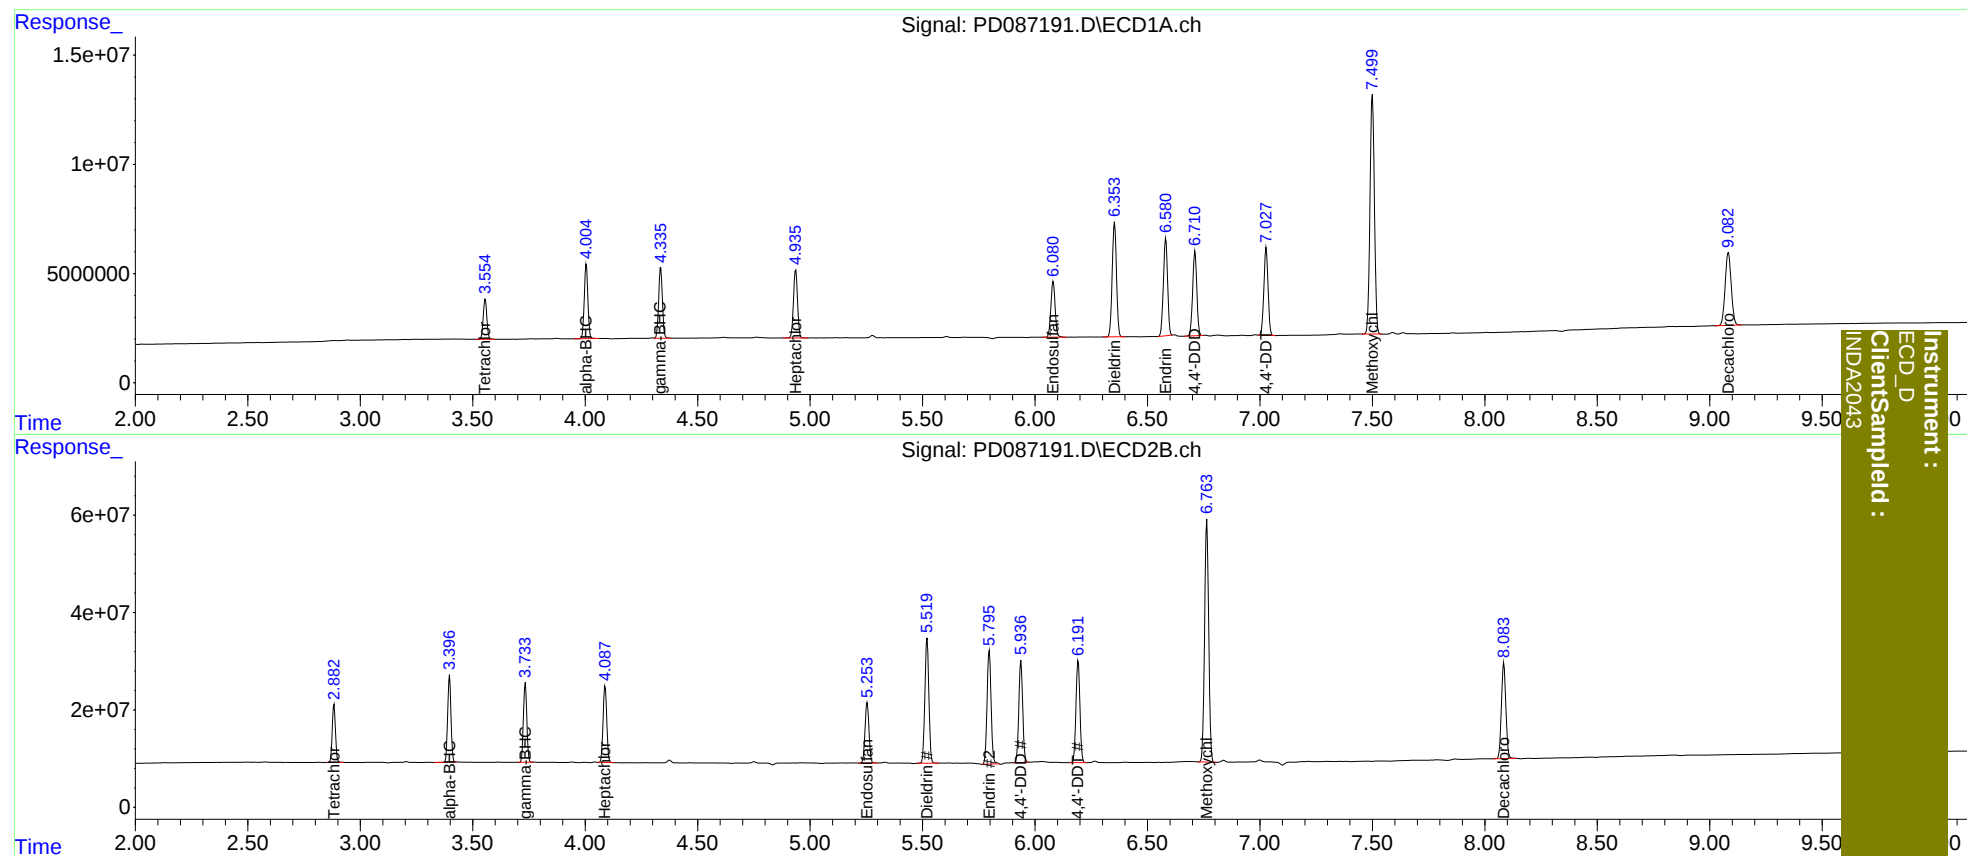


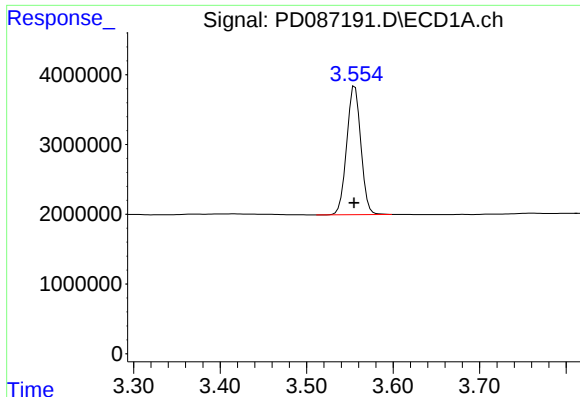

#1 Tetrachloro-m-xylene


R.T.: 3.556 min
Delta R.T.: 0.000 min
Response: 20855281
Conc: 10.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA2043

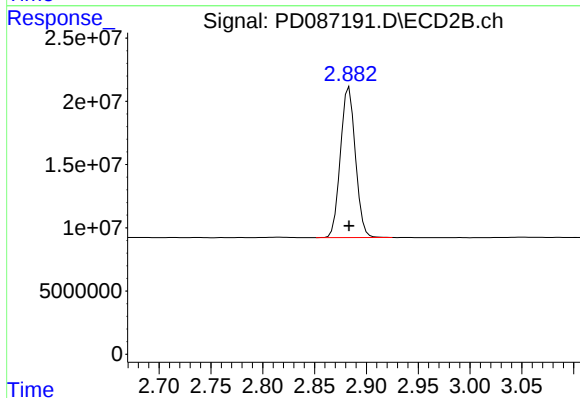


#1 Tetrachloro-m-xylene

R.T.: 2.883 min
Delta R.T.: 0.000 min
Response: 119666364
Conc: 10.84 ng/ml

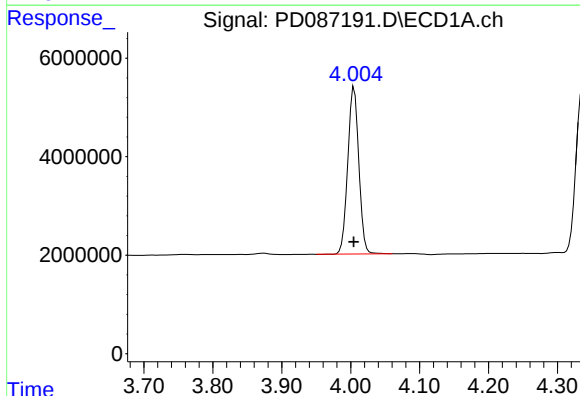


#2 alpha-BHC

R.T.: 4.005 min
Delta R.T.: 0.000 min
Response: 37863987
Conc: 9.82 ng/ml

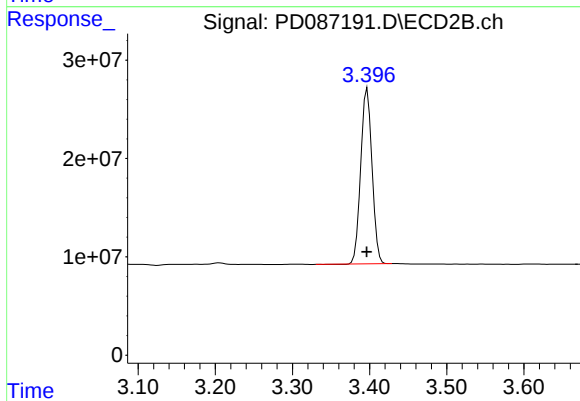

#2 alpha-BHC


R.T.: 3.397 min
Delta R.T.: 0.000 min
Response: 182163327
Conc: 10.47 ng/ml

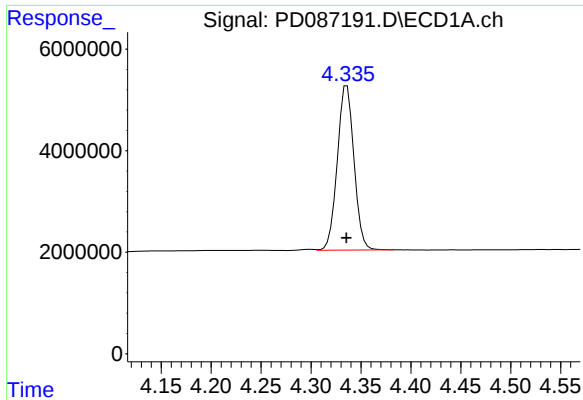

#3 gamma-BHC (Lindane)


R.T.: 4.336 min
Delta R.T.: 0.000 min
Response: 37645493
Conc: 10.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA2043

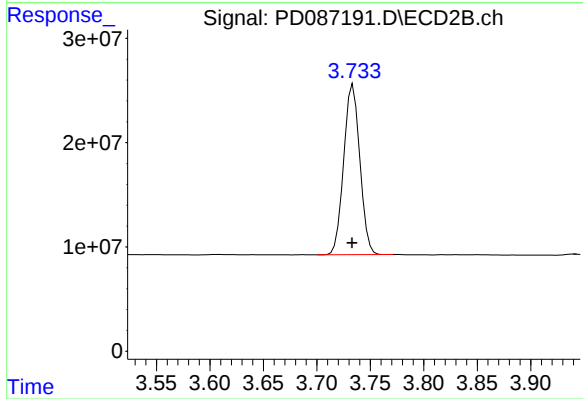


#3 gamma-BHC (Lindane)

R.T.: 3.734 min
Delta R.T.: 0.000 min
Response: 171571643
Conc: 10.66 ng/ml

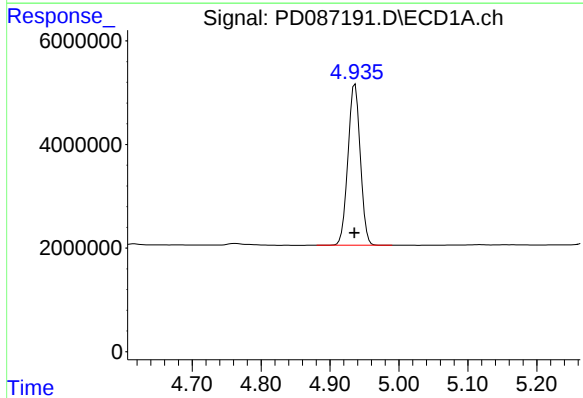


#4 Heptachlor

R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 38771149
Conc: 10.20 ng/ml

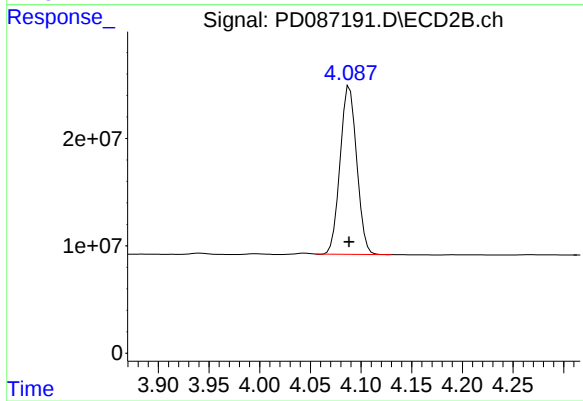

#4 Heptachlor


R.T.: 4.089 min
Delta R.T.: 0.000 min
Response: 177928997
Conc: 10.77 ng/ml

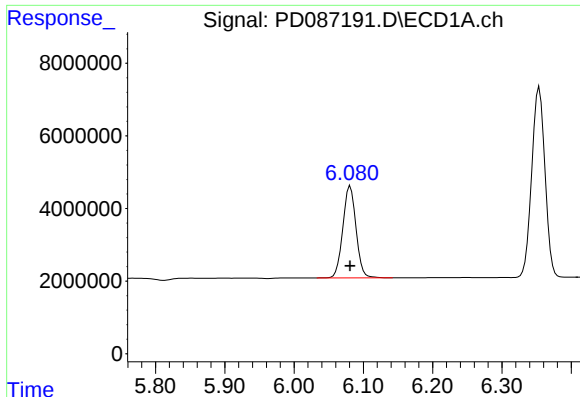

#9 Endosulfan I


R.T.: 6.081 min
Delta R.T.: 0.000 min
Response: 33411178
Conc: 10.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA2043

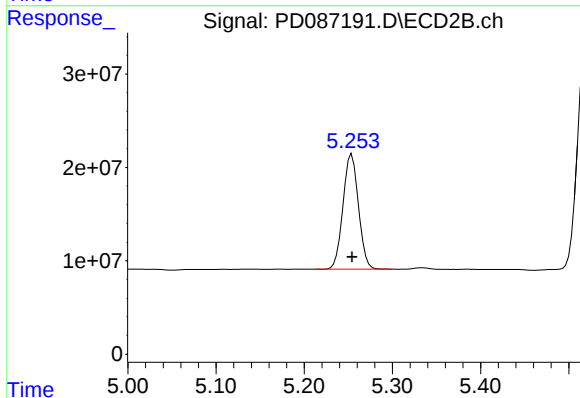


#9 Endosulfan I

R.T.: 5.254 min
Delta R.T.: 0.000 min
Response: 149976838
Conc: 10.80 ng/ml

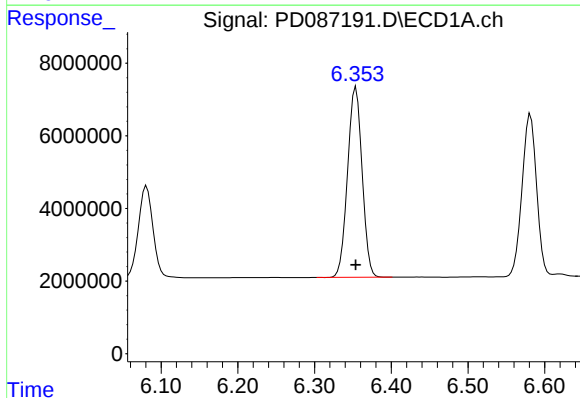


#13 Dieldrin

R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 69472057
Conc: 20.04 ng/ml

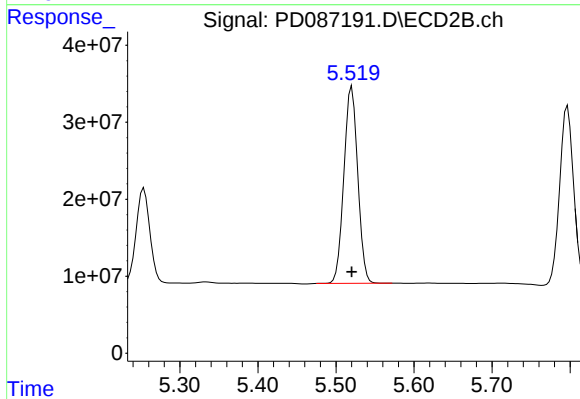

#13 Dieldrin


R.T.: 5.520 min
Delta R.T.: 0.000 min
Response: 315377577
Conc: 21.46 ng/ml

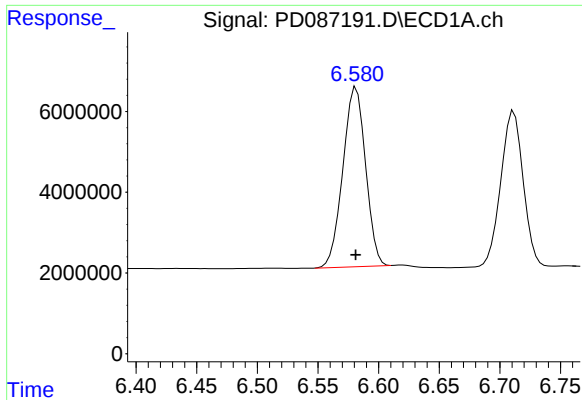

#14 Endrin


R.T.: 6.582 min
Delta R.T.: 0.000 min
Response: 58009502
Conc: 20.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA2043

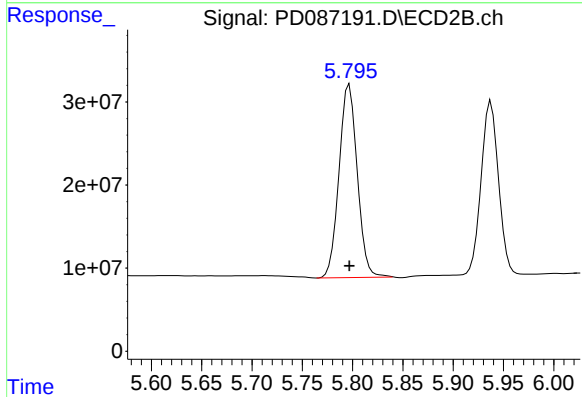


#14 Endrin

R.T.: 5.797 min
Delta R.T.: 0.000 min
Response: 292718773
Conc: 21.85 ng/ml

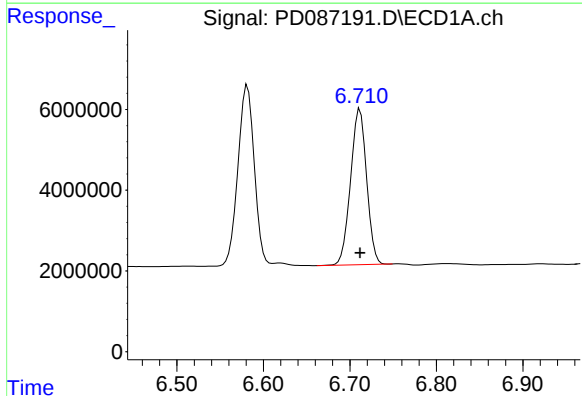


#16 4,4'-DDD

R.T.: 6.712 min
Delta R.T.: 0.000 min
Response: 49687008
Conc: 19.99 ng/ml

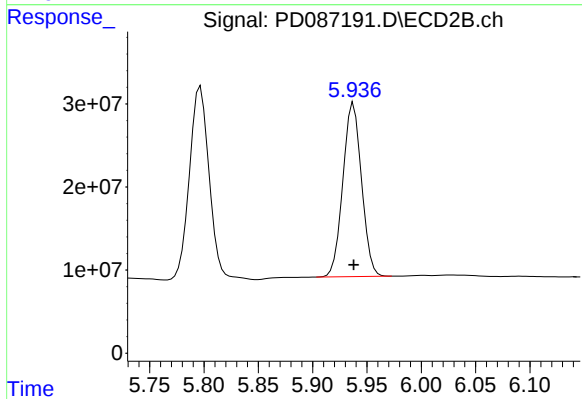

#16 4,4'-DDD


R.T.: 5.938 min
Delta R.T.: 0.000 min
Response: 250431468
Conc: 21.43 ng/ml

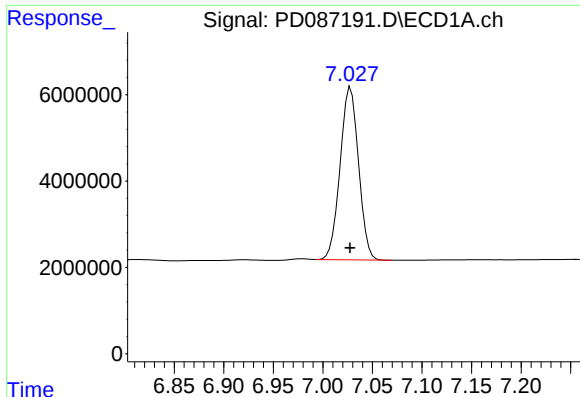

#17 4,4'-DDT


R.T.: 7.028 min
Delta R.T.: 0.000 min
Response: 51763557
Conc: 19.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA2043

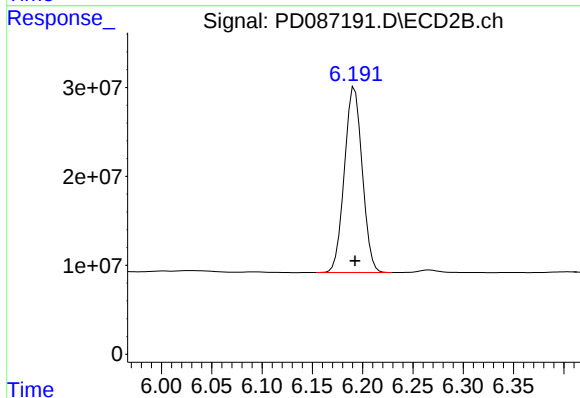


#17 4,4'-DDT

R.T.: 6.192 min
Delta R.T.: 0.000 min
Response: 256416327
Conc: 20.95 ng/ml

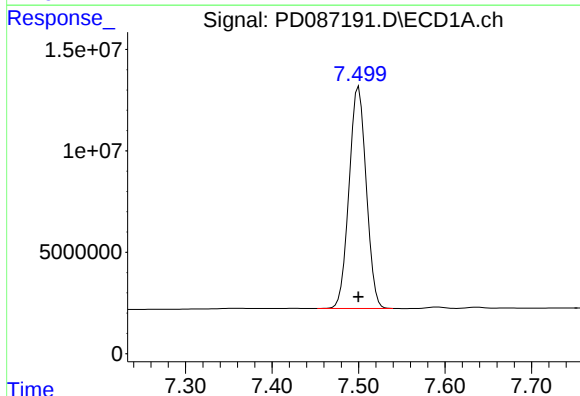


#20 Methoxychlor

R.T.: 7.500 min
Delta R.T.: 0.000 min
Response: 150303971
Conc: 103.55 ng/ml

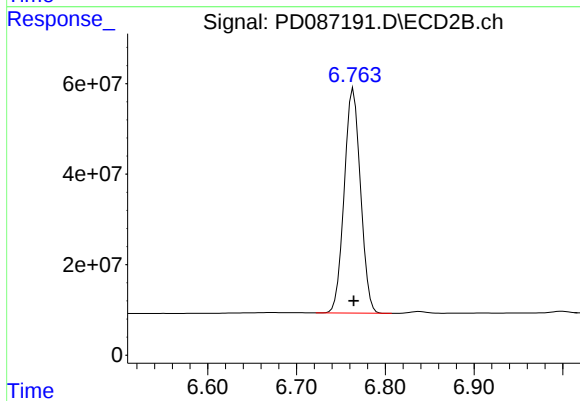

#20 Methoxychlor


R.T.: 6.764 min
Delta R.T.: 0.000 min
Response: 633061584
Conc: 111.27 ng/ml

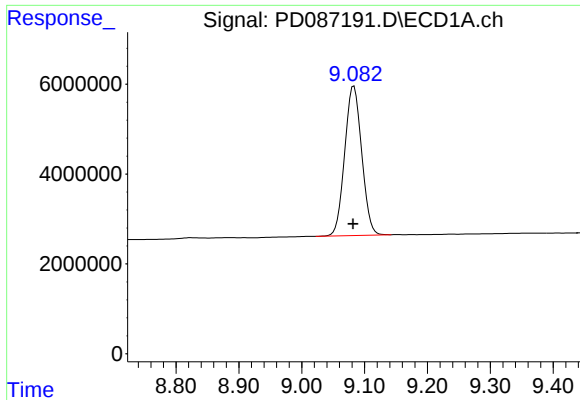

#27 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: 0.000 min
Response: 62488575
Conc: 21.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA2043

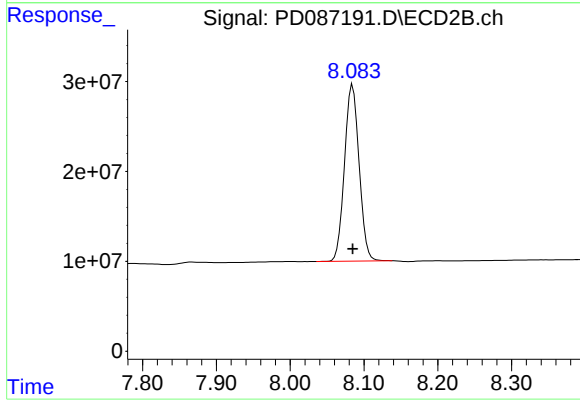

#27 Decachlorobiphenyl

R.T.: 8.085 min
Delta R.T.: 0.000 min
Response: 270319613
Conc: 21.84 ng/ml