

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121924\
 Data File : PD087195.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2024 15:20
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA4047

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 05:41:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121924CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 20 05:39:10 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.883	79886478	428.3E6	40.202	38.786
27)	SA Decachlor...	9.082	8.084	227.4E6	954.2E6	78.015	77.106
Target Compounds							
2)	A alpha-BHC	4.004	3.397	168.1E6	692.0E6	43.623	39.783
3)	MA gamma-BHC...	4.335	3.733	160.2E6	636.2E6	42.748	39.512
4)	MA Heptachlor	4.936	4.088	160.0E6	645.0E6	42.122	39.029
9)	A Endosulfan I	6.081	5.254	131.4E6	538.5E6	40.998	38.794
13)	MA Dieldrin	6.354	5.520	295.4E6	1146.9E6	85.221	78.038
14)	MA Endrin	6.581	5.797	245.2E6	1042.3E6	84.973	77.797
16)	A 4,4'-DDD	6.711	5.937	211.4E6	912.0E6	85.036	78.028
17)	MA 4,4'-DDT	7.027	6.192	220.9E6	967.4E6	85.304	79.053
20)	A Methoxychlor	7.499	6.764	588.7E6	2098.0E6	405.592	368.738


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121924\
Data File : PD087195.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2024 15:20
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 05:41:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121924CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 05:39:10 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

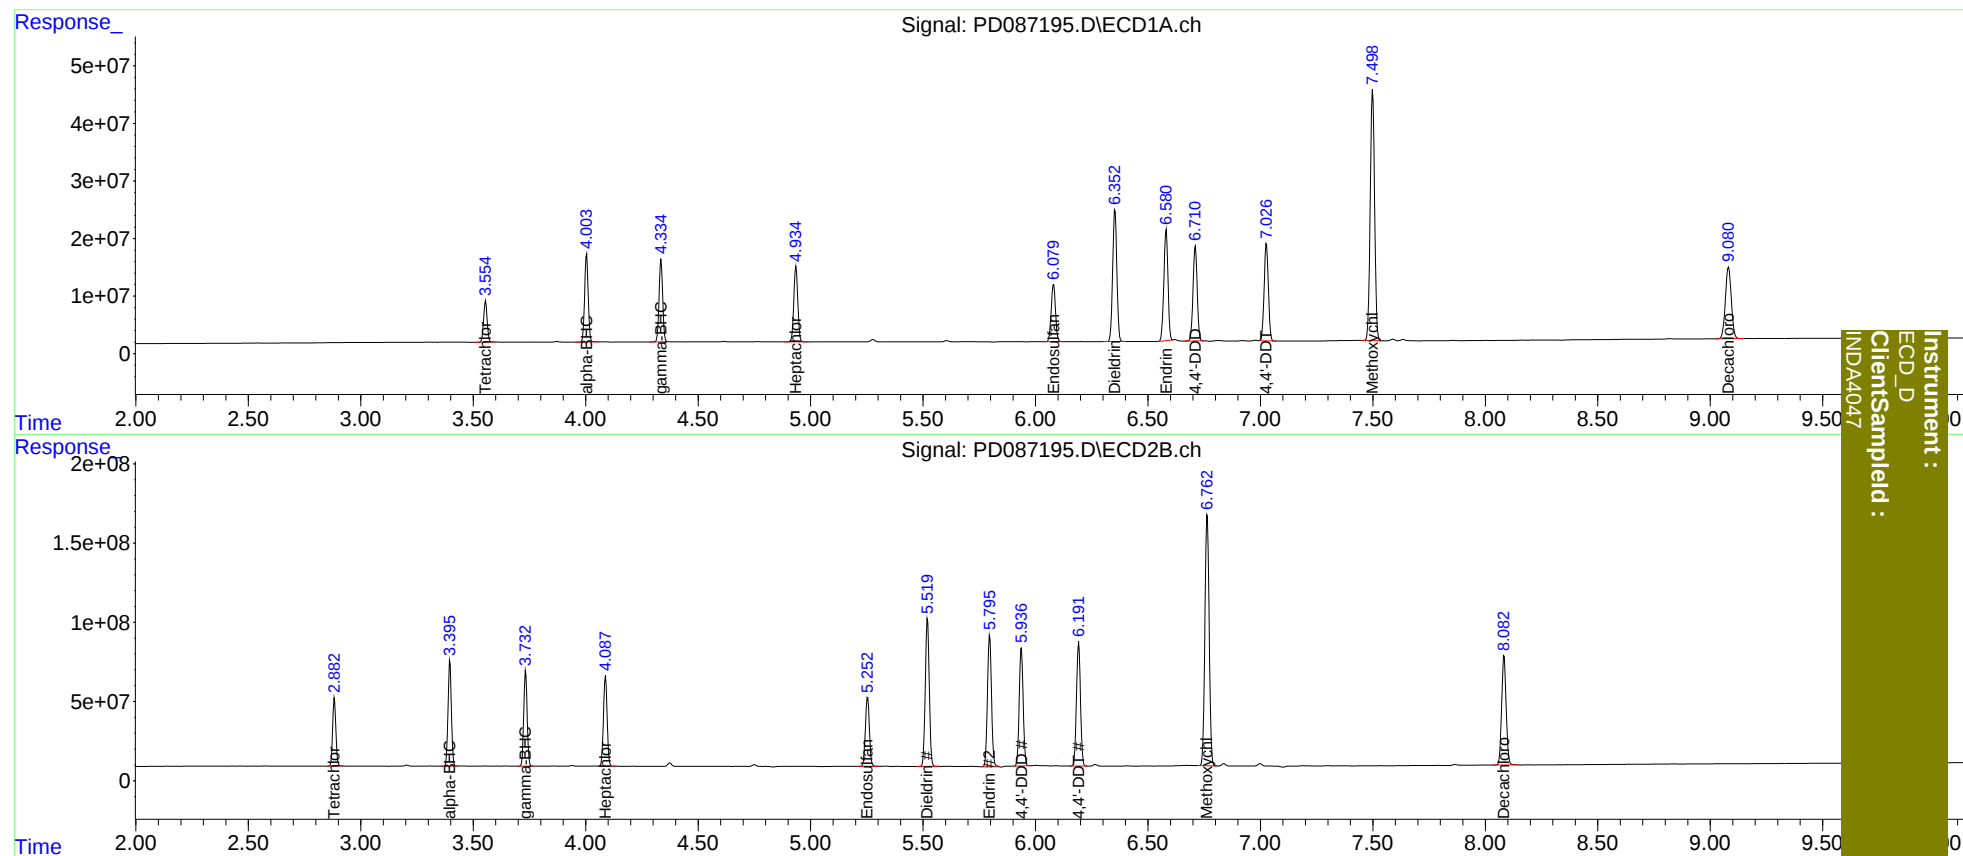


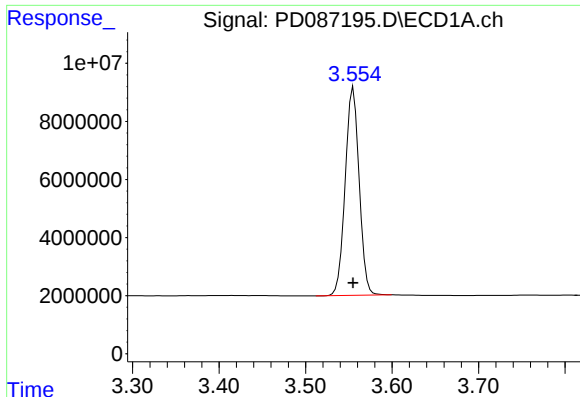

#1 Tetrachloro-m-xylene


R.T.: 3.555 min
Delta R.T.: 0.000 min
Response: 79886478
Conc: 40.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4047

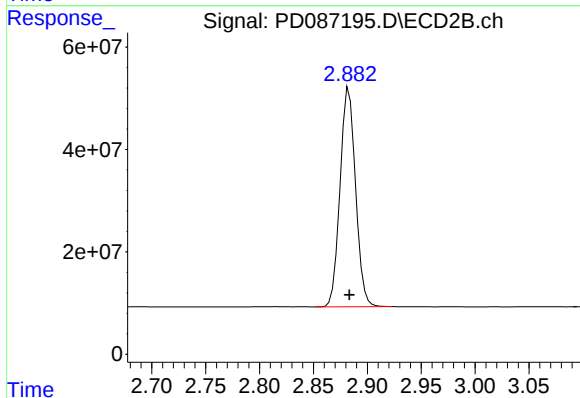


#1 Tetrachloro-m-xylene

R.T.: 2.883 min
Delta R.T.: 0.000 min
Response: 428303274
Conc: 38.79 ng/ml

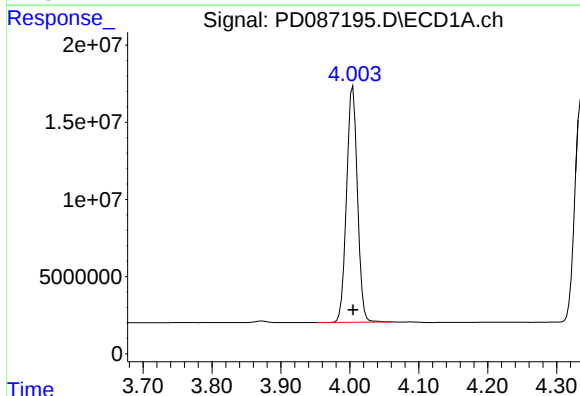


#2 alpha-BHC

R.T.: 4.004 min
Delta R.T.: 0.000 min
Response: 168133699
Conc: 43.62 ng/ml

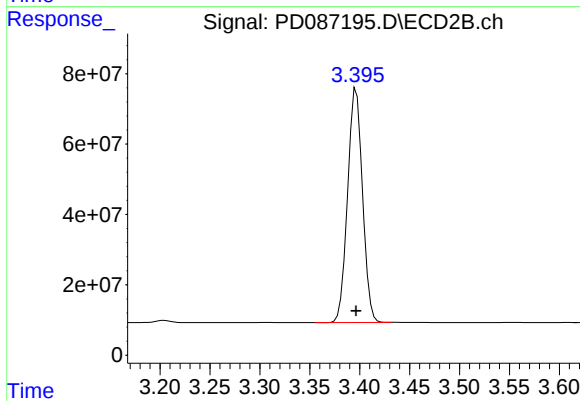

#2 alpha-BHC


R.T.: 3.397 min
Delta R.T.: 0.000 min
Response: 692023141
Conc: 39.78 ng/ml

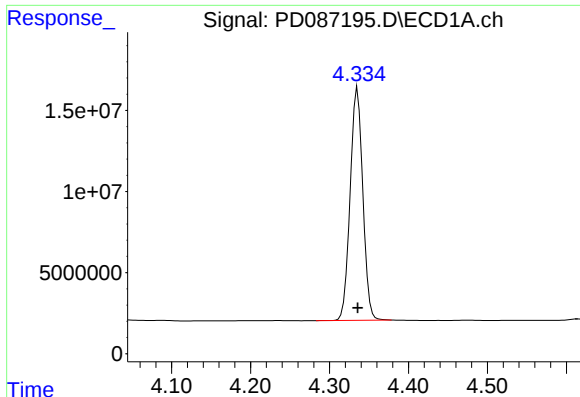

#3 gamma-BHC (Lindane)


R.T.: 4.335 min
Delta R.T.: 0.000 min
Response: 160165769
Conc: 42.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4047

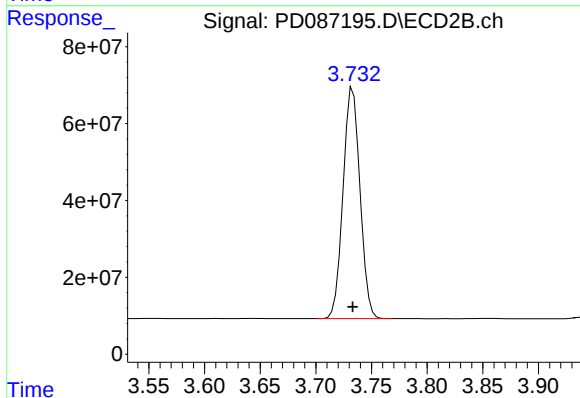


#3 gamma-BHC (Lindane)

R.T.: 3.733 min
Delta R.T.: 0.000 min
Response: 636160917
Conc: 39.51 ng/ml

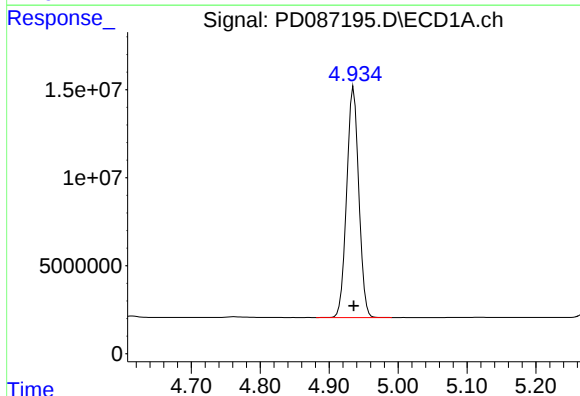


#4 Heptachlor

R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 160047759
Conc: 42.12 ng/ml

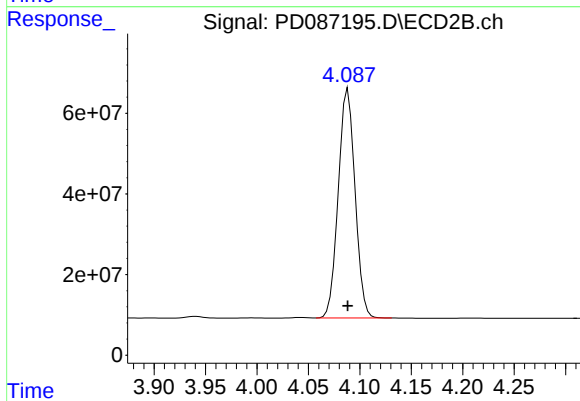

#4 Heptachlor


R.T.: 4.088 min
Delta R.T.: 0.000 min
Response: 645000021
Conc: 39.03 ng/ml

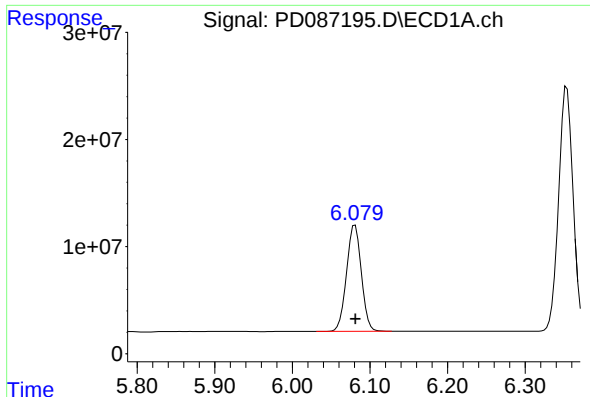

#9 Endosulfan I


R.T.: 6.081 min
Delta R.T.: 0.000 min
Response: 131437861
Conc: 41.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4047

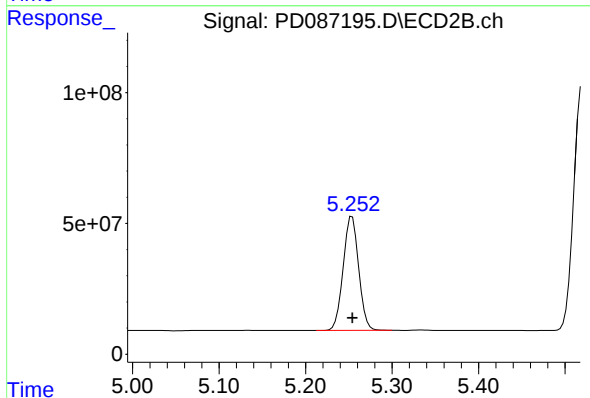


#9 Endosulfan I

R.T.: 5.254 min
Delta R.T.: 0.000 min
Response: 538509916
Conc: 38.79 ng/ml

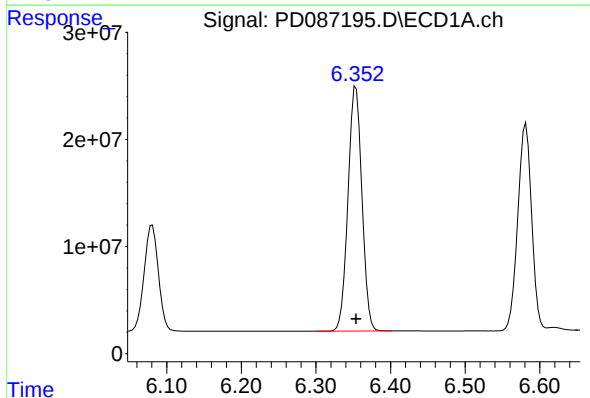


#13 Dieldrin

R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 295432021
Conc: 85.22 ng/ml

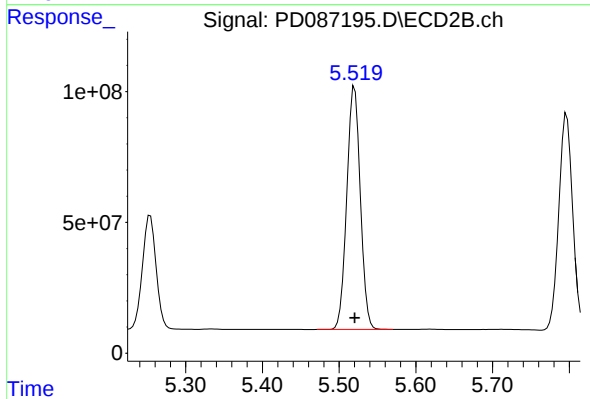

#13 Dieldrin


R.T.: 5.520 min
Delta R.T.: 0.000 min
Response: 1146857033
Conc: 78.04 ng/ml

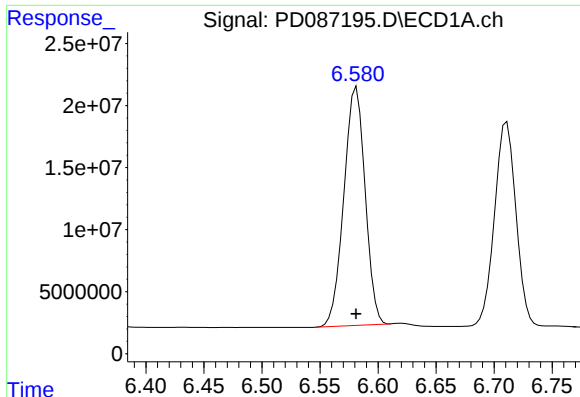

#14 Endrin


R.T.: 6.581 min
Delta R.T.: 0.000 min
Response: 245183532
Conc: 84.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4047

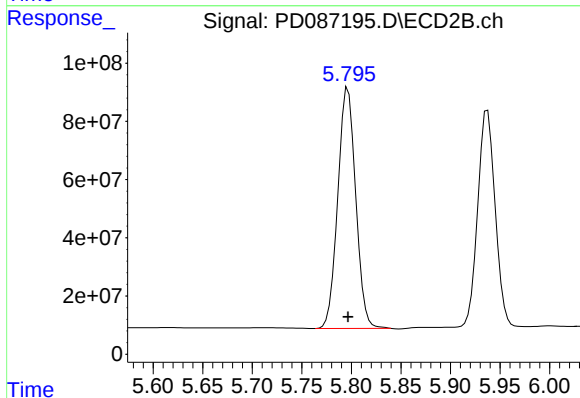


#14 Endrin

R.T.: 5.797 min
Delta R.T.: 0.000 min
Response: 1042292354
Conc: 77.80 ng/ml

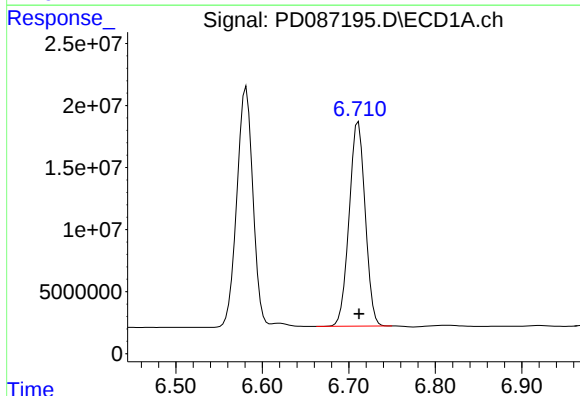


#16 4,4'-DDD

R.T.: 6.711 min
Delta R.T.: 0.000 min
Response: 211388115
Conc: 85.04 ng/ml

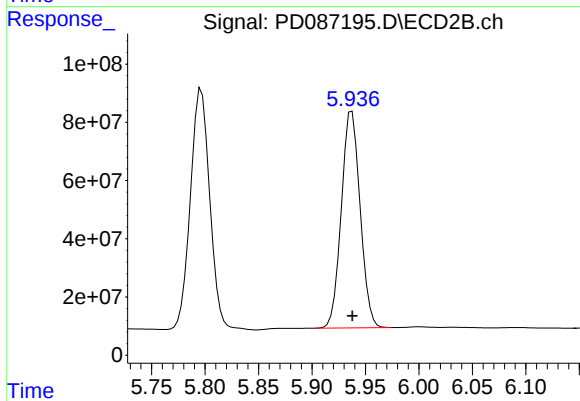

#16 4,4'-DDD


R.T.: 5.937 min
Delta R.T.: 0.000 min
Response: 911987044
Conc: 78.03 ng/ml

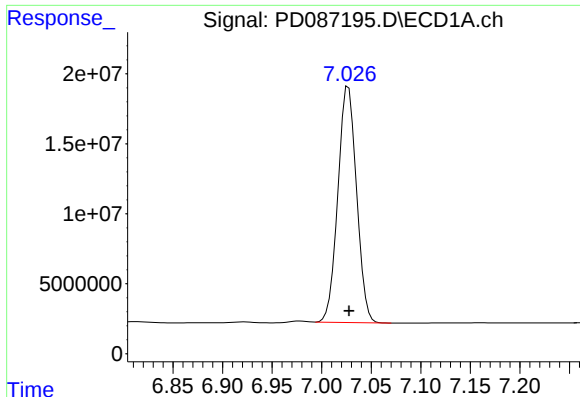

#17 4,4'-DDT


R.T.: 7.027 min
Delta R.T.: 0.000 min
Response: 220863930
Conc: 85.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4047

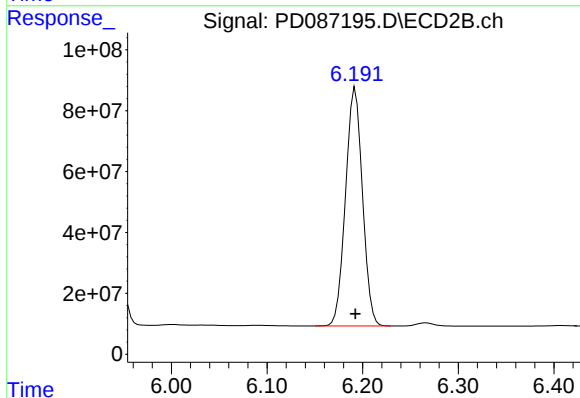


#17 4,4'-DDT

R.T.: 6.192 min
Delta R.T.: 0.000 min
Response: 967403188
Conc: 79.05 ng/ml

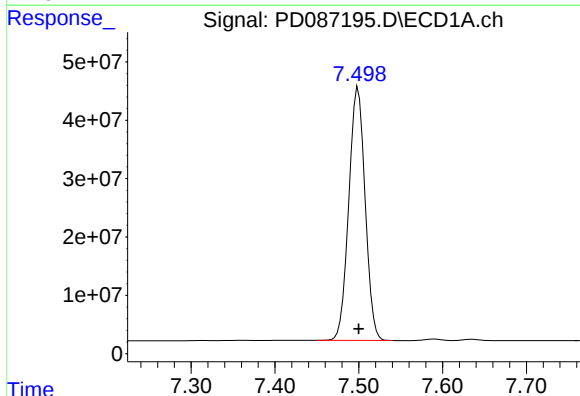


#20 Methoxychlor

R.T.: 7.499 min
Delta R.T.: 0.000 min
Response: 588732222
Conc: 405.59 ng/ml

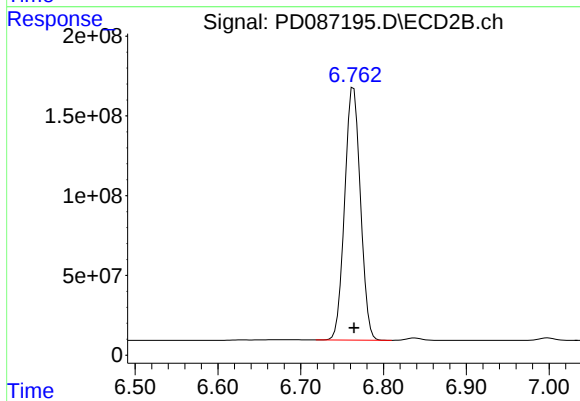

#20 Methoxychlor


R.T.: 6.764 min
Delta R.T.: 0.000 min
Response: 2097975323
Conc: 368.74 ng/ml

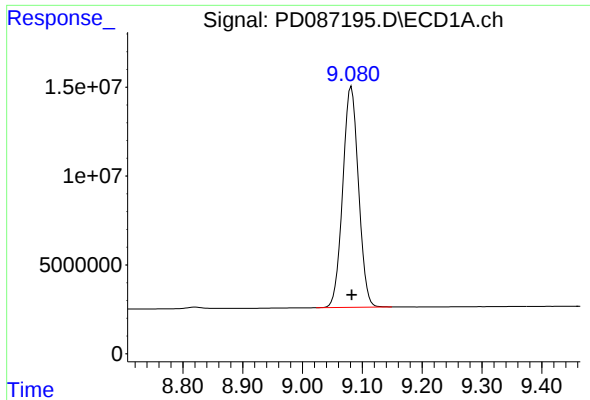

#27 Decachlorobiphenyl

R.T.: 9.082 min
Delta R.T.: 0.000 min
Response: 227386888
Conc: 78.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4047

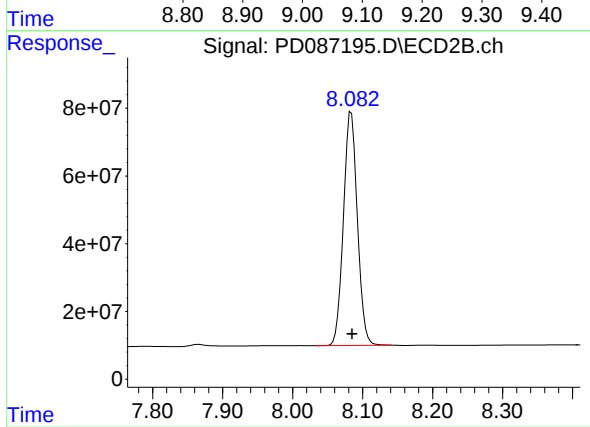

#27 Decachlorobiphenyl

R.T.: 8.084 min
Delta R.T.: -0.001 min
Response: 954170027
Conc: 77.11 ng/ml