

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121924\
 Data File : PD087199.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2024 16:16
 Operator : AR\AJ
 Sample : INDA601
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA6051

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 05:41:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121924CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 20 05:39:10 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.883	328.6E6	1577.4E6	165.358	142.845
27)	SA Decachlor...	9.082	8.084	870.4E6	3558.0E6	298.627	287.525
Target Compounds							
2)	A alpha-BHC	4.004	3.397	774.0E6	2638.8E6	200.819	151.700
3)	MA gamma-BHC...	4.336	3.733	719.1E6	2405.4E6	191.935	149.401
4)	MA Heptachlor	4.936	4.089	700.6E6	2334.0E6	184.386	141.228
9)	A Endosulfan I	6.081	5.254	550.6E6	1921.9E6	171.759	138.450
13)	MA Dieldrin	6.354	5.520	1277.0E6	4116.9E6	368.352	280.131
14)	MA Endrin	6.580	5.797	1064.7E6	3648.4E6	368.996	272.314 #
16)	A 4,4'-DDD	6.711	5.938	926.1E6	3289.0E6	372.535	281.404
17)	MA 4,4'-DDT	7.027	6.192	972.1E6	3542.4E6	375.463	289.472
20)	A Methoxychlor	7.499	6.764	2330.8E6	6392.2E6	1605.716	1123.487 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121924\
Data File : PD087199.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2024 16:16
Operator : AR\AJ
Sample : INDA601
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 05:41:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121924CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 05:39:10 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

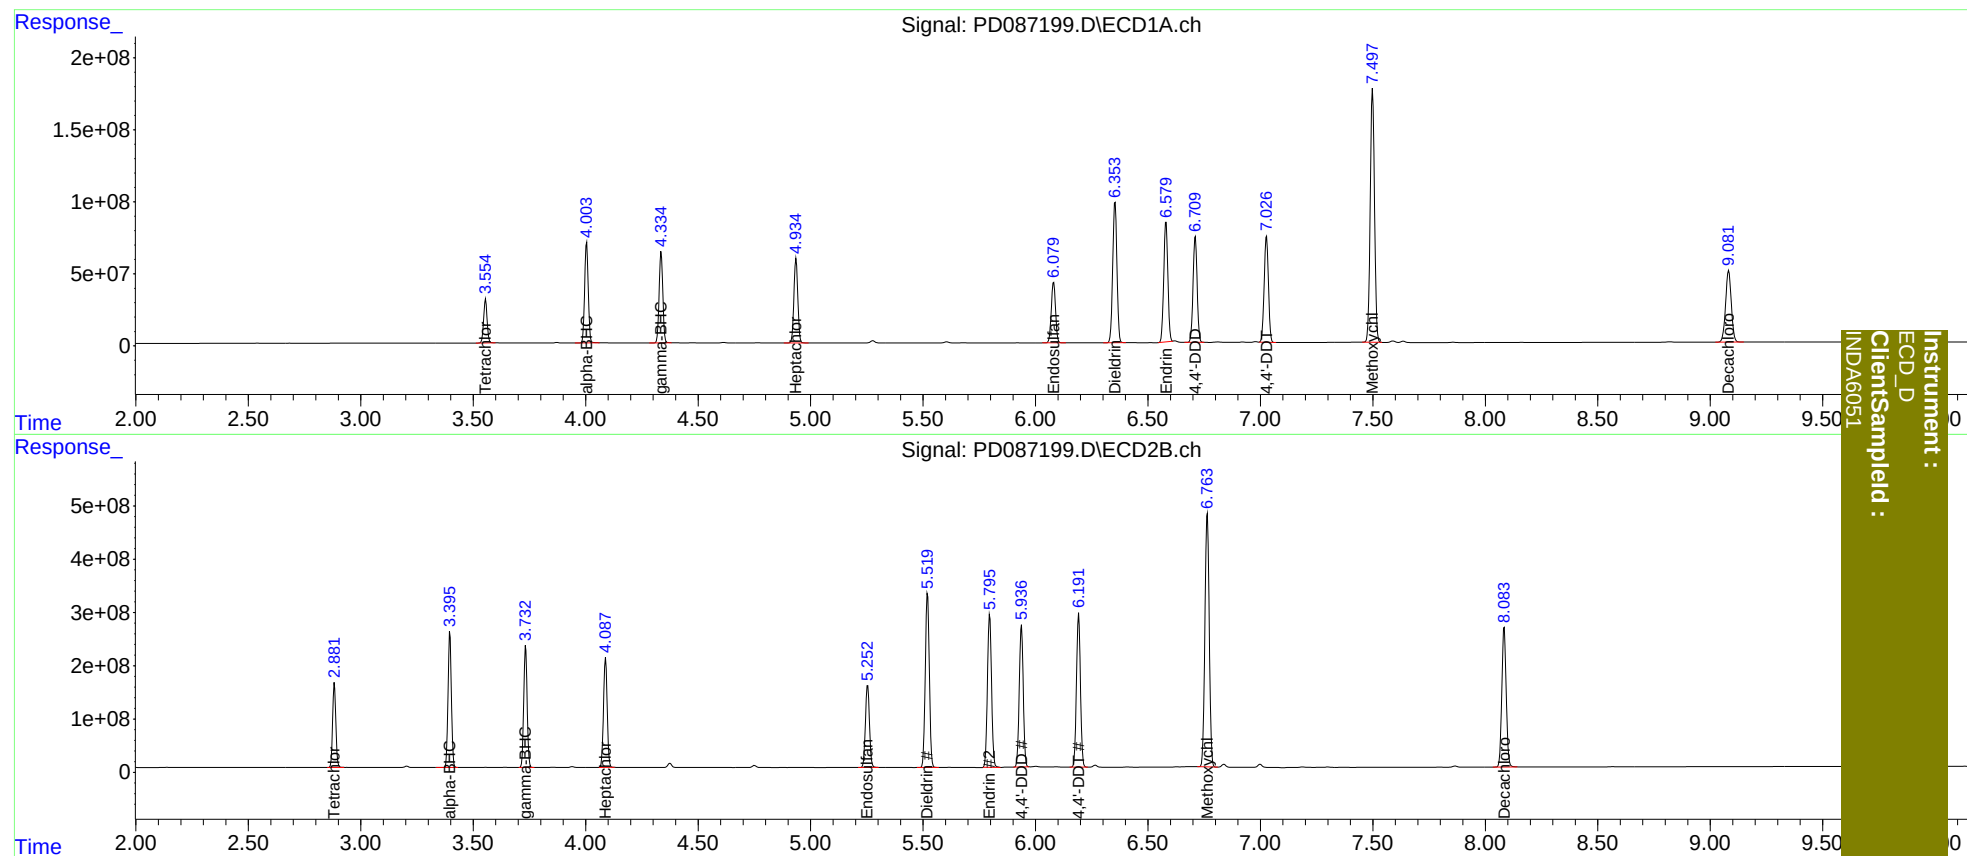


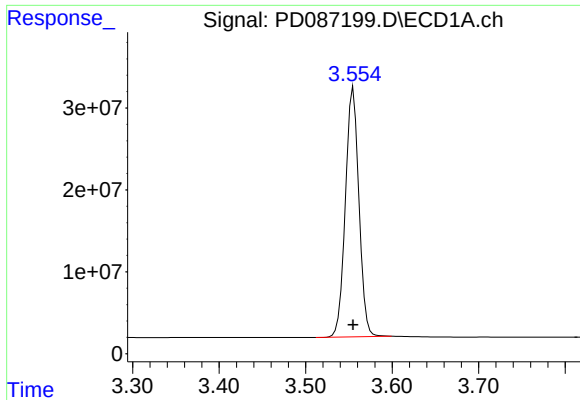

#1 Tetrachloro-m-xylene


R.T.: 3.555 min
Delta R.T.: 0.000 min
Response: 328584791
Conc: 165.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA6051

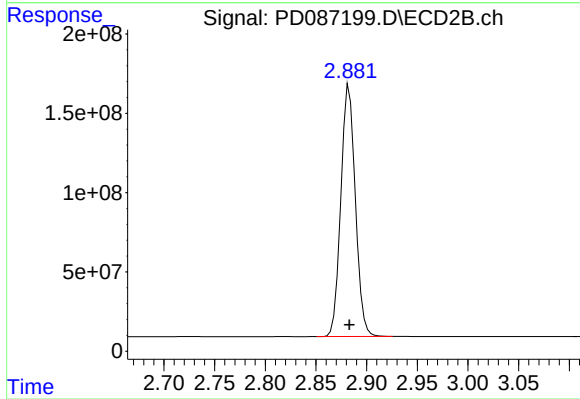


#1 Tetrachloro-m-xylene

R.T.: 2.883 min
Delta R.T.: 0.000 min
Response: 1577379127
Conc: 142.84 ng/ml

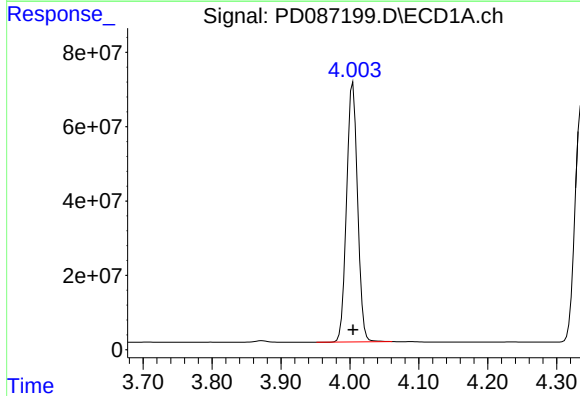


#2 alpha-BHC

R.T.: 4.004 min
Delta R.T.: 0.000 min
Response: 774000234
Conc: 200.82 ng/ml

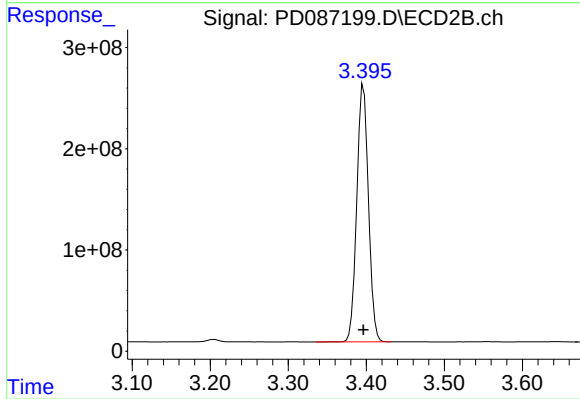

#2 alpha-BHC


R.T.: 3.397 min
Delta R.T.: 0.000 min
Response: 2638832506
Conc: 151.70 ng/ml

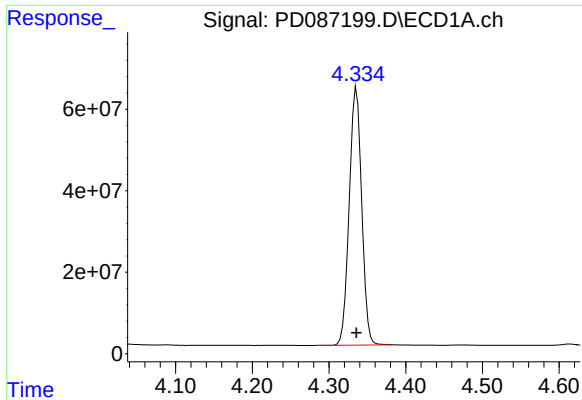

#3 gamma-BHC (Lindane)


R.T.: 4.336 min
Delta R.T.: 0.000 min
Response: 719131516
Conc: 191.94 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA6051

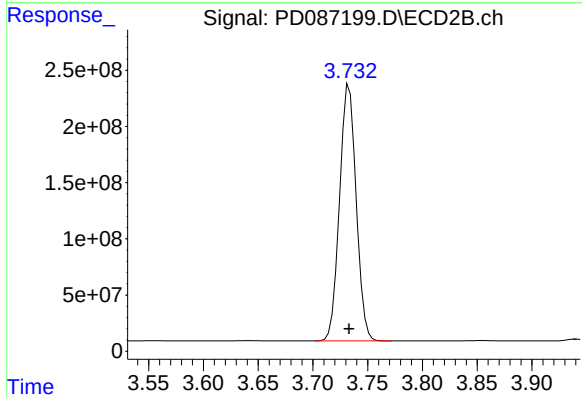


#3 gamma-BHC (Lindane)

R.T.: 3.733 min
Delta R.T.: 0.000 min
Response: 2405401491
Conc: 149.40 ng/ml

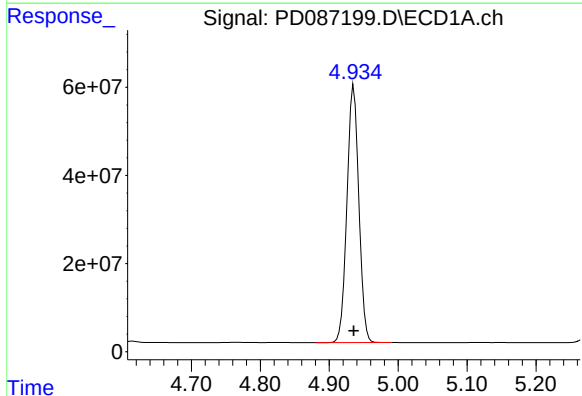


#4 Heptachlor

R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 700590768
Conc: 184.39 ng/ml

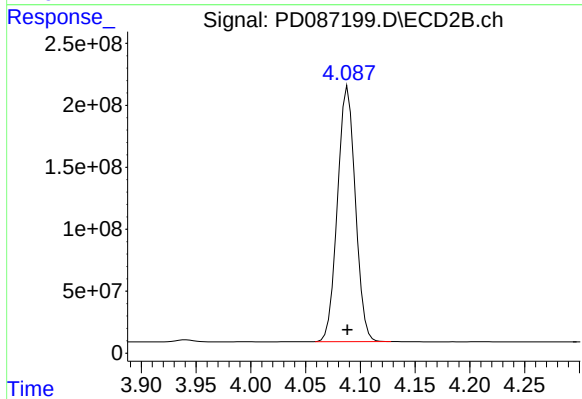

#4 Heptachlor


R.T.: 4.089 min
Delta R.T.: 0.000 min
Response: 2333972778
Conc: 141.23 ng/ml

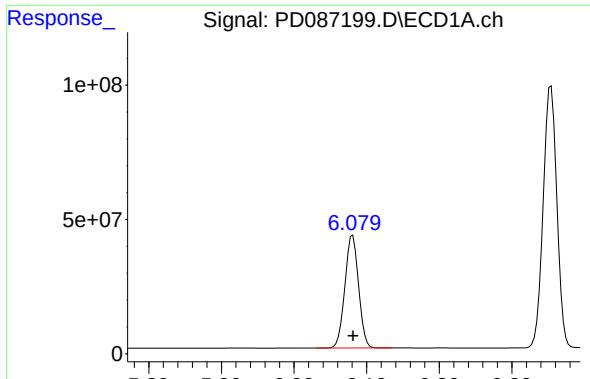

#9 Endosulfan I


R.T.: 6.081 min
Delta R.T.: 0.000 min
Response: 550649223
Conc: 171.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA6051

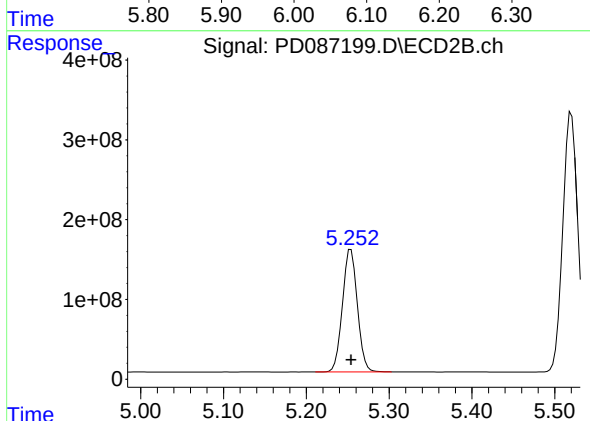


#9 Endosulfan I

R.T.: 5.254 min
Delta R.T.: 0.000 min
Response: 1921881365
Conc: 138.45 ng/ml

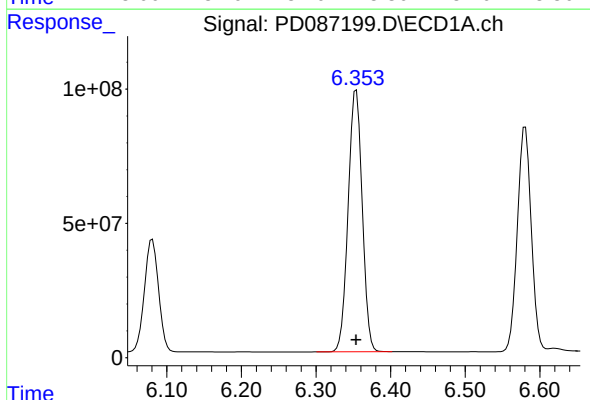


#13 Dieldrin

R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 1276955113
Conc: 368.35 ng/ml

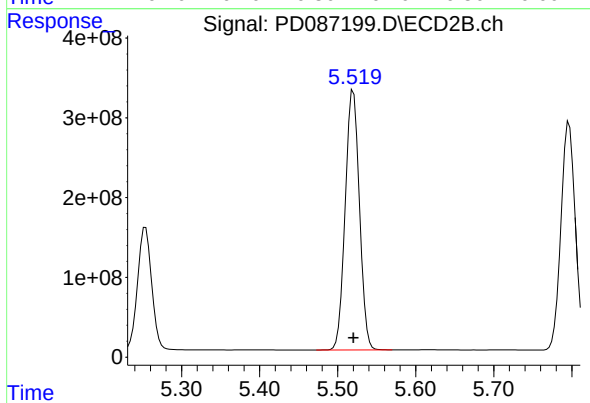

#13 Dieldrin


R.T.: 5.520 min
Delta R.T.: 0.000 min
Response: 4116850172
Conc: 280.13 ng/ml

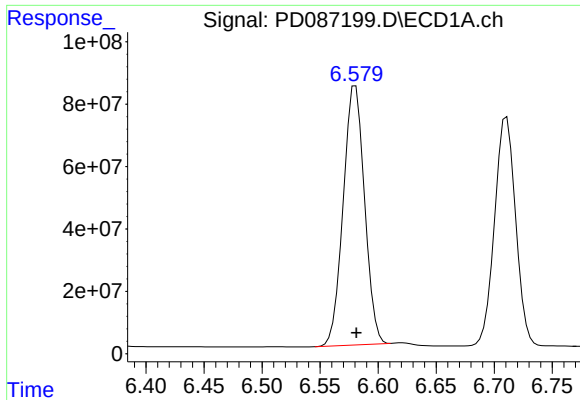

#14 Endrin


R.T.: 6.580 min
Delta R.T.: 0.000 min
Response: 1064711199
Conc: 369.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA6051

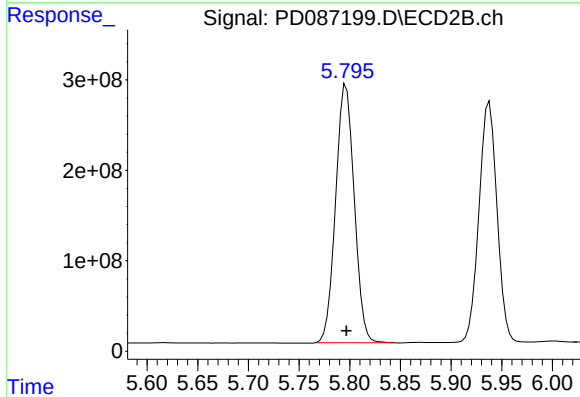


#14 Endrin

R.T.: 5.797 min
Delta R.T.: 0.000 min
Response: 3648354781
Conc: 272.31 ng/ml

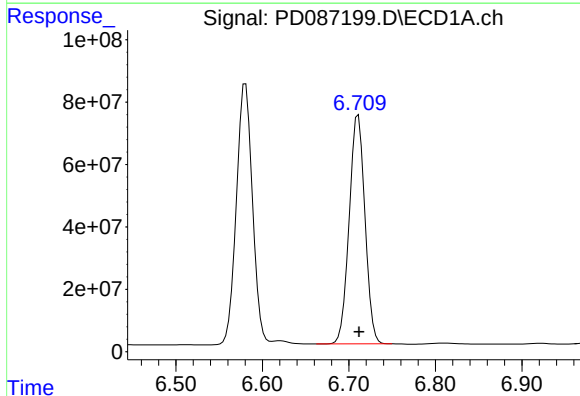


#16 4,4'-DDD

R.T.: 6.711 min
Delta R.T.: 0.000 min
Response: 926072453
Conc: 372.53 ng/ml

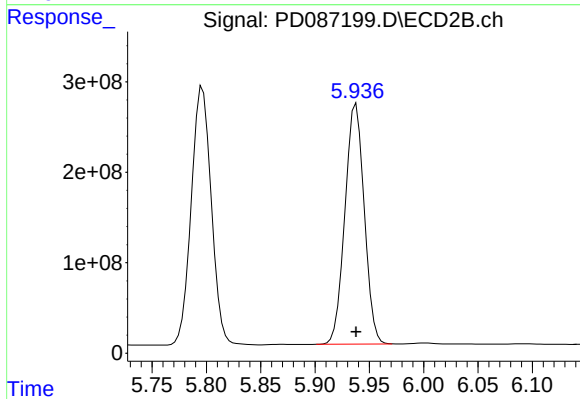

#16 4,4'-DDD


R.T.: 5.938 min
Delta R.T.: 0.000 min
Response: 3289048662
Conc: 281.40 ng/ml

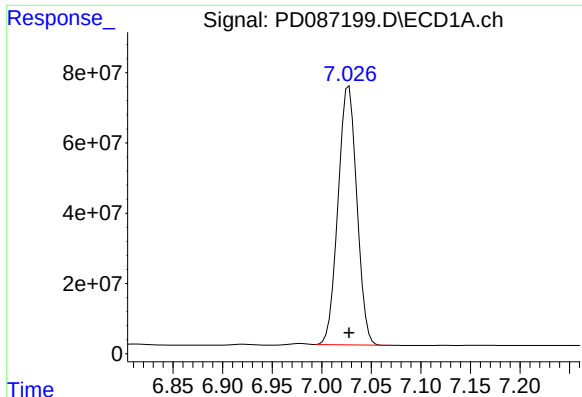

#17 4,4'-DDT


R.T.: 7.027 min
Delta R.T.: 0.000 min
Response: 972128438
Conc: 375.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA6051

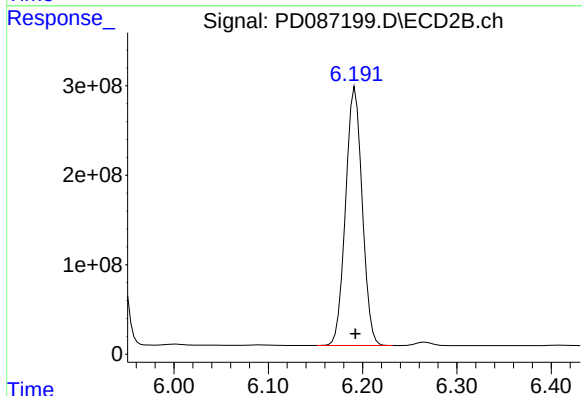


#17 4,4'-DDT

R.T.: 6.192 min
Delta R.T.: 0.000 min
Response: 3542373946
Conc: 289.47 ng/ml

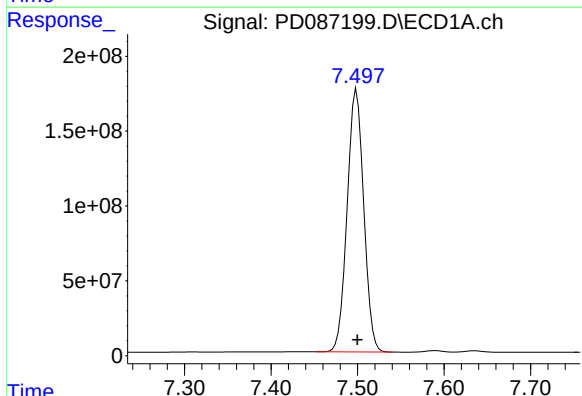


#20 Methoxychlor

R.T.: 7.499 min
Delta R.T.: -0.001 min
Response: 2330760564
Conc: 1605.72 ng/ml

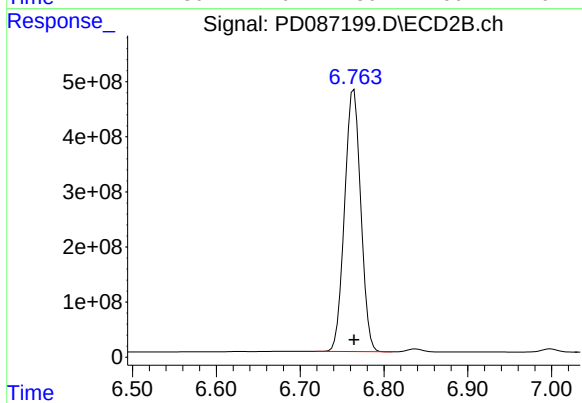

#20 Methoxychlor


R.T.: 6.764 min
Delta R.T.: 0.000 min
Response: 6392199021
Conc: 1123.49 ng/ml

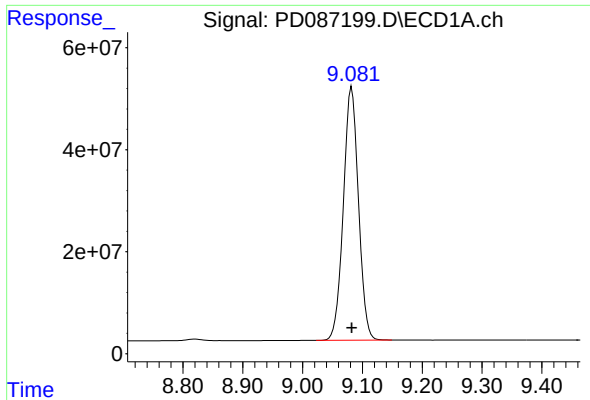

#27 Decachlorobiphenyl

R.T.: 9.082 min
Delta R.T.: 0.000 min
Response: 870395164
Conc: 298.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA6051

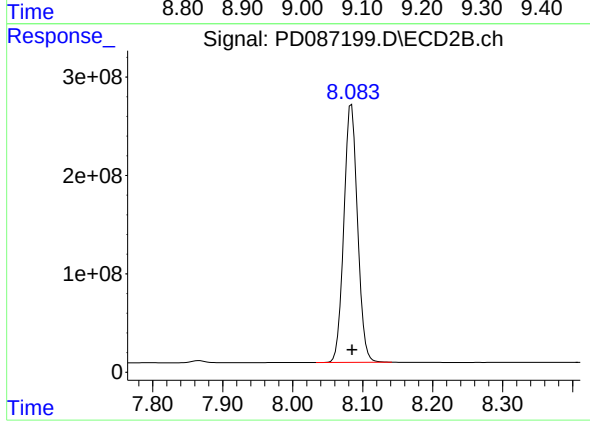

#27 Decachlorobiphenyl

R.T.: 8.084 min
Delta R.T.: 0.000 min
Response: 3558048912
Conc: 287.53 ng/ml