

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121924\
 Data File : PD087181.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2024 11:57
 Operator : AR\AJ
 Sample : RESC054
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC010

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 06:14:10 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121924CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 20 05:48:59 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.560	2.884	40679688	226.6E6	20.048	20.615
27)	SA Decachlor...	9.087	8.085	115.5E6	481.3E6	38.986	38.947
Target Compounds							
2)	A alpha-BHC	4.010	3.397	37616786	181.3E6	9.132	10.419
3)	MA gamma-BHC...	4.341	3.734	37306332	168.7E6	9.384	10.453
4)	MA Heptachlor	4.941	4.089	38008201	174.6E6	9.530	10.655
5)	MB Aldrin	5.283	4.376	37097323	169.0E6	9.496	10.563
6)	B beta-BHC	4.525	4.030	17070754	78360855	9.947	10.510
7)	B delta-BHC	4.773	4.267	35840788	168.0E6	8.856	10.082
8)	B Heptachlo...	5.703	4.880	33793659	153.3E6	9.476	10.301
9)	A Endosulfan I	6.086	5.255	32414962	146.9E6	9.788	10.716
10)	B trans-Chl...	5.957	5.134	32528893	160.9E6	9.253	10.340
11)	B cis-Chlor...	6.038	5.198	34144243	155.3E6	9.652	10.326
12)	B 4,4'-DDE	6.207	5.384	60483137	291.3E6	17.969	20.382
13)	MA Dieldrin	6.359	5.521	67926480	309.9E6	18.740	21.305
14)	MA Endrin	6.586	5.798	54668264	290.9E6	18.106	21.794
15)	B Endosulfa...	6.797	6.089	53385651	265.0E6	17.814	20.668
16)	A 4,4'-DDD	6.716	5.939	48905404	246.8E6	18.813	21.372
17)	MA 4,4'-DDT	7.032	6.194	49979711	251.1E6	18.427	20.812
18)	B Endrin al...	6.926	6.267	44958956	209.3E6	19.212	21.010
19)	B Endosulfa...	7.160	6.491	54685825	260.6E6	18.925	20.767
20)	A Methoxychlor	7.504	6.765	148.3E6	617.0E6	101.031	113.994
21)	B Endrin ke...	7.640	7.000	59698838	292.9E6	18.731	21.371

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121924\
Data File : PD087181.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2024 11:57
Operator : AR\AJ
Sample : RESC054
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 06:14:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121924CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 05:48:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

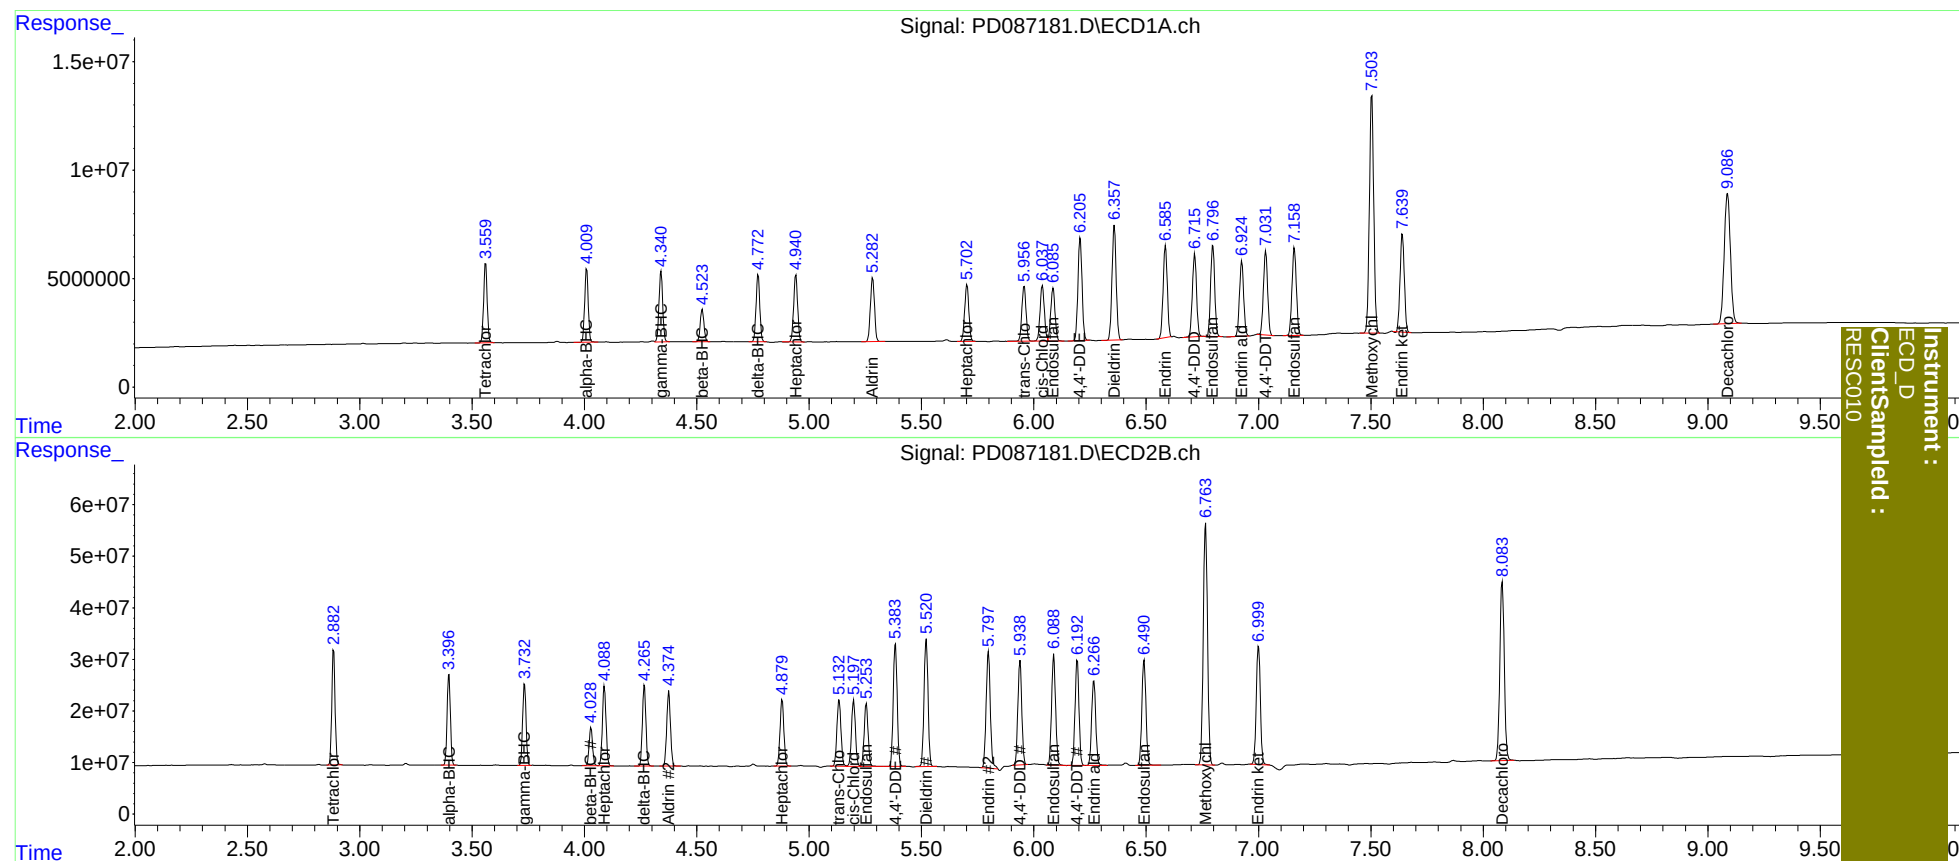

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121924\
Data File : PD087181.D
Acq On : 19 Dec 2024 11:57
Operator : AR\AJ
Sample : RESC054
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC010

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121924CLP-TCLP.M
Title : GC Extractables
Last Update : Fri Dec 20 05:48:59 2024
Integrator: ChemStation

RT#1	RT#2	Resolution
3.560	4.010	100.00%
4.010	4.341	100.00%
4.341	4.525	100.00%
4.525	4.773	100.00%
4.773	4.941	100.00%
4.941	5.283	100.00%
5.283	5.703	100.00%
5.703	5.957	100.00%
5.957	6.038	99.29%
6.038	6.086	95.58%
6.086	6.207	100.00%
6.207	6.359	100.00%
6.359	6.586	100.00%
6.586	6.716	100.00%
6.716	6.797	100.00%
6.797	6.926	100.00%
6.926	7.032	100.00%
7.032	7.160	100.00%
7.160	7.504	100.00%
7.504	7.640	100.00%
7.640	9.087	100.00%

Signal #2


2.884	3.397	100.00%
3.397	3.734	100.00%
3.734	4.030	100.00%
4.030	4.089	100.00%
4.089	4.267	100.00%
4.267	4.376	100.00%
4.376	4.880	100.00%
4.880	5.134	100.00%
5.134	5.198	100.00%
5.198	5.255	100.00%
5.255	5.384	100.00%
5.384	5.521	100.00%
5.521	5.798	100.00%
5.798	5.939	100.00%
5.939	6.089	100.00%
6.089	6.194	100.00%
6.194	6.267	100.00%
6.267	6.491	100.00%
6.491	6.765	100.00%
6.765	7.000	100.00%
7.000	8.085	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121924\
Data File : PD087181.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2024 11:57
Operator : AR\AJ
Sample : RESC054
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC010

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 06:14:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121924CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 05:48:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

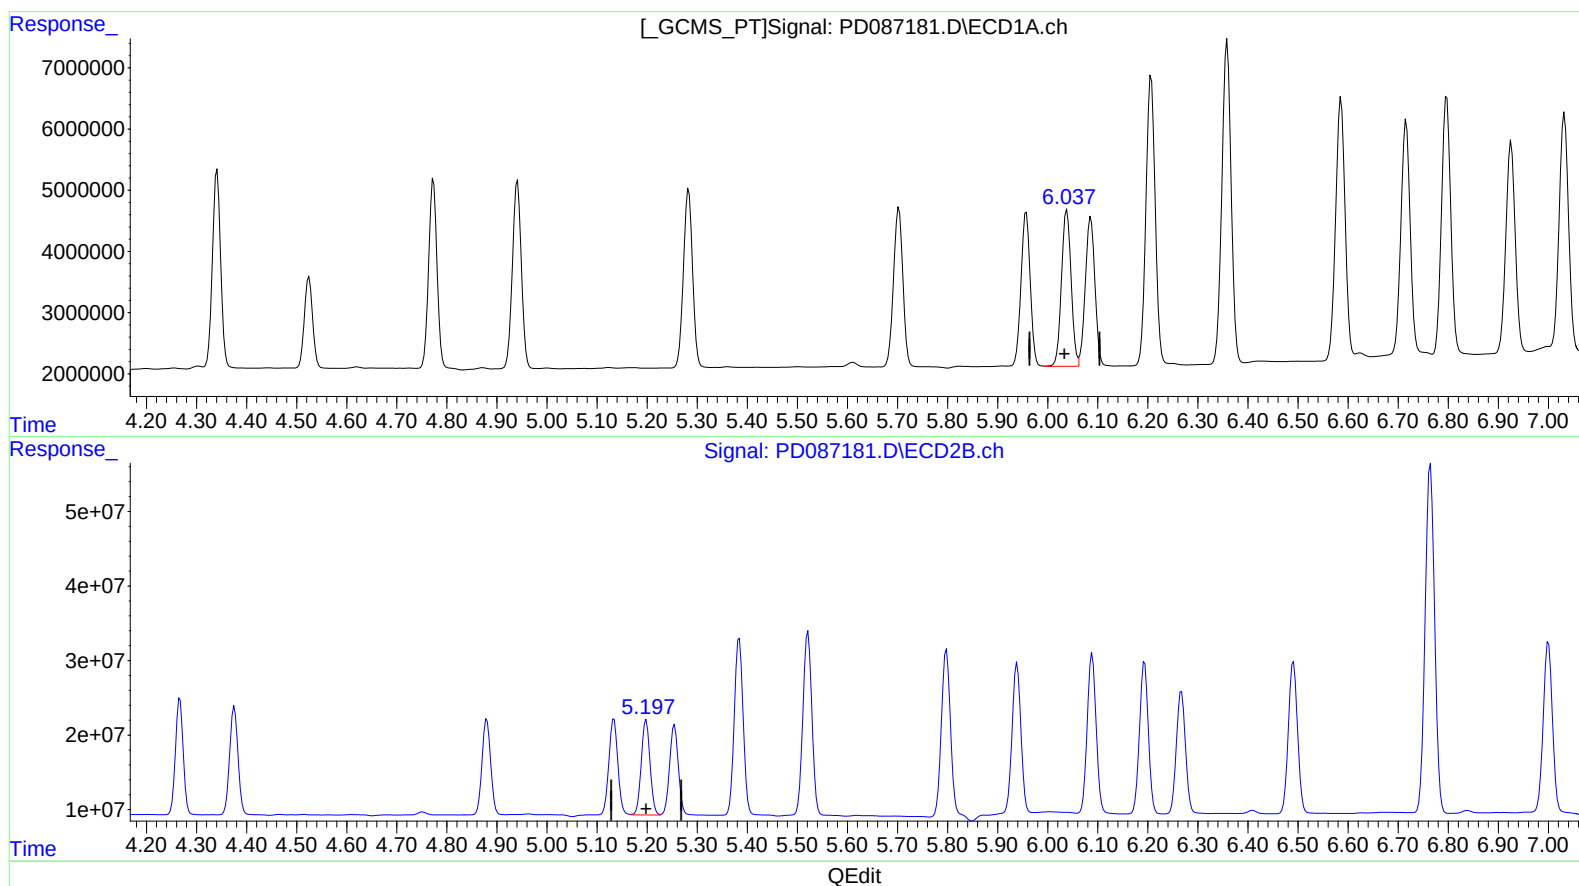

(11) cis-Chlordane (B)

6.038min 9.652 ng/ml

response 34144243

(11) cis-Chlordane #2 (B)

5.198min 10.326 ng/ml


response 155325669

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121924\
Data File : PD087181.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2024 11:57
Operator : AR\AJ
Sample : RESC054
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC010

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 06:14:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121924CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 05:48:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

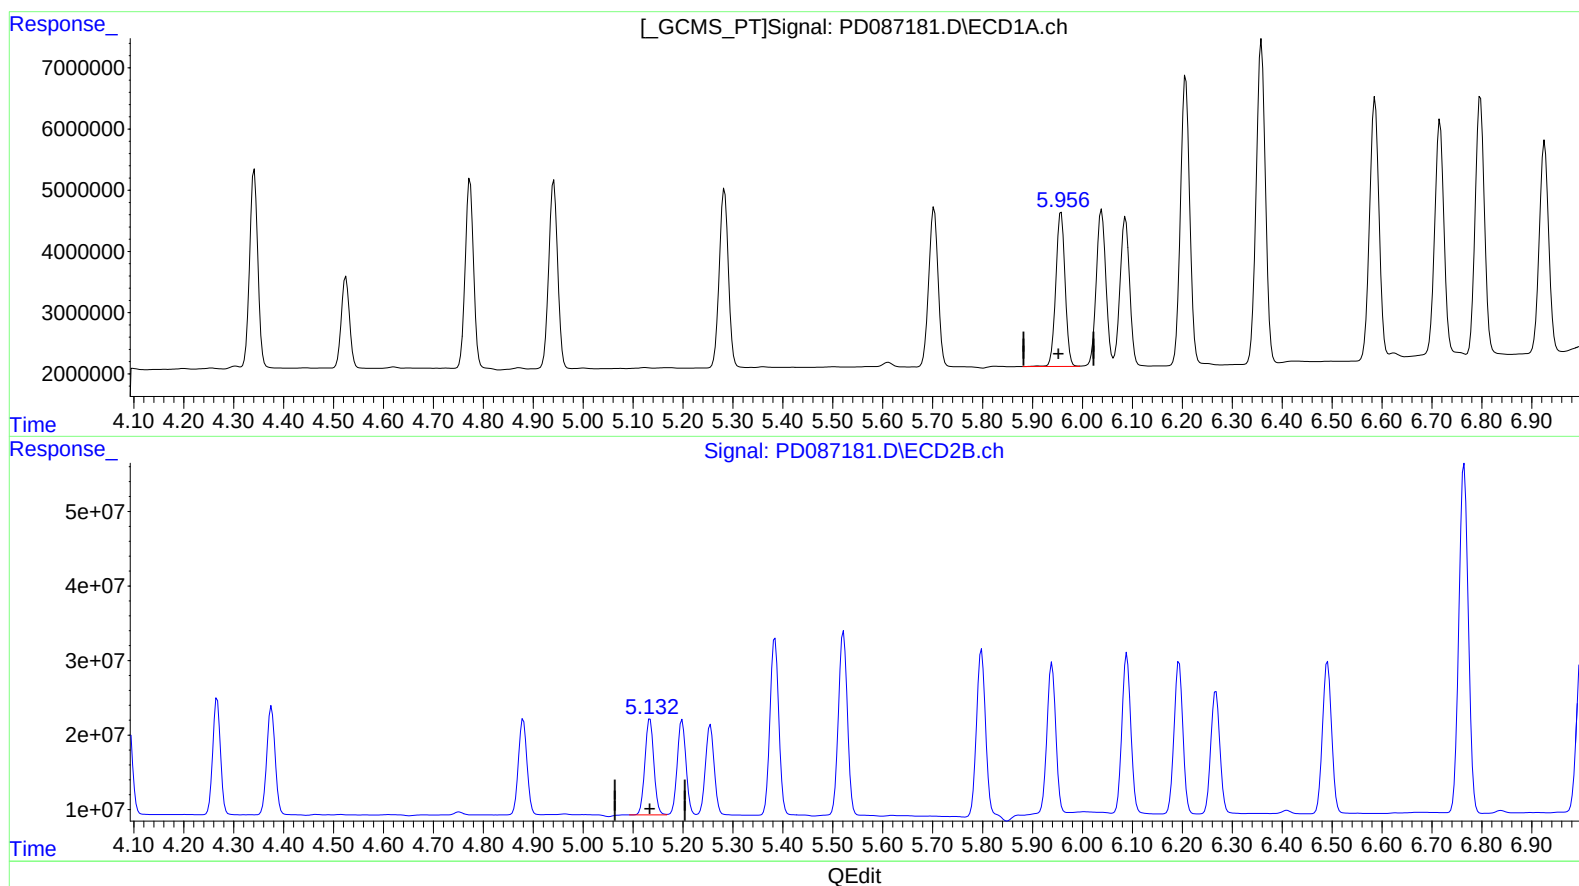

(10) trans-Chlordane (B)

5.957min 9.253 ng/ml

response 32528893

(10) trans-Chlordane #2 (B)

5.134min 10.340 ng/ml

response 160934299