

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121924\
 Data File : PD087193.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2024 14:52
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3045

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 05:41:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121924CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 20 05:39:10 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.883	39742234	220.9E6	20.000	20.000
2)	SA Decachlor...	9.082	8.085	116.6E6	495.0E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	4.005	3.396	77084276	347.9E6	20.000	20.000
3)	MA gamma-BHC...	4.336	3.733	74934722	322.0E6	20.000	20.000
4)	MA Heptachlor	4.936	4.088	75991792	330.5E6	20.000	20.000
9)	A Endosulfan I	6.081	5.254	64118654	277.6E6	20.000	20.000
13)	MA Dieldrin	6.354	5.520	138.7E6	587.8E6	40.000	40.000
14)	MA Endrin	6.581	5.797	115.4E6	535.9E6	40.000	40.000
16)	A 4,4'-DDD	6.712	5.938	99434709	467.5E6	40.000	40.000
17)	MA 4,4'-DDT	7.027	6.192	103.6E6	489.5E6	40.000	40.000
20)	A Methoxychlor	7.500	6.764	290.3E6	1137.9E6	200.000	200.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121924\
Data File : PD087193.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2024 14:52
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 05:41:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121924CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 05:39:10 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

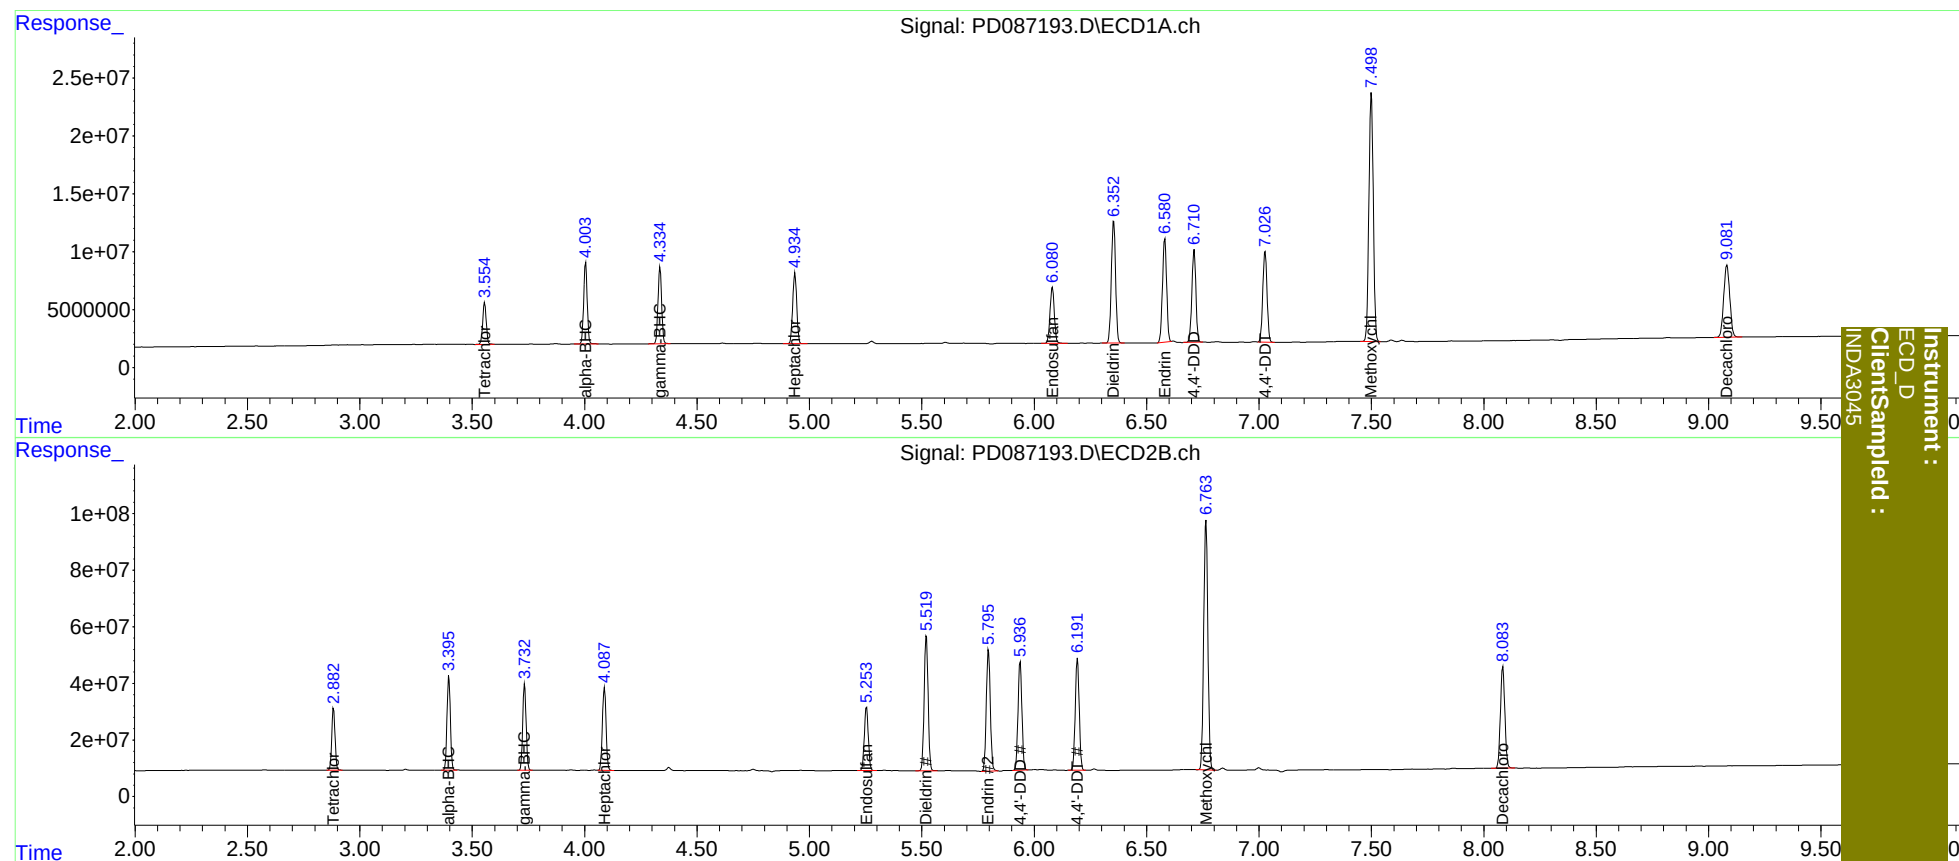

Instrument :
ECD_D
ClientSampled :
INDA3045