

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121924\
 Data File : PD087197.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2024 15:48
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA5049

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 05:41:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121924CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 20 05:39:10 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.883	157.3E6	804.8E6	79.148	72.883
27)	SA Decachlor...	9.082	8.084	431.4E6	1774.5E6	148.005	143.399
Target Compounds							
2)	A alpha-BHC	4.004	3.396	353.4E6	1320.5E6	91.682	75.911
3)	MA gamma-BHC...	4.336	3.733	331.6E6	1210.9E6	88.507	75.210
4)	MA Heptachlor	4.935	4.088	326.9E6	1204.3E6	86.023	72.873
9)	A Endosulfan I	6.081	5.254	262.2E6	995.4E6	81.778	71.709
13)	MA Dieldrin	6.354	5.520	601.4E6	2137.8E6	173.494	145.470
14)	MA Endrin	6.581	5.797	499.5E6	1918.4E6	173.102	143.188
16)	A 4,4'-DDD	6.711	5.938	431.1E6	1695.5E6	173.407	145.062
17)	MA 4,4'-DDT	7.027	6.192	450.9E6	1815.5E6	174.138	148.356
20)	A Methoxychlor	7.499	6.764	1142.3E6	3634.7E6	786.974	638.823

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121924\
Data File : PD087197.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2024 15:48
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 05:41:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121924CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 05:39:10 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

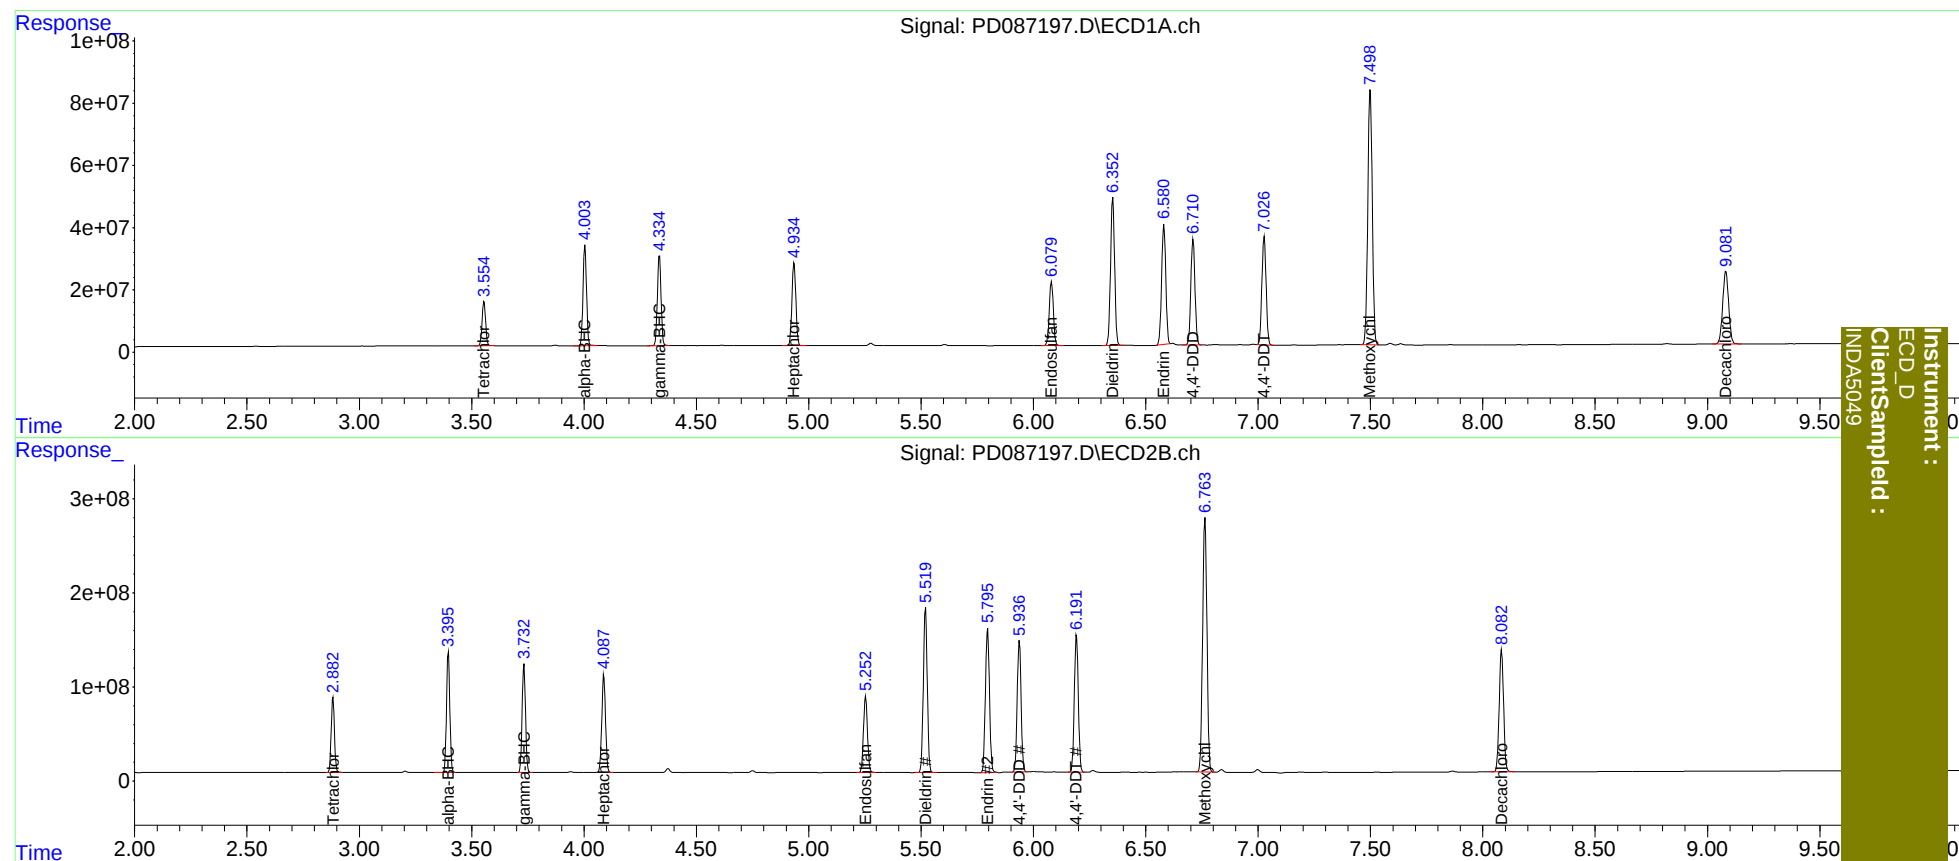

Instrument :
ECD_D
ClientSampled :
INDA5049