

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122019\
 Data File : PD056693.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2019 16:48
 Operator : SG\AJ
 Sample : K6257-20
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFEW8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 22:16:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.286	3.959	8599030	15711402	10.383	13.068 #
27)	SA Decachlor...	7.955	8.992	11796134	17115304	13.064	14.225
Target Compounds							
15)	B Endosulfa...	0.000	6.872	0	1031719	N.D.	0.704


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122019\
Data File : PD056693.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2019 16:48
Operator : SG\AJ
Sample : K6257-20
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BFEW8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 22:16:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

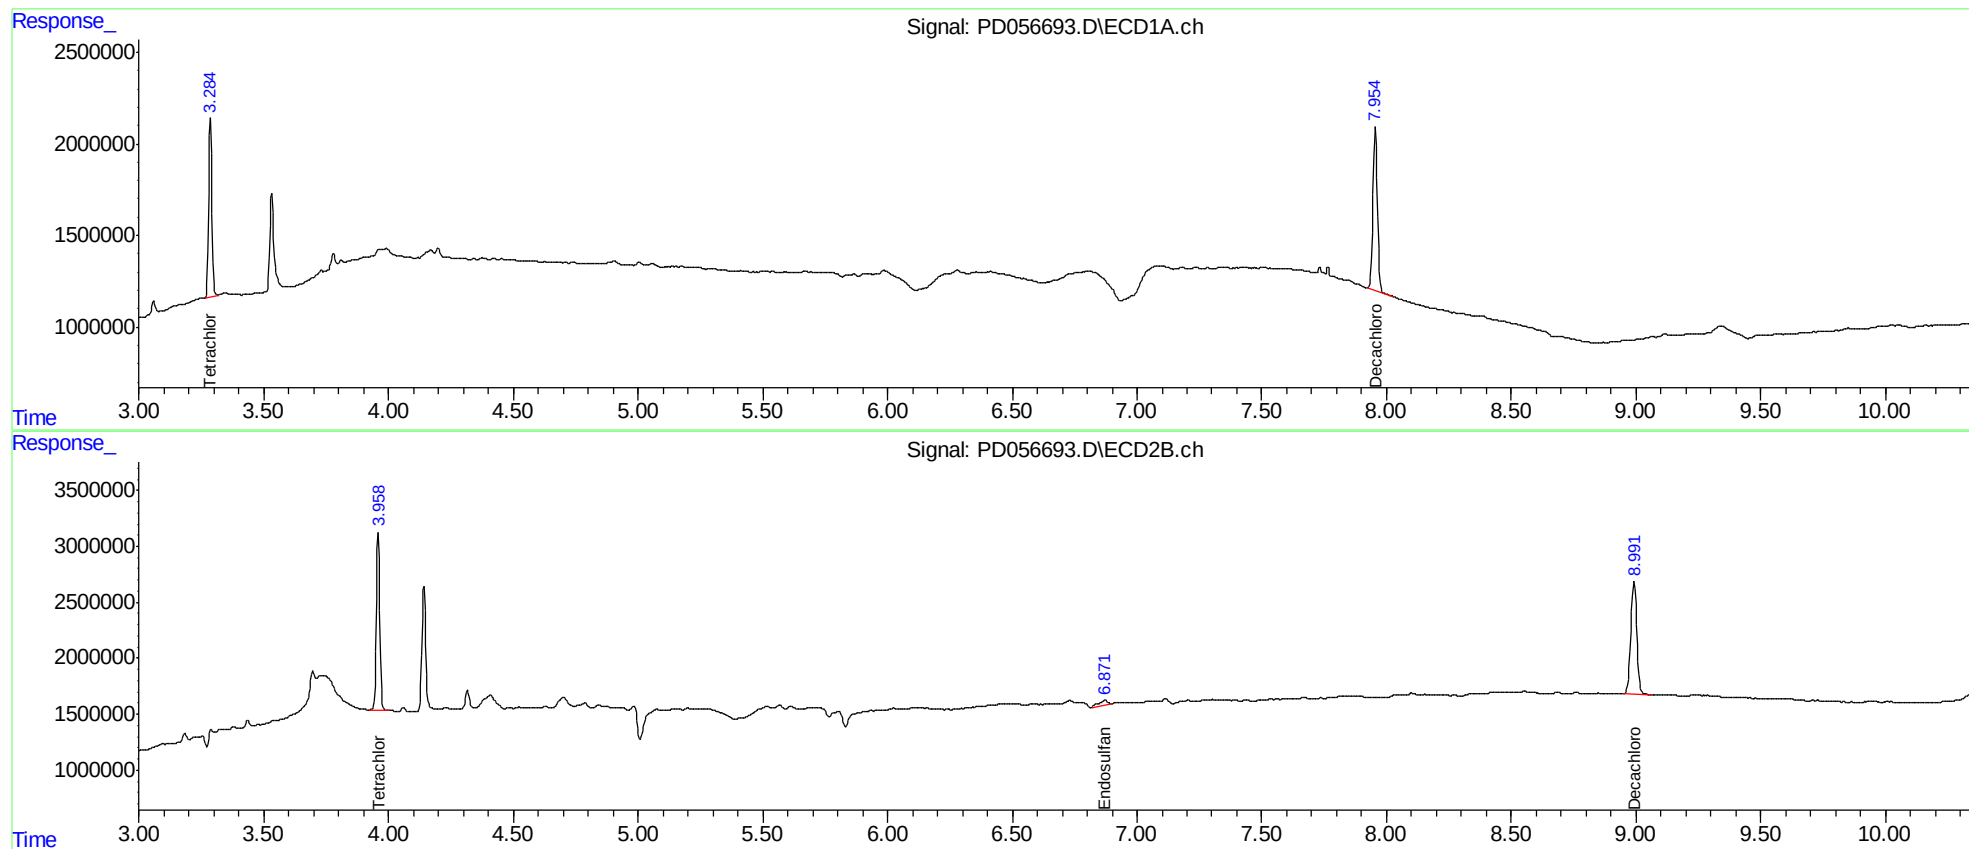


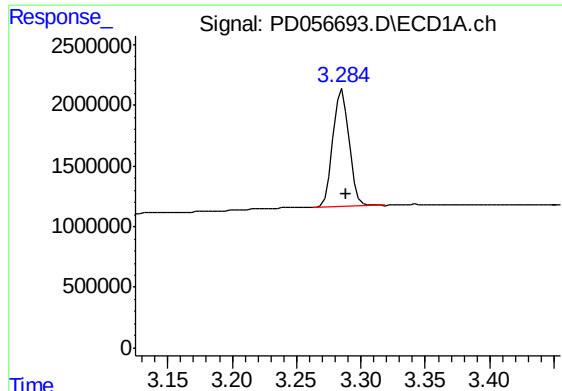

#1 Tetrachloro-m-xylene


R.T.: 3.286 min
Delta R.T.: -0.002 min
Response: 8599030
Conc: 10.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFEW8

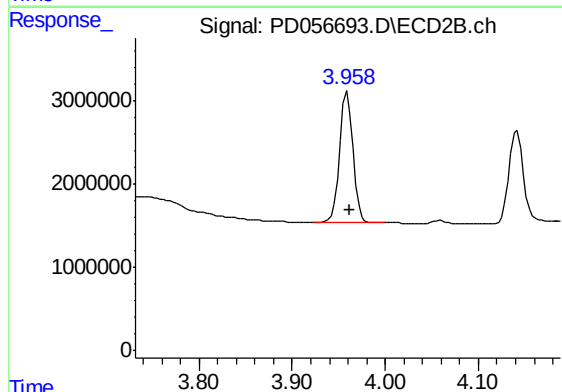


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: -0.003 min
Response: 15711402
Conc: 13.07 ng/ml

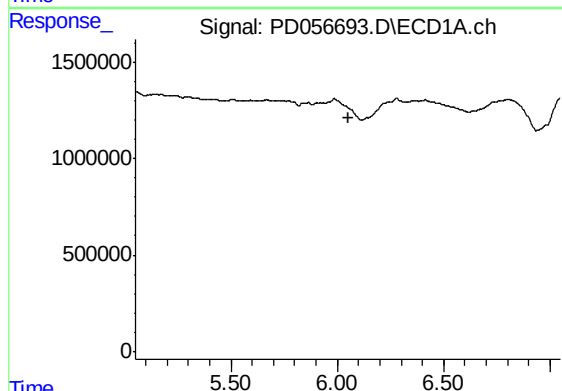


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.051 min
Response: 0
Conc: N.D.

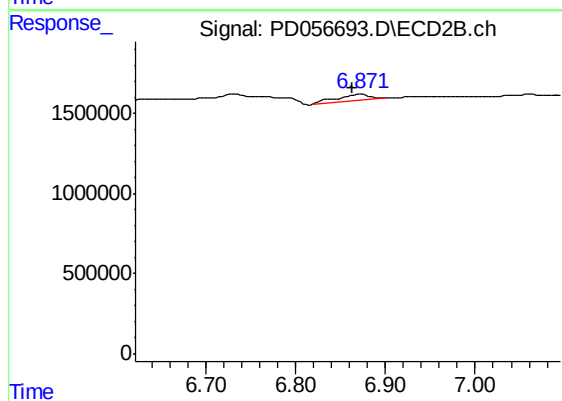

#15 Endosulfan II


R.T.: 6.872 min
Delta R.T.: 0.009 min
Response: 1031719
Conc: 0.70 ng/ml

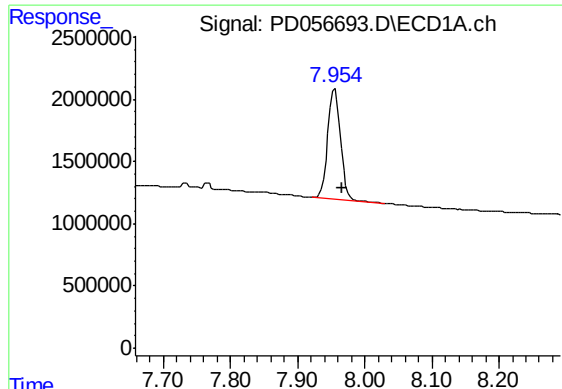

#27 Decachlorobiphenyl

R.T.: 7.955 min
Delta R.T.: -0.010 min
Response: 11796134
Conc: 13.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFEW8

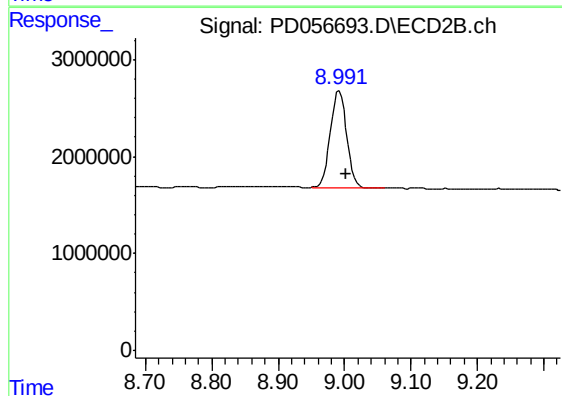

#27 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: -0.010 min
Response: 17115304
Conc: 14.23 ng/ml