

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122019\
 Data File : PD056675.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2019 12:23
 Operator : SG\AJ
 Sample : K6238-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFPZ7

Manual Integrations
 APPROVED

Ankita
 12/23/2019 11:02:41 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 22:11:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.292	3.959	5562629	12220206	6.717	10.164 #
2) SA Decachlor...	7.965	8.995	8274713	11212838	9.164	9.320m
Target Compounds						
10) B trans-Chl...	5.176	6.048	1016298	3978914	0.969m	2.406m#
11) B cis-Chlor...	5.234	6.130	1200334	3078579	1.175m	1.910 #
12) B 4,4'-DDE	5.403	6.282	702465	1870517	0.695m	1.191 #
16) A 4,4'-DDD	5.916	6.771	491264	1417037	0.690m	1.204m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122019\
Data File : PD056675.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2019 12:23
Operator : SG\AJ
Sample : K6238-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 22:11:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

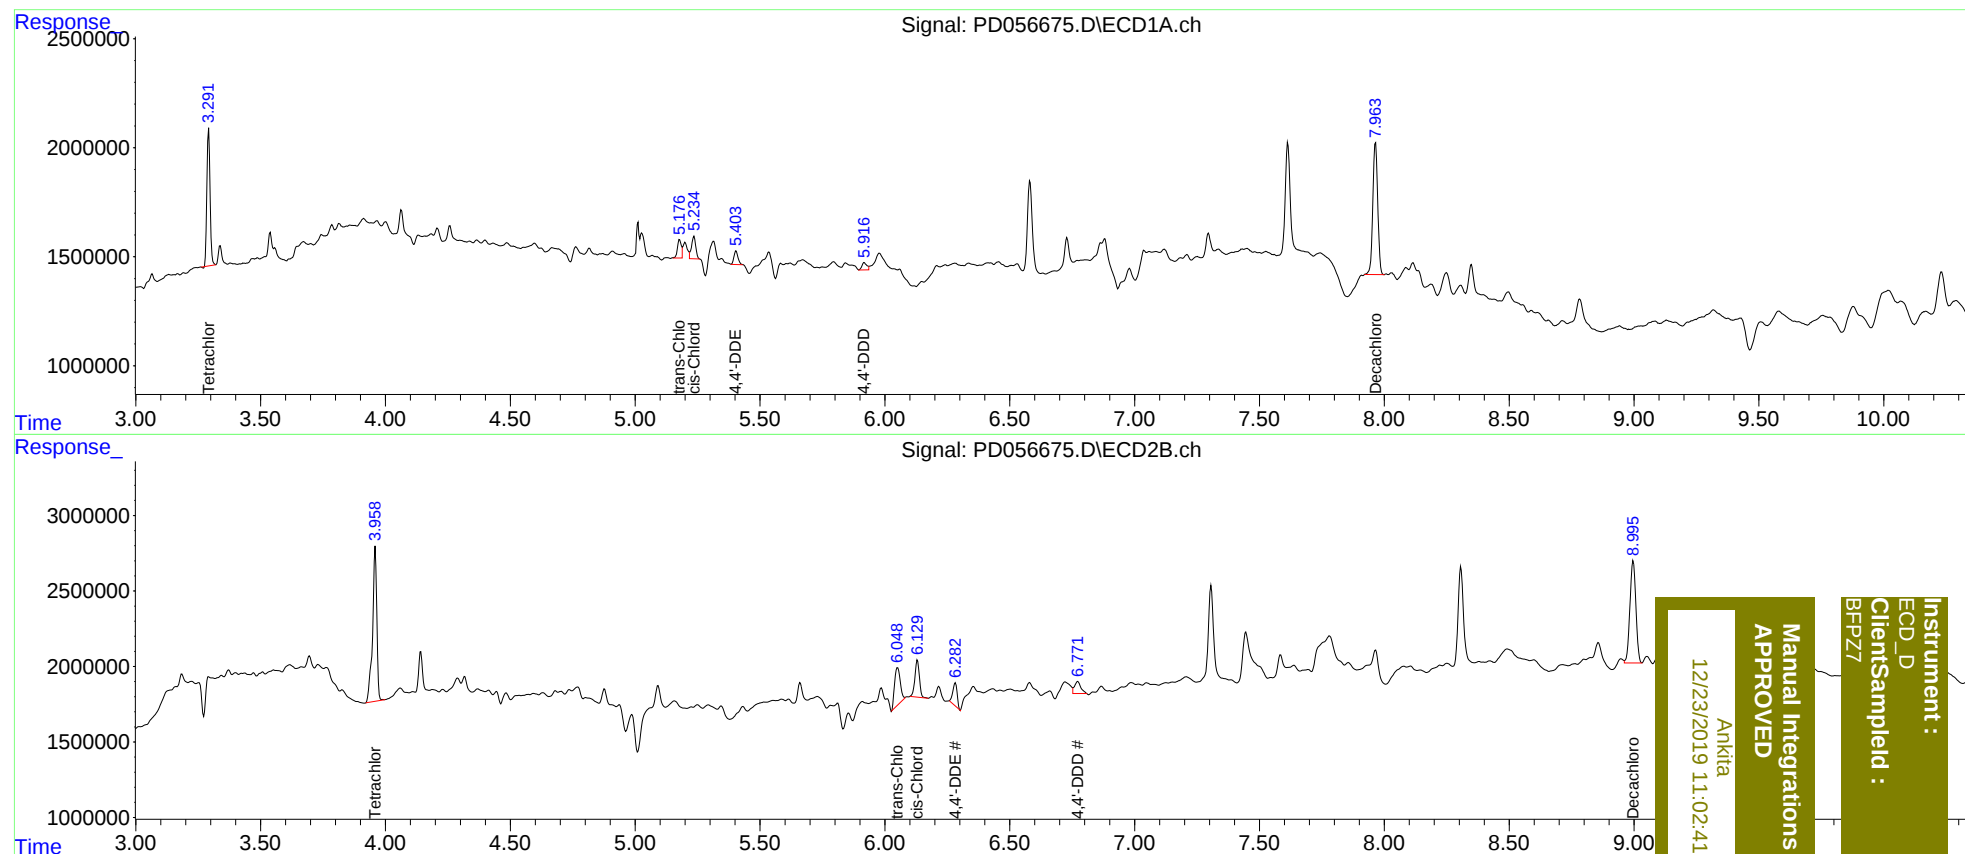

Instrument :
ECD_D
ClientSampled :
BFPZ7

Manual Integrations
APPROVED
Ankita
12/23/2019 11:02:41 AM