

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122019\
 Data File : PD056700.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2019 18:26
 Operator : SG\AJ
 Sample : K6277-22MSD
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0C93MSD

Manual Integrations
 APPROVED

Ankita
 12/23/2019 11:03:17 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 00:51:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.959	10921579	17270731	13.187	14.365
27)	SA Decachlor...	7.956	8.991	12138753	21599706	13.443	17.953m#
Target Compounds							
3)	MA gamma-BHC...	3.987	4.627	41131805	61992121	36.629	38.413m
4)	MA Heptachlor	4.272	5.132	37137919	56497951	36.846	34.666m
5)	MB Aldrin	4.510	5.437	31191204	49148880	28.721m	29.911
13)	MA Dieldrin	5.517	6.431	68625546	92900377	67.561	59.119m
14)	MA Endrin	5.771	6.649	49358613	78137374	59.063	61.740
15)	B Endosulfa...	6.050	6.846	3787374	3549081	3.976m	2.422 #
16)	A 4,4'-DDD	5.910	6.767	4881088	11535655	6.858	9.803 #
17)	MA 4,4'-DDT	6.140	7.069	38840848	72770699	55.200	61.558

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122019\
Data File : PD056700.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2019 18:26
Operator : SG\AJ
Sample : K6277-22MSD
Misc :
ALS Vial : 35 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 00:51:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

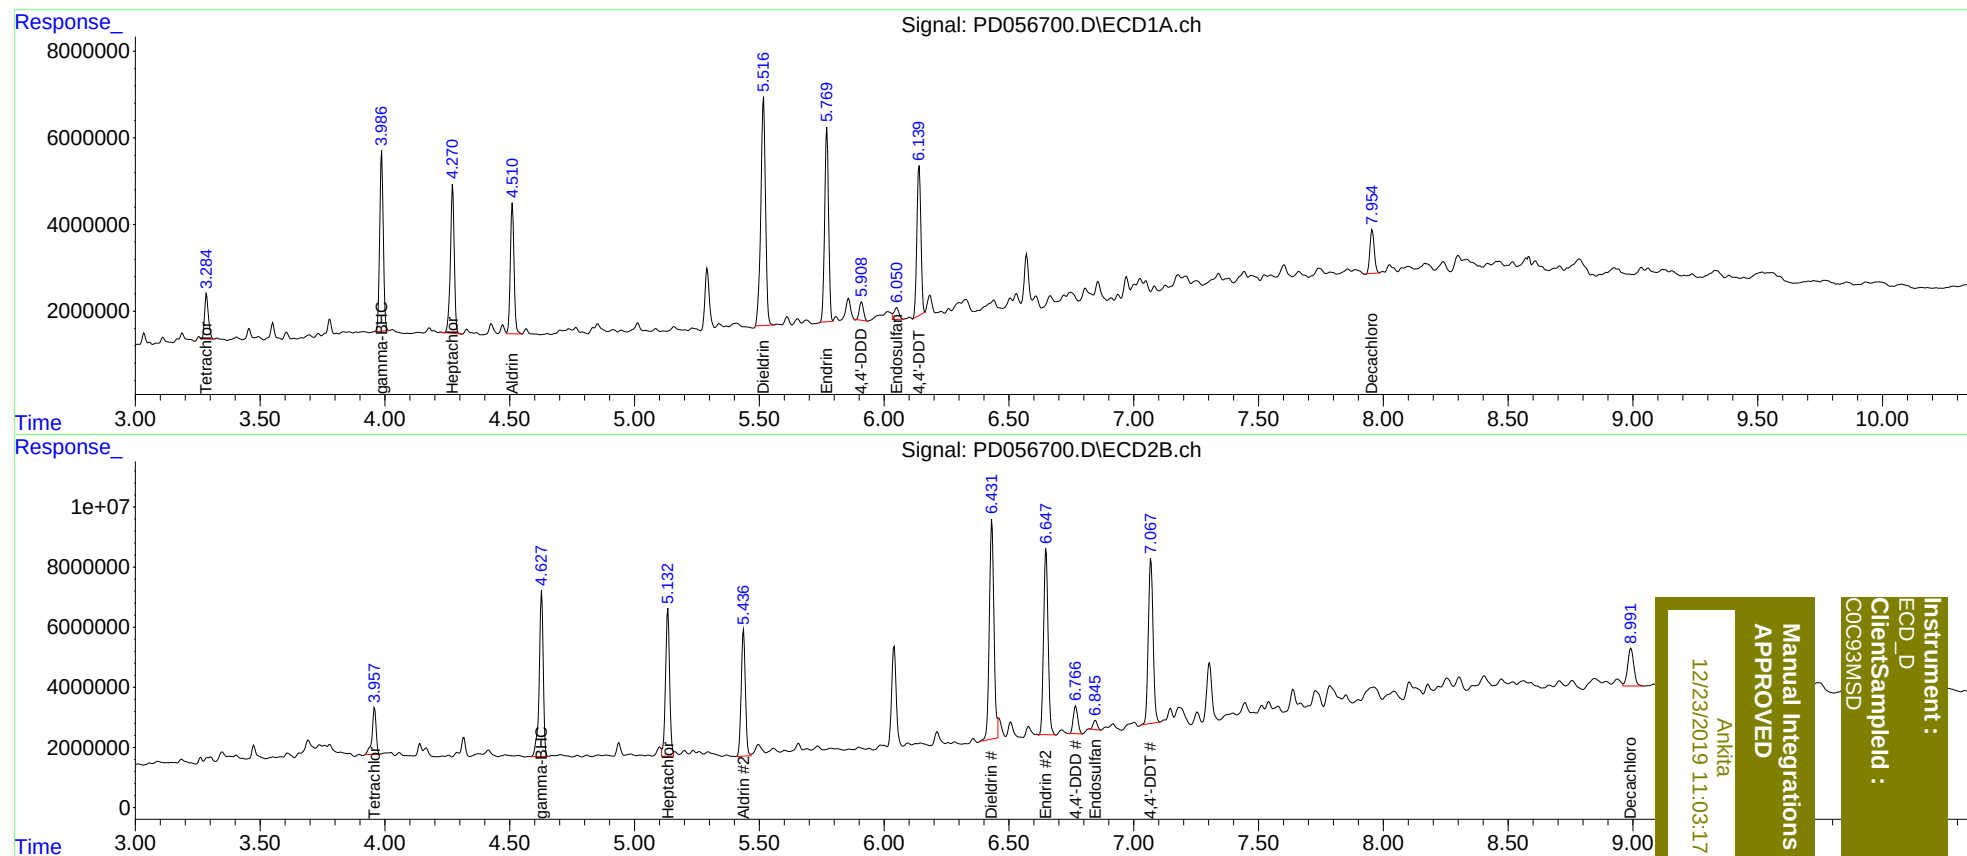

12/23/2019 11:03:17 AM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
Client Sampled :
C0C93MSD