

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122022\
 Data File : PD073370.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2022 17:13
 Operator : AR\AJ
 Sample : N6129-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 20:23:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121622.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 16 15:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.694	3.455	20900073	799.2E6	9.972	8.127
28)	SA Decachlor...	7.821	8.902	27511546	189.1E6	11.363	10.725
Target Compounds							
2)	A alpha-BHC	0.000	3.900f	0	4814195	N.D.	0.036 #
3)	MA gamma-BHC...	0.000	4.247	0	19559629	N.D.	0.198 #
4)	MA Heptachlor	0.000	4.819	0	6150794	N.D.	0.097 #
6)	B beta-BHC	0.000	4.484	0	3433018	N.D.	0.101 #
8)	B Heptachlo...	0.000	5.609f	0	568047	N.D.	0.013 #
11)	B alpha-Chl...	0.000	5.897f	0	4711803	N.D.	0.108 #
16)	A 4,4'-DDD	5.672f	0.000	10142736	0	4.497	N.D. #
18)	B Endrin al...	6.045	0.000	153192	0	0.081	N.D. #
26)	Chlordane-4	0.000	5.897f	0	4711803	N.D.	0.647 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122022\
Data File : PD073370.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2022 17:13
Operator : AR\AJ
Sample : N6129-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 20:23:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121622.M
Quant Title : GC Extractables
QLast Update : Fri Dec 16 15:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

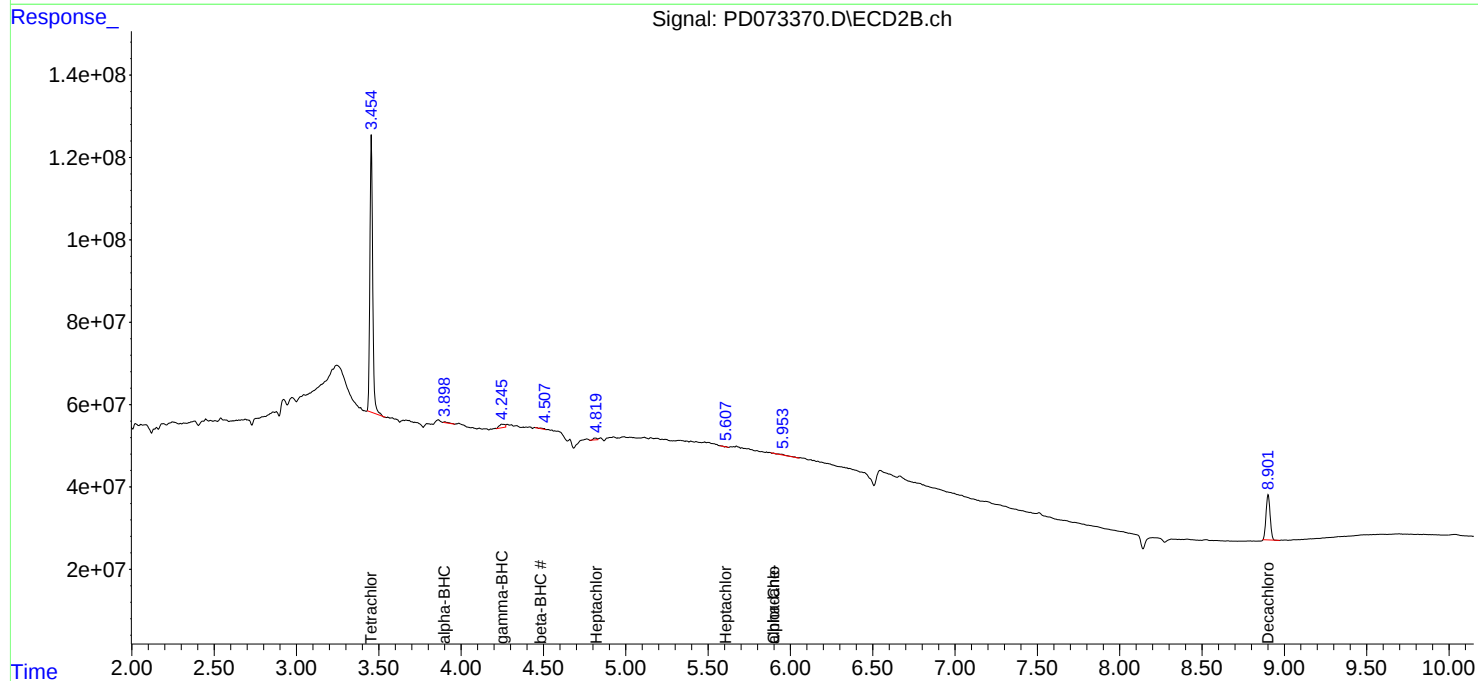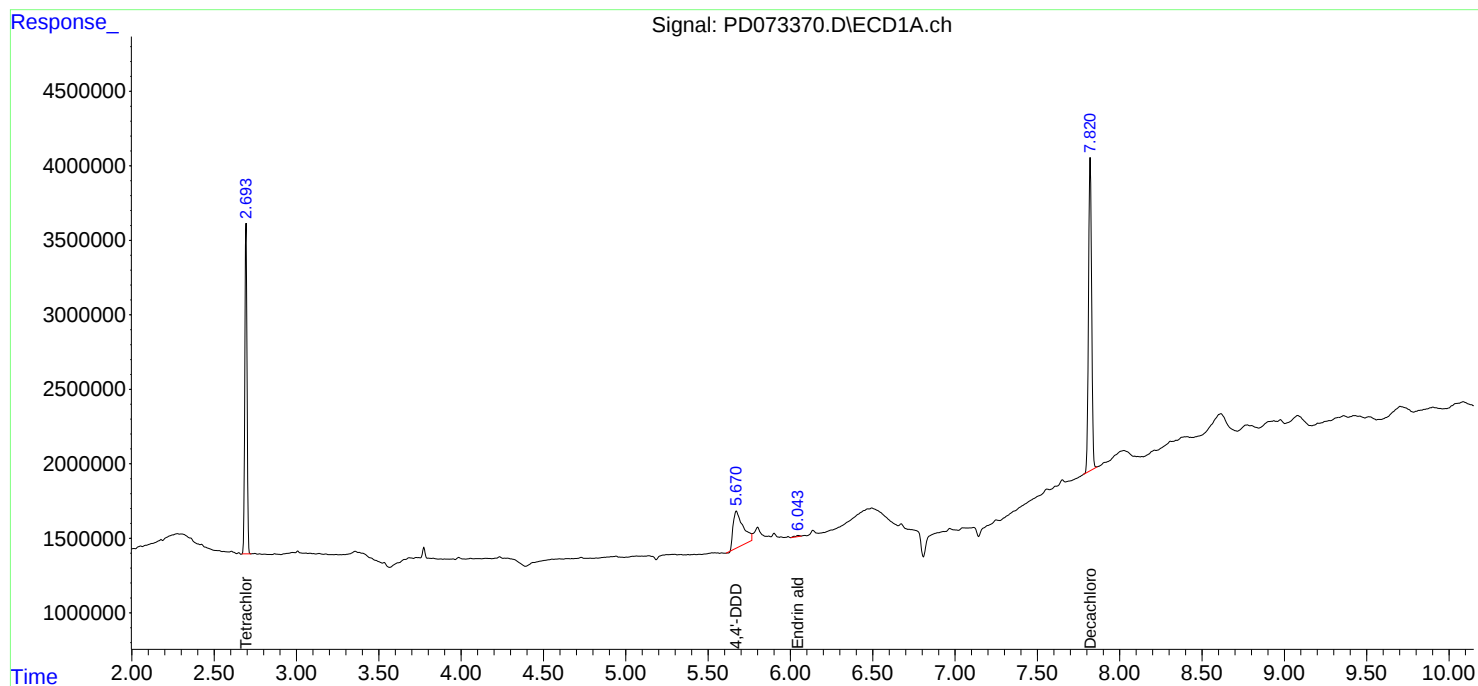


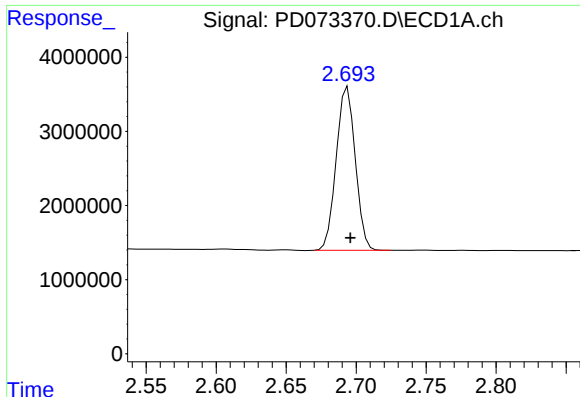

#1 Tetrachloro-m-xylene


R.T.: 2.694 min
Delta R.T.: -0.002 min
Response: 20900073
Conc: 9.97 ng/ml

Instrument :
ECD_D
ClientSampleId :

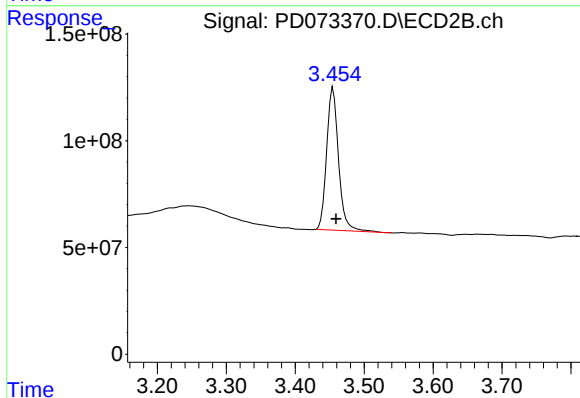


#1 Tetrachloro-m-xylene

R.T.: 3.455 min
Delta R.T.: -0.004 min
Response: 799241144
Conc: 8.13 ng/ml

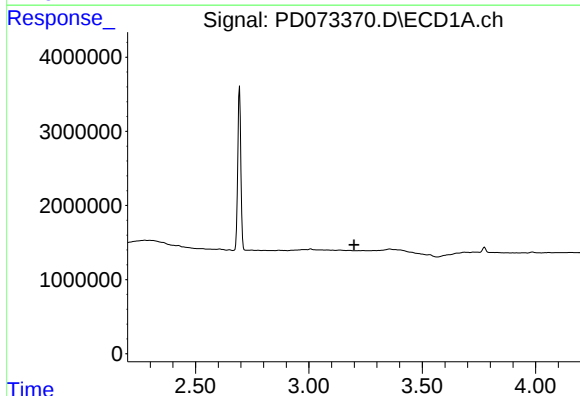


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.199 min
Response: 0
Conc: N.D.

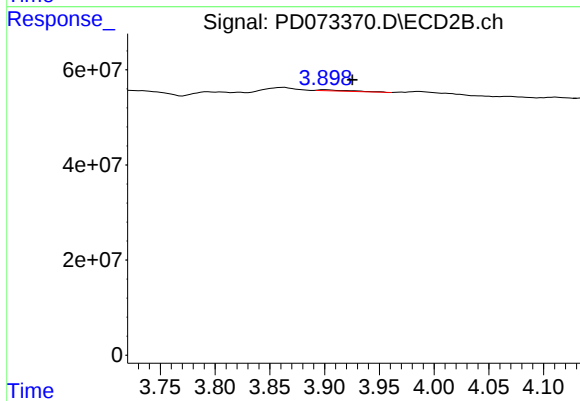

#2 alpha-BHC


R.T.: 3.900 min
Delta R.T.: -0.025 min
Response: 4814195
Conc: 0.04 ng/ml

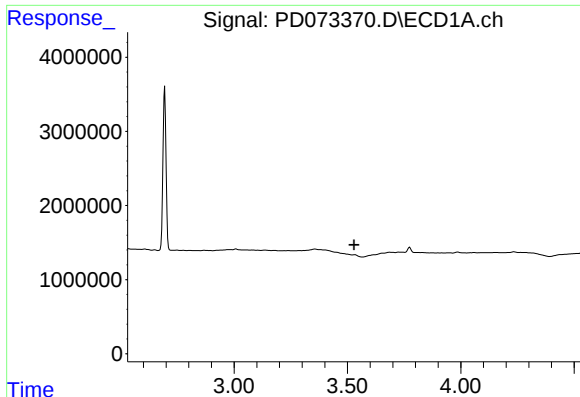

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 3.529 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

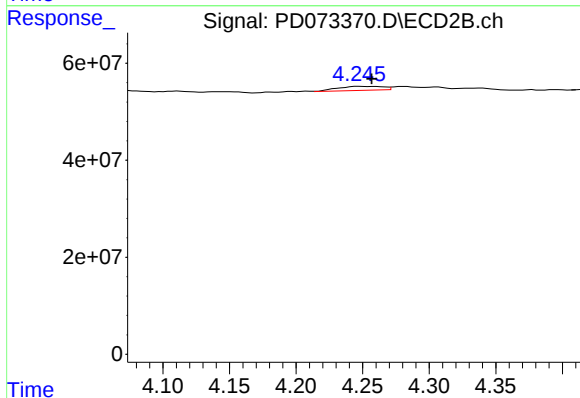


#3 gamma-BHC (Lindane)

R.T.: 4.247 min
Delta R.T.: -0.010 min
Response: 19559629
Conc: 0.20 ng/ml

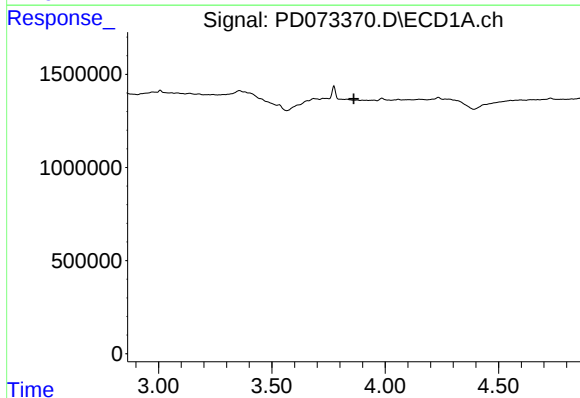


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 3.861 min
Response: 0
Conc: N.D.

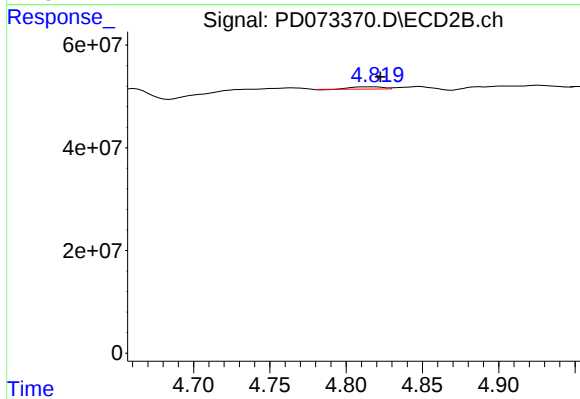

#4 Heptachlor


R.T.: 4.819 min
Delta R.T.: -0.004 min
Response: 6150794
Conc: 0.10 ng/ml

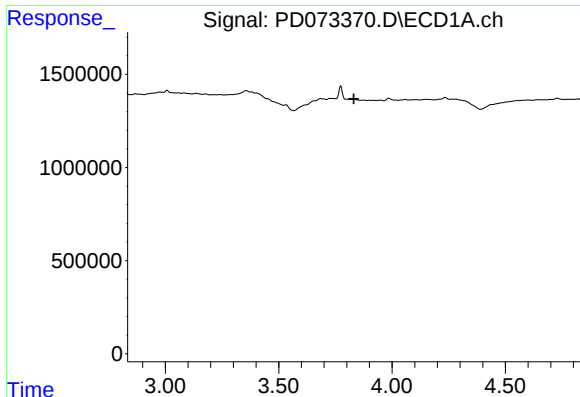

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 3.831 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

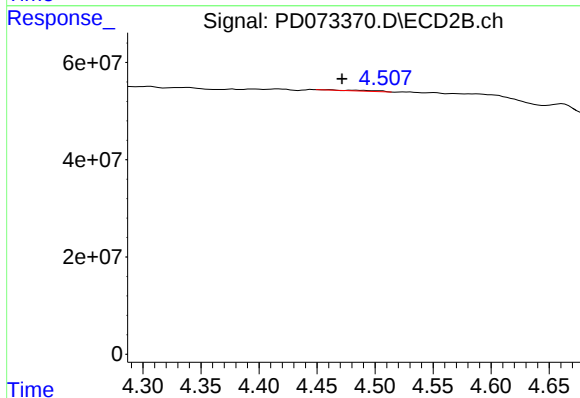


#6 beta-BHC

R.T.: 4.484 min
Delta R.T.: 0.013 min
Response: 3433018
Conc: 0.10 ng/ml

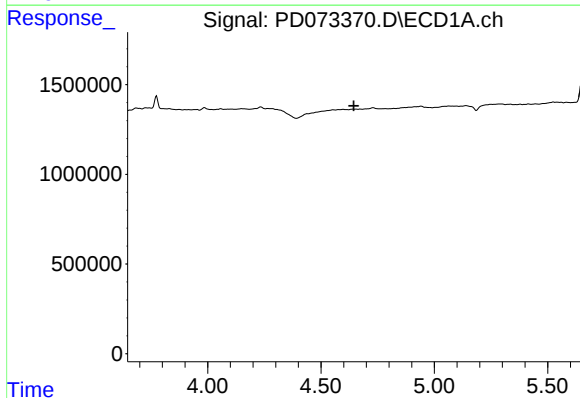


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.645 min
Response: 0
Conc: N.D.

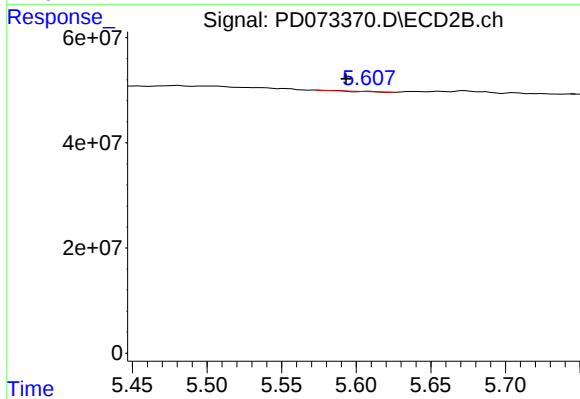

#8 Heptachlor epoxide


R.T.: 5.609 min
Delta R.T.: 0.016 min
Response: 568047
Conc: 0.01 ng/ml

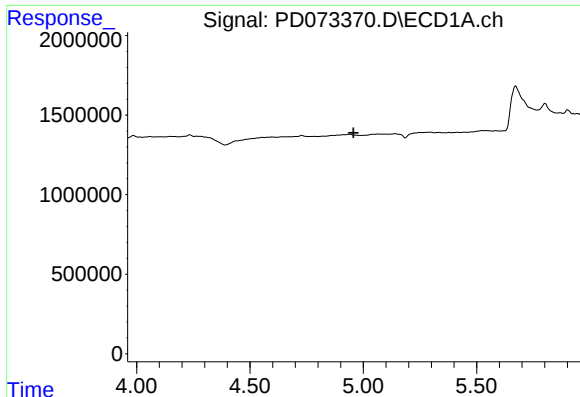

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 4.957 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

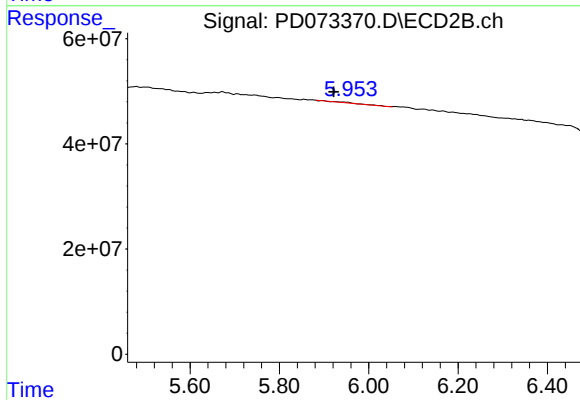


#11 alpha-Chlordane

R.T.: 5.897 min
Delta R.T.: -0.025 min
Response: 4711803
Conc: 0.11 ng/ml

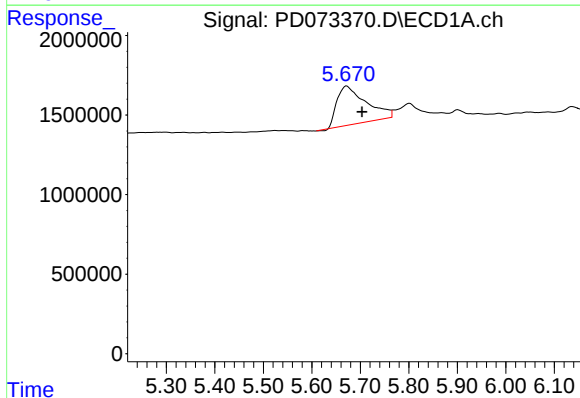


#16 4,4'-DDD

R.T.: 5.672 min
Delta R.T.: -0.032 min
Response: 10142736
Conc: 4.50 ng/ml

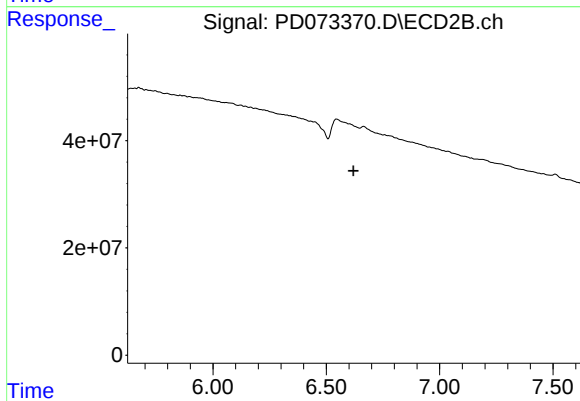

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.620 min
Response: 0
Conc: N.D.

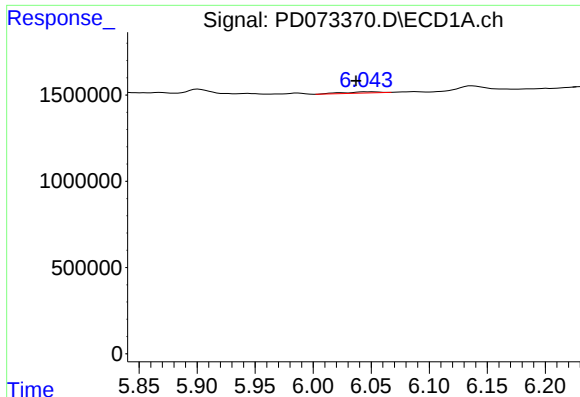

#18 Endrin aldehyde


R.T.: 6.045 min
Delta R.T.: 0.008 min
Response: 153192
Conc: 0.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

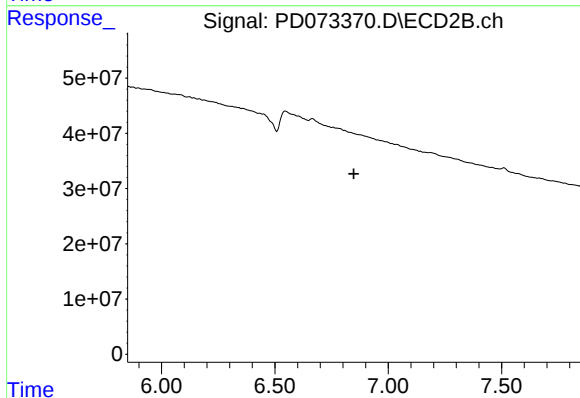


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.848 min
Response: 0
Conc: N.D.

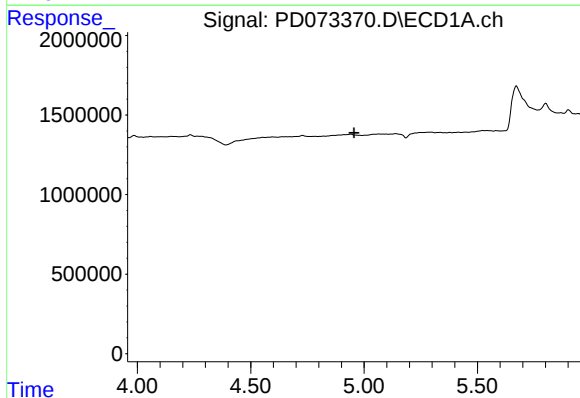


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 4.956 min
Response: 0
Conc: N.D.

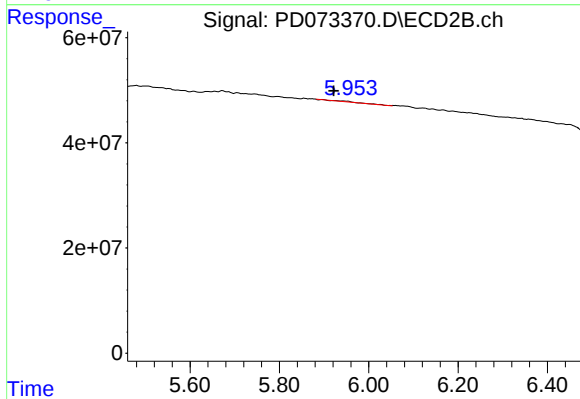

#26 Chlordane-4


R.T.: 5.897 min
Delta R.T.: -0.025 min
Response: 4711803
Conc: 0.65 ng/ml

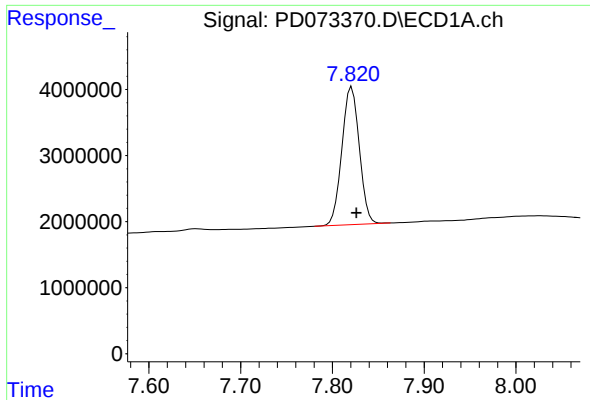

#28 Decachlorobiphenyl

R.T.: 7.821 min
Delta R.T.: -0.005 min
Response: 27511546
Conc: 11.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

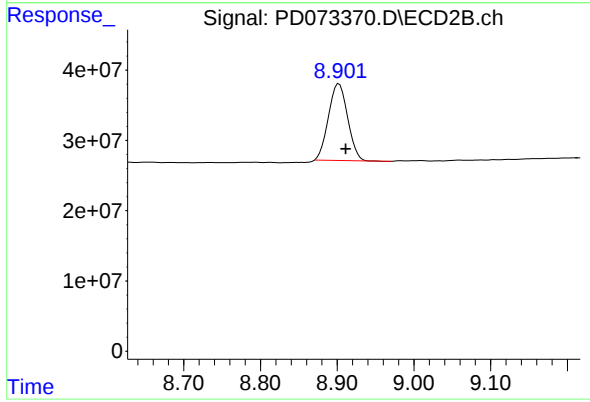

#28 Decachlorobiphenyl

R.T.: 8.902 min
Delta R.T.: -0.009 min
Response: 189058001
Conc: 10.73 ng/ml