

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122022\
 Data File : PD073380.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2022 19:26
 Operator : AR\AJ
 Sample : N6092-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 20221269-FIELD-BLANK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 20:35:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121622.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 16 15:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.695	3.456	29890298	983.7E6	14.262	10.002 #
28)	SA Decachlor...	7.820	8.903	21359445	141.2E6	8.822	8.008

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122022\
Data File : PD073380.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2022 19:26
Operator : AR\AJ
Sample : N6092-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
20221269-FIELD-BLANK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 20:35:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121622.M
Quant Title : GC Extractables
QLast Update : Fri Dec 16 15:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

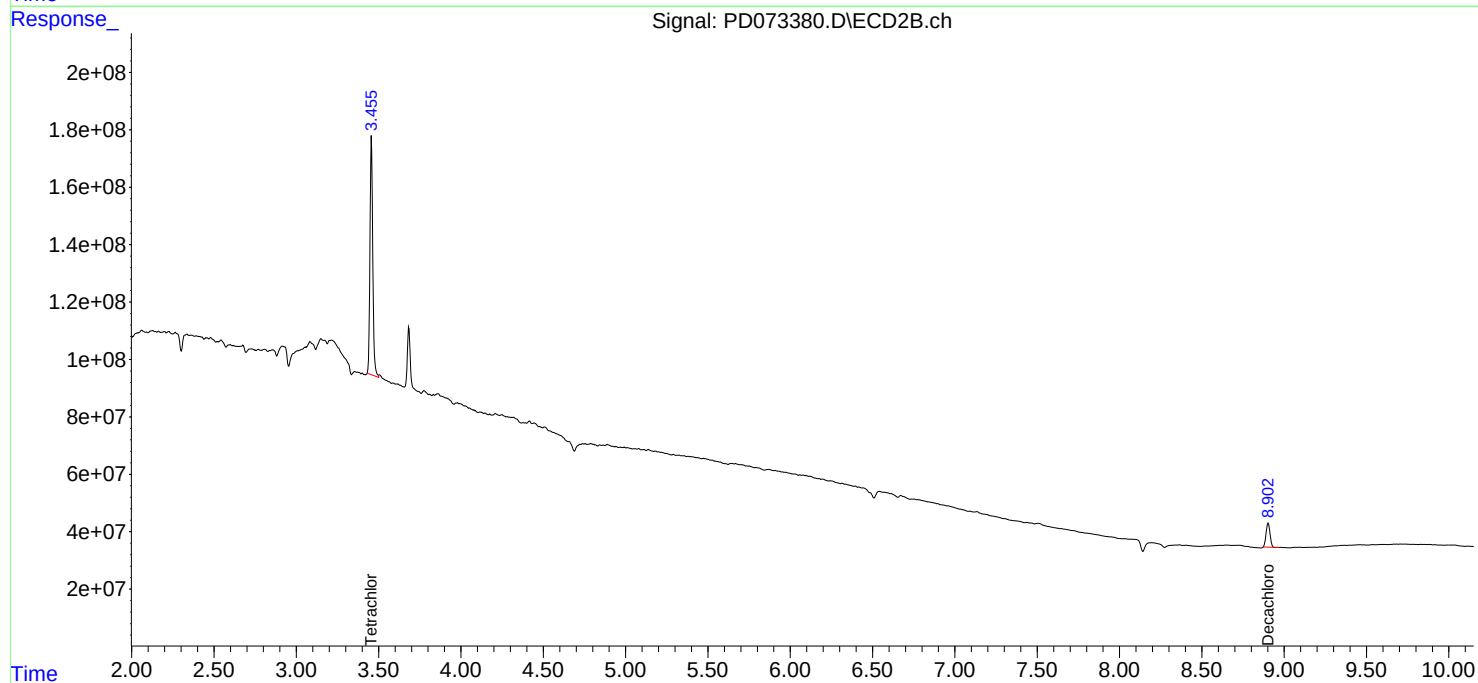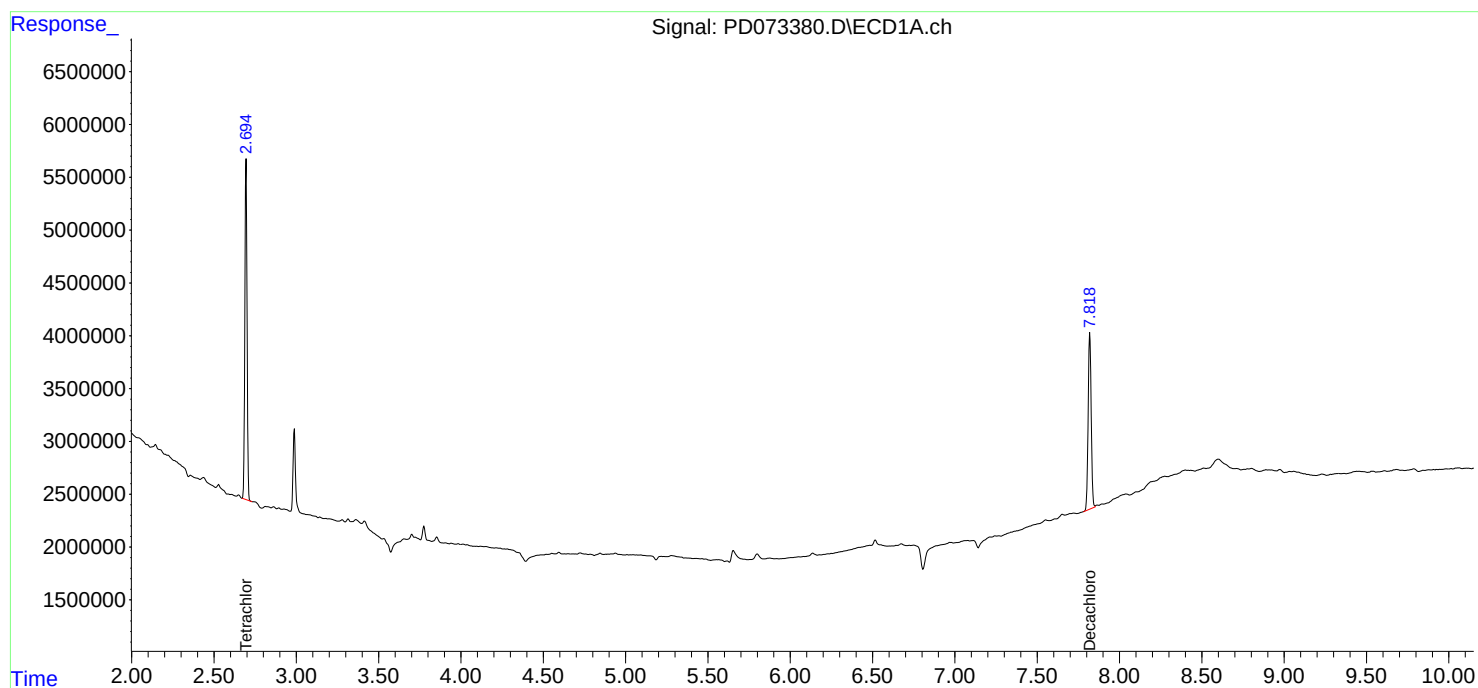


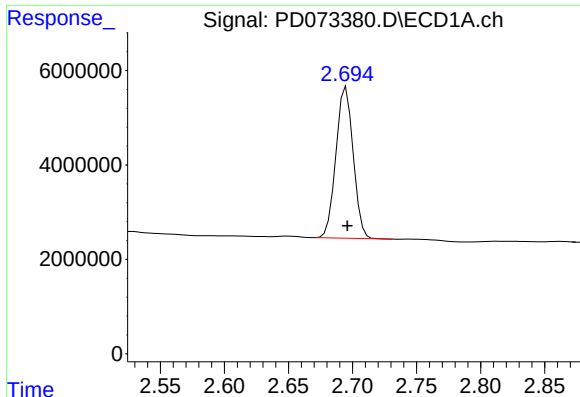

#1 Tetrachloro-m-xylene


R.T.: 2.695 min
Delta R.T.: 0.000 min
Response: 29890298
Conc: 14.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
20221269-FIELD-BLANK

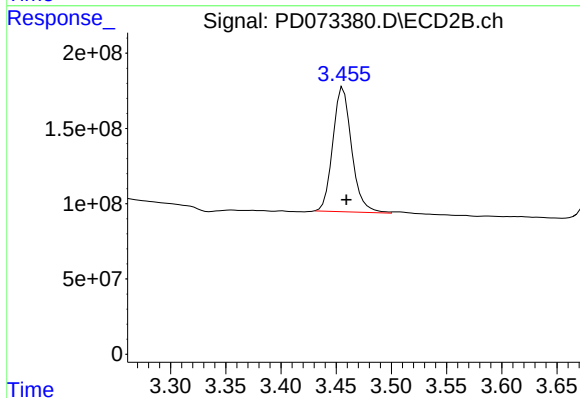


#1 Tetrachloro-m-xylene

R.T.: 3.456 min
Delta R.T.: -0.003 min
Response: 983670005
Conc: 10.00 ng/ml

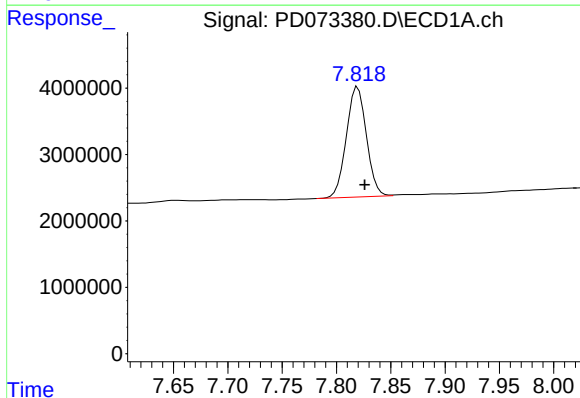

#28 Decachlorobiphenyl

R.T.: 7.820 min
Delta R.T.: -0.006 min
Response: 21359445
Conc: 8.82 ng/ml

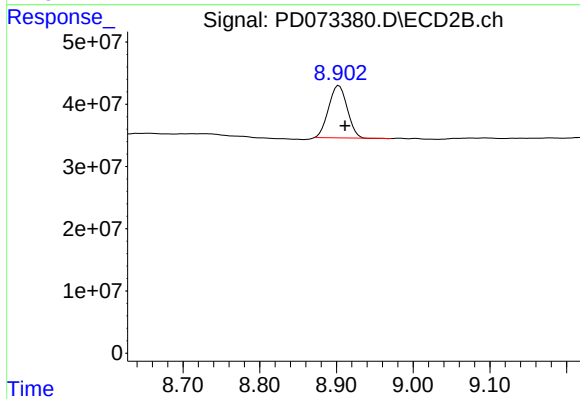

#28 Decachlorobiphenyl

R.T.: 8.903 min
Delta R.T.: -0.008 min
Response: 141154760
Conc: 8.01 ng/ml