

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122022\
 Data File : PD073381.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2022 19:40
 Operator : AR\AJ
 Sample : N6099-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PURGE-WATER-2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/21/2022
 Supervised By : Ankita Jodhani 12/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 20:36:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121622.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 16 15:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	2.695	3.456	28700494	909.9E6	13.694	9.252 #
2) SA Decachlor...	7.820	8.902	27980581	200.9E6	11.556	11.396m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122022\
Data File : PD073381.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2022 19:40
Operator : AR\AJ
Sample : N6099-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
PURGE-WATER-2


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/21/2022
Supervised By : Ankita Jodhani 12/21/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 20:36:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121622.M
Quant Title : GC Extractables
QLast Update : Fri Dec 16 15:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

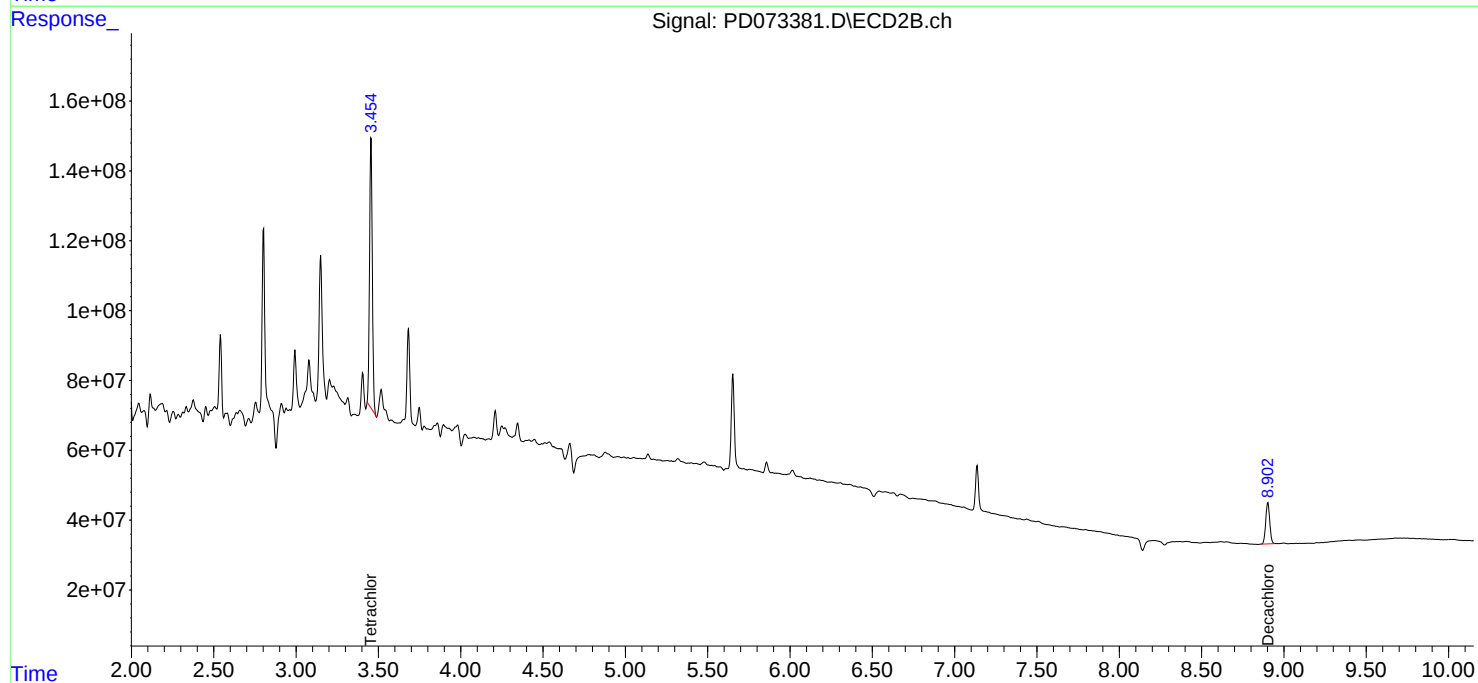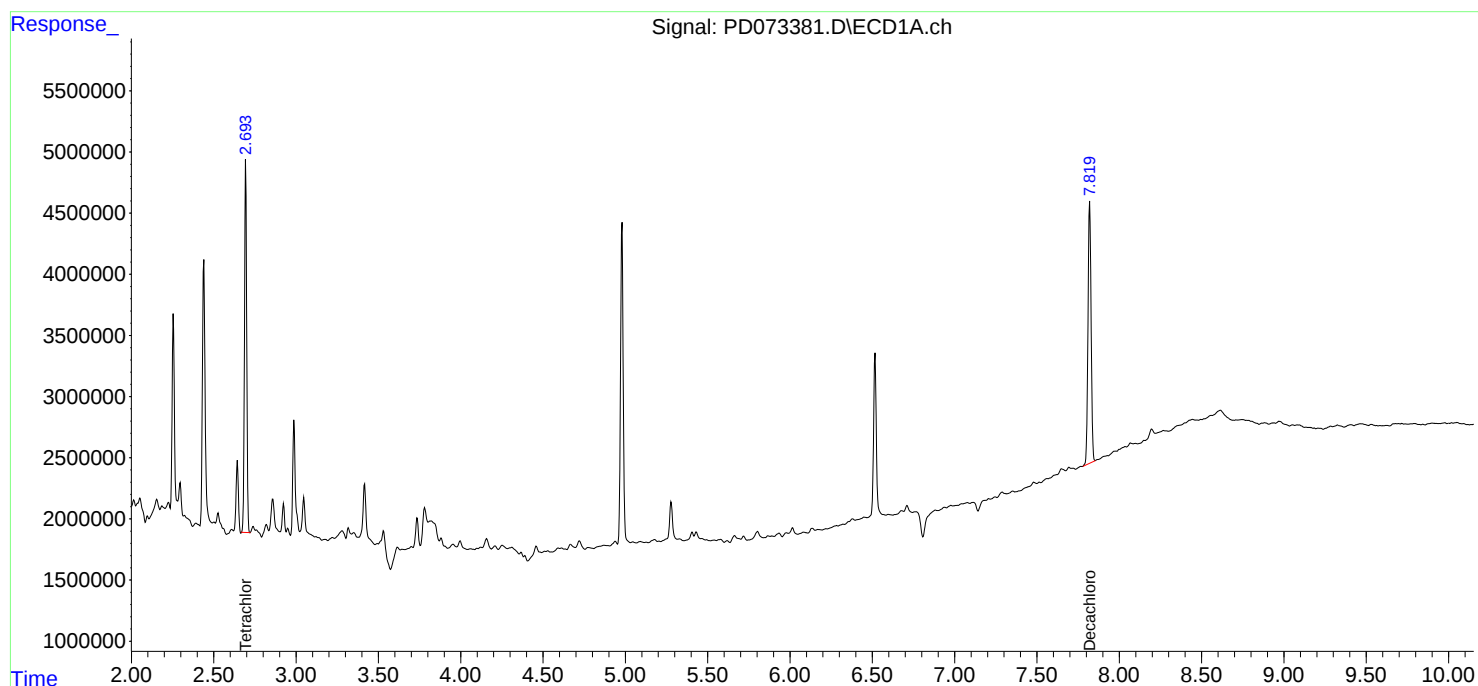

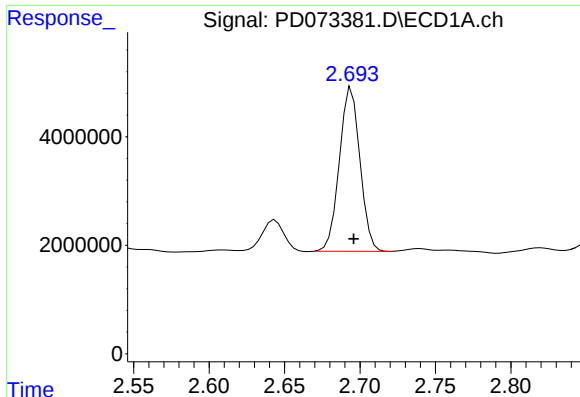


#1 Tetrachloro-m-xylene

R.T.: 2.695 min
Delta R.T.: -0.001 min
Response: 28700494
Conc: 13.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
PURGE-WATER-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/21/2022
Supervised By :Ankita Jodhani 12/21/2022

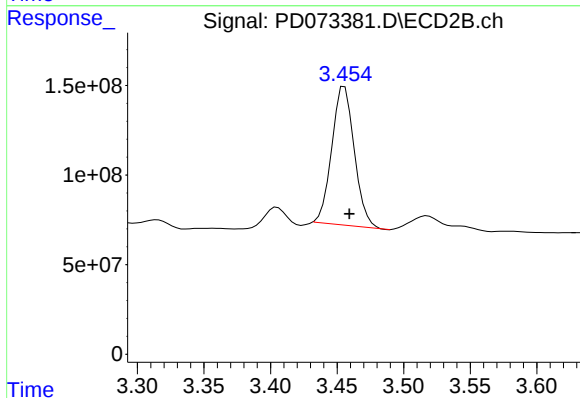


#1 Tetrachloro-m-xylene

R.T.: 3.456 min
Delta R.T.: -0.004 min
Response: 909859744
Conc: 9.25 ng/ml

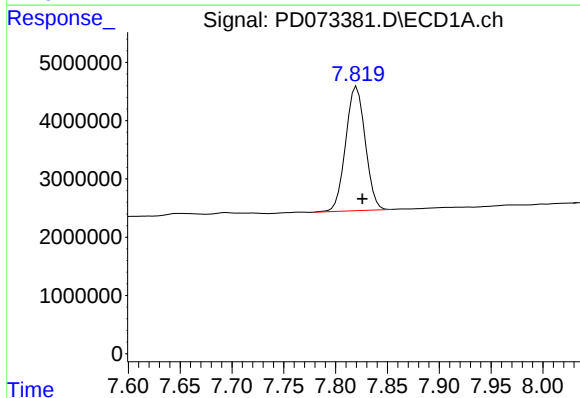

#28 Decachlorobiphenyl

R.T.: 7.820 min
Delta R.T.: -0.006 min
Response: 27980581
Conc: 11.56 ng/ml

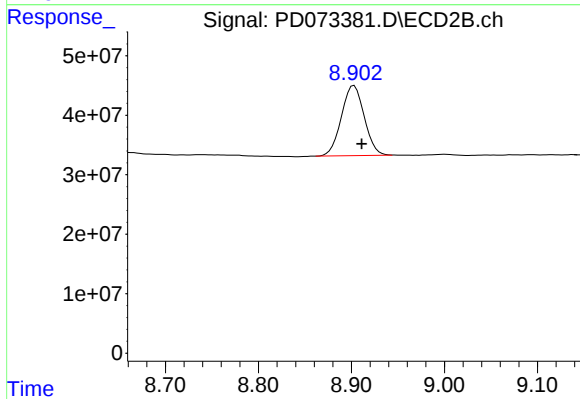

#28 Decachlorobiphenyl

R.T.: 8.902 min
Delta R.T.: -0.010 min
Response: 200886001
Conc: 11.40 ng/ml m