

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122023\
 Data File : PD080185.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2023 10:25
 Operator : AR\AJ
 Sample : 05794-05DL 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH3P9DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/19/2023
 Supervised By : Ankita Jodhani 12/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 00:44:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 18 00:44:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.575	2.799	1948222	4526919	1.526m	2.036 #
27)	SA Decachlor...	9.132	7.949	8232974	17952044	5.121	7.479 #
Target Compounds							
10)	B trans-Chl...	5.956	4.985	146.3E6	310.0E6	71.279m	94.160m#
11)	B cis-Chlor...	6.067	5.100	9981509	22504949	4.755	6.694 #
12)	B 4,4'-DDE	6.237	5.263	372.2E6	479.7E6	192.653m	152.732
13)	MA Dieldrin	6.389	5.394	195.6E6	236.7E6	105.082m	78.963m
14)	MA Endrin	6.618	5.675	59322932	321.0E6	37.875m	122.021m#
15)	B Endosulfa...	6.837	5.957	65681101	87902186	35.034	30.318
17)	MA 4,4'-DDT	7.071	6.064	328.8E6	1757.2E6	222.474m	728.780 #
19)	B Endosulfa...	7.187	6.364	166.7E6	581.7E6	90.887	207.385 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122023\
Data File : PD080185.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2023 10:25
Operator : AR\AJ
Sample : 05794-05DL 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 00:44:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Mon Dec 18 00:44:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

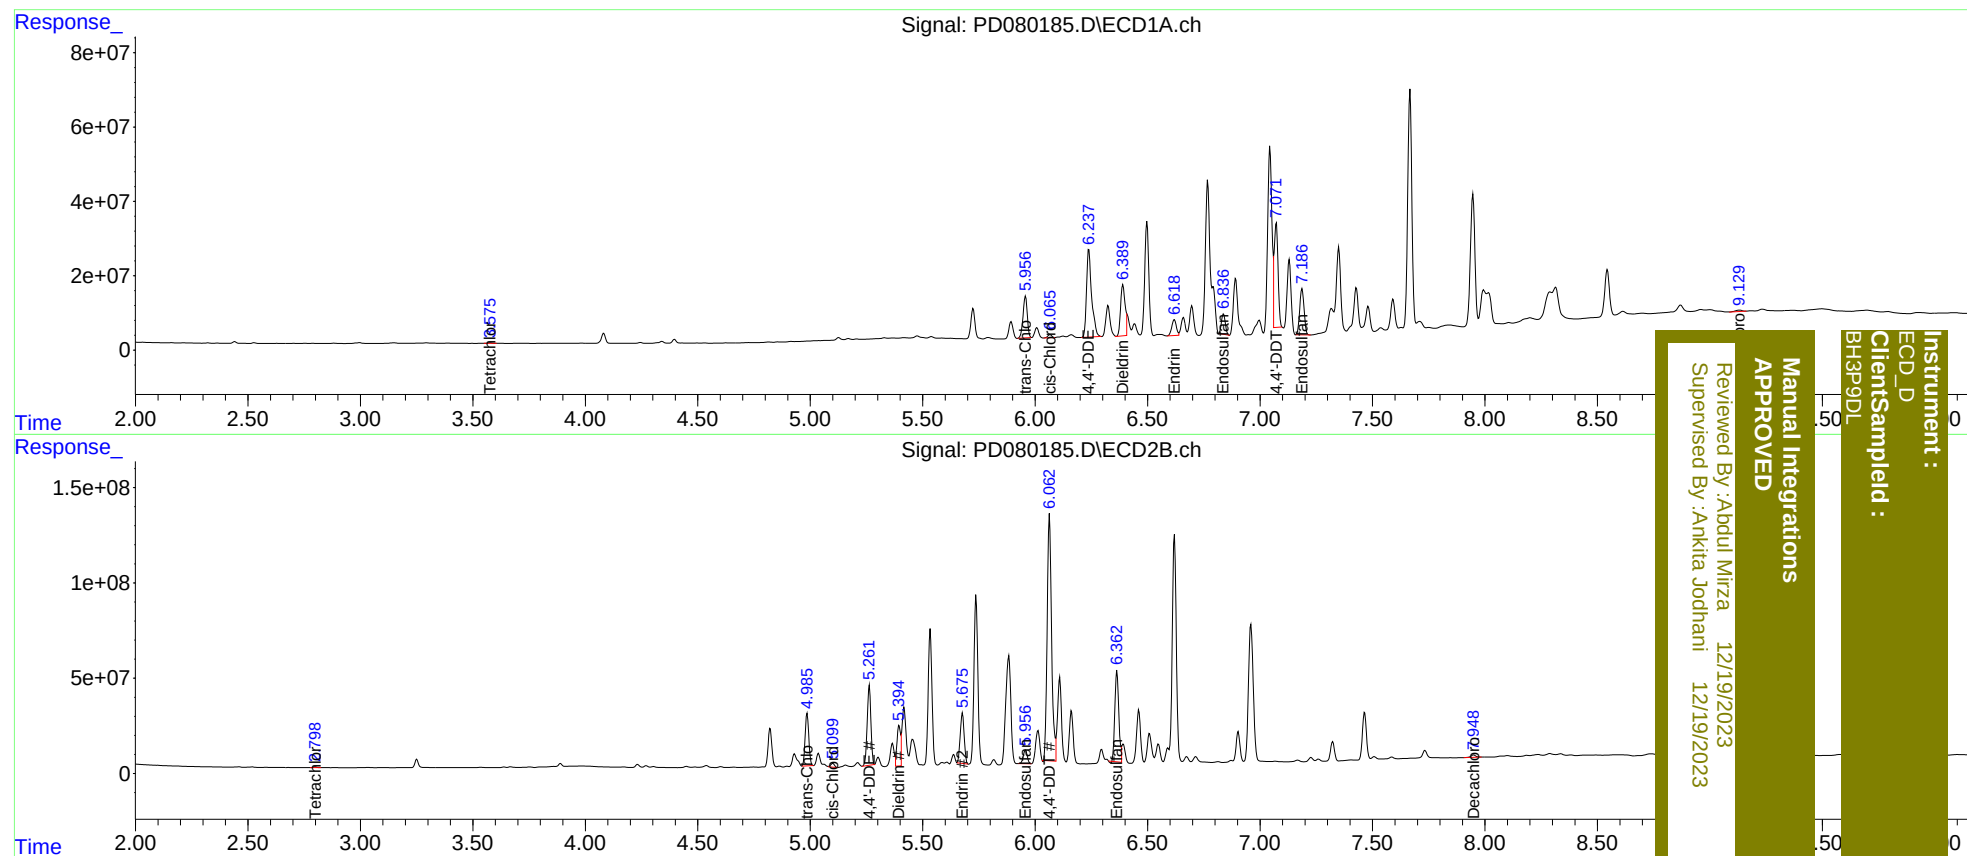

Instrument :
ECD_D
ClientSampled :
BH3P9DL

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/19/2023
Supervised By :Ankita Jodhani 12/19/2023