

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122023\
 Data File : PD080187.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2023 11:18
 Operator : AR\AJ
 Sample : 05794-07DL 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH3Q1DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/19/2023
 Supervised By : Ankita Jodhani 12/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 00:45:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 18 00:44:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.568	2.800	3582920	9121724	2.806	4.102 #
2) SA Decachlor...	9.108	7.947	17797299	16662143	11.070	6.942 #
Target Compounds						
12) B 4,4'-DDE	6.231	5.262	653.3E6	1205.6E6	338.197	383.839
13) MA Dieldrin	6.387	5.395	26752137	116.7E6	14.374m	38.939m#
16) A 4,4'-DDD	6.749	5.817	193.6E6	315.5E6	139.594	137.208
17) MA 4,4'-DDT	7.065	6.068	1095.9E6	1674.6E6	741.591	694.532

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122023\
Data File : PD080187.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2023 11:18
Operator : AR\AJ
Sample : 05794-07DL 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 00:45:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Mon Dec 18 00:44:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

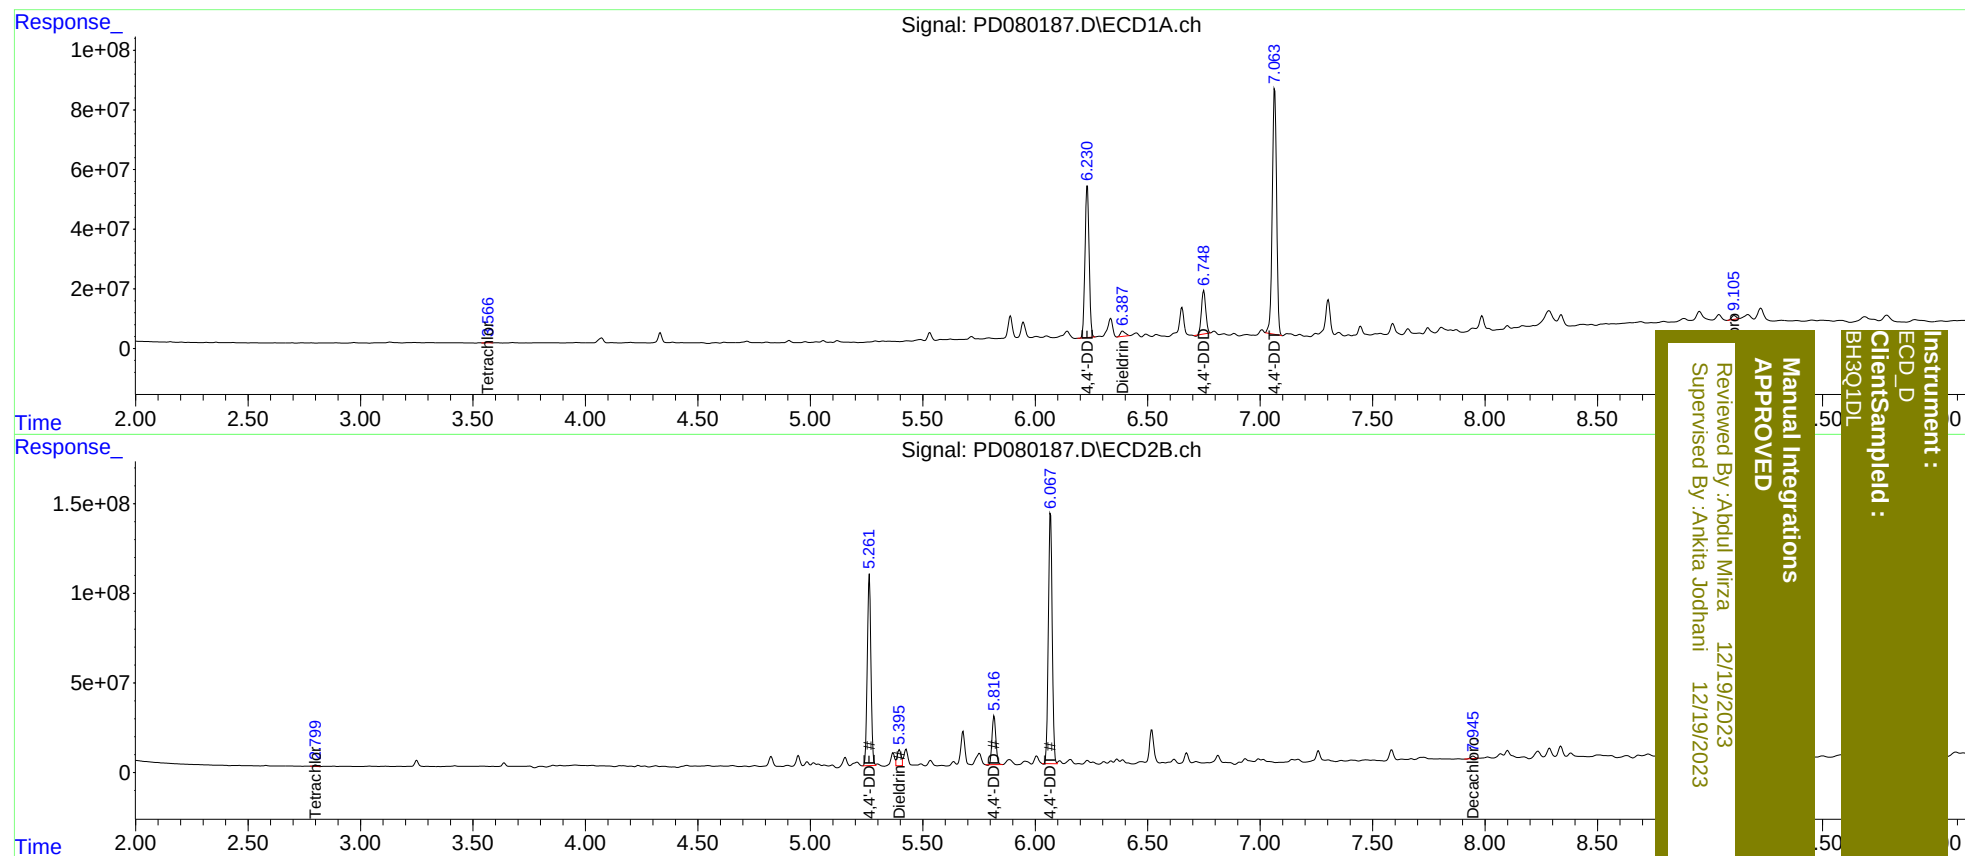

Instrument :
ECD_D
ClientSampled :
BH3Q1DL

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/19/2023
Supervised By :Ankita Jodhani 12/19/2023