

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD122023\  
Data File : PD080200.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 18 Dec 2023 17:52  
Operator : AR\AJ  
Sample : 05794-08DL2 20X  
Misc :  
ALS Vial : 21 Sample Multiplier: 1



Instrument :  
ECD\_D  
ClientSampleId :  
BH3Q2DL2

## Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 12/19/2023  
Supervised By :Ankita Jodhani 12/19/2023

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 19 00:49:41 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD121623CLP.M  
Quant Title : GC Extractables  
QLast Update : Mon Dec 18 00:44:33 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

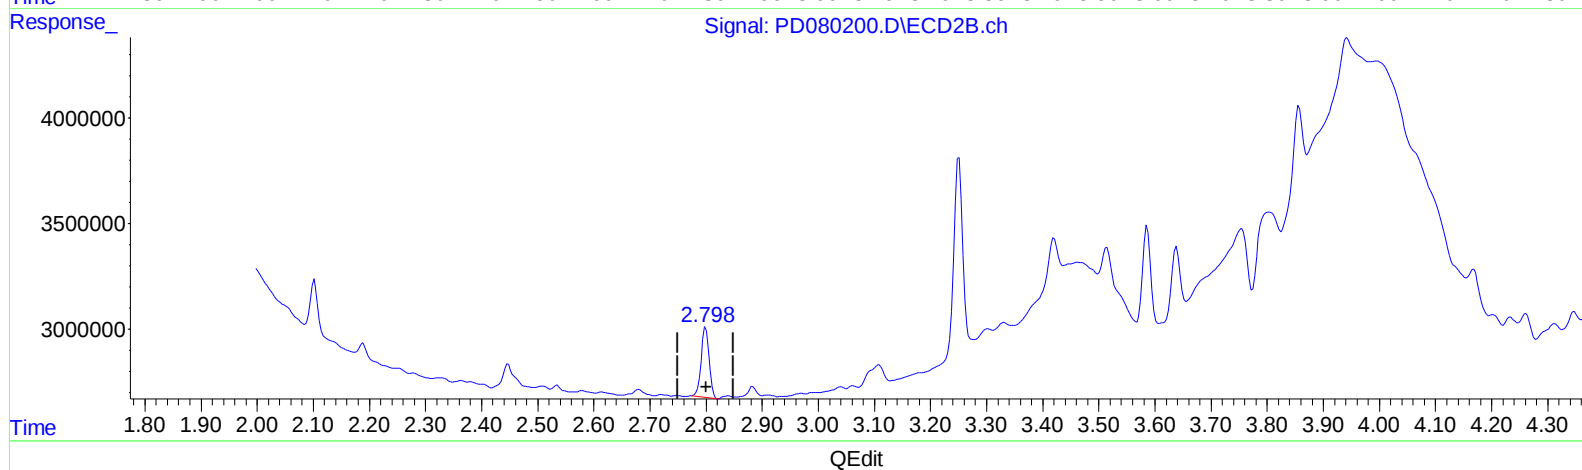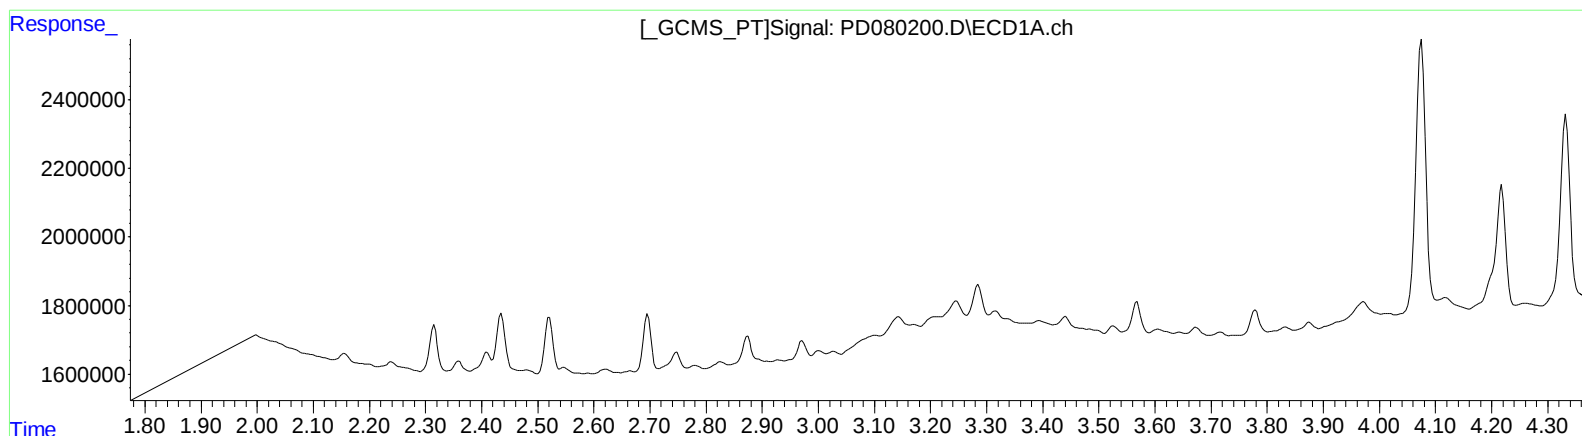

(1) Tetrachloro-m-xylene (SA)

0.000min 0.000 ng/ml

response 0

(1) Tetrachloro-m-xylene #2 (SA)

2.800min 1.502 ng/ml

response 3339061

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD122023\  
Data File : PD080200.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 18 Dec 2023 17:52  
Operator : AR\AJ  
Sample : 05794-08DL2 20X  
Misc :  
ALS Vial : 21 Sample Multiplier: 1


Instrument :  
ECD\_D  
ClientSampleId :  
BH3Q2DL2

## Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 12/19/2023  
Supervised By :Ankita Jodhani 12/19/2023

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 19 00:49:41 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD121623CLP.M  
Quant Title : GC Extractables  
QLast Update : Mon Dec 18 00:44:33 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

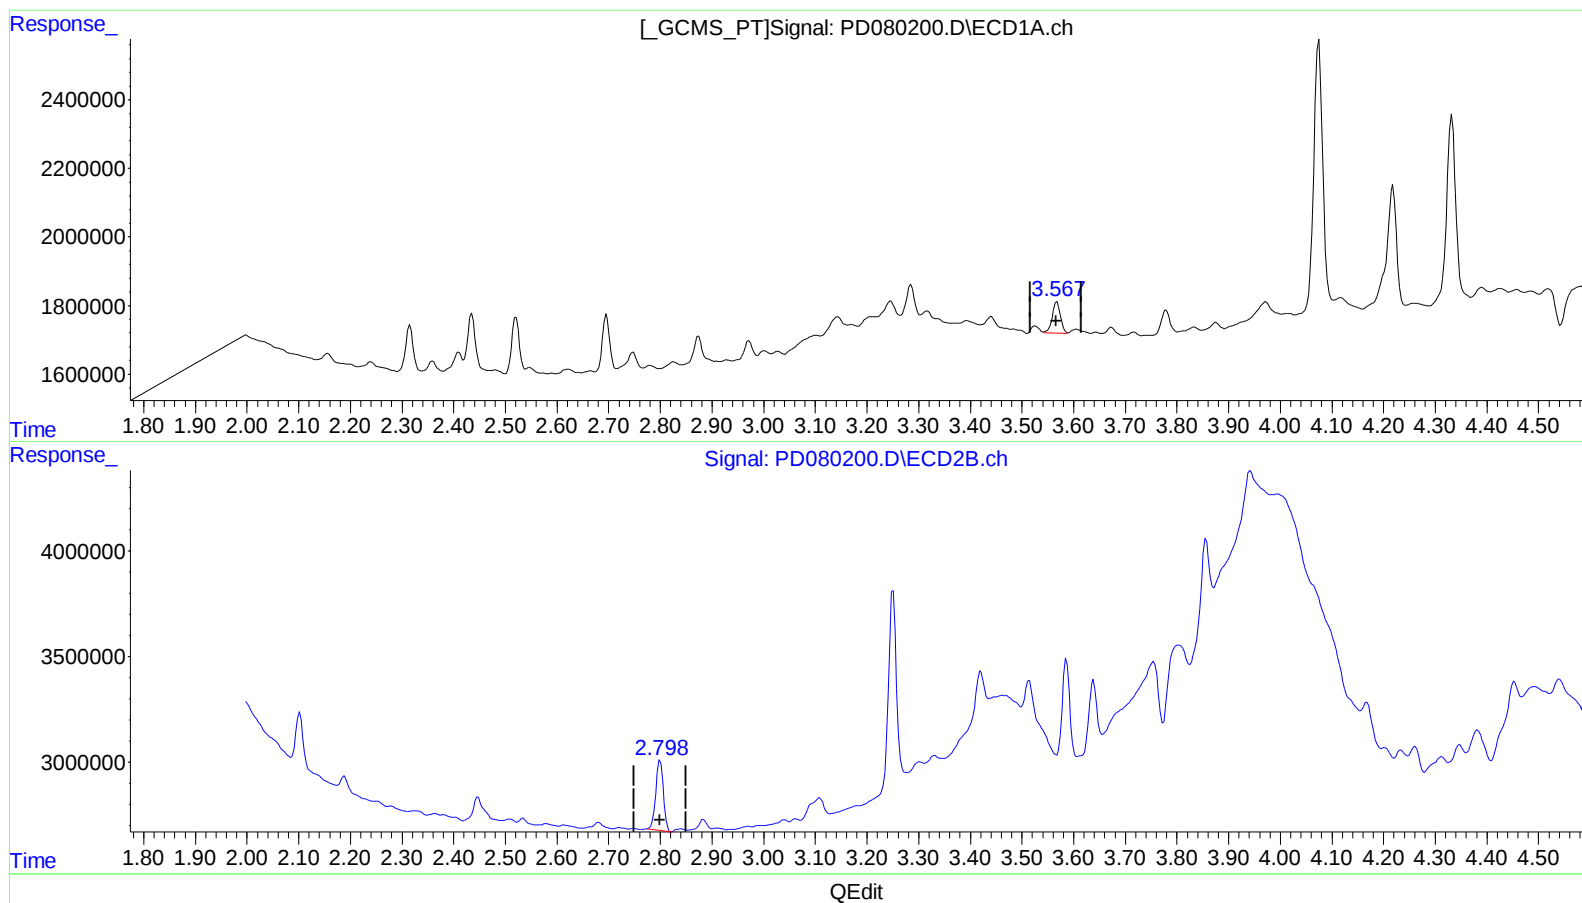

(1) Tetrachloro-m-xylene (SA)

3.567min 0.787 ng/ml m

response 1004440

(1) Tetrachloro-m-xylene #2 (SA)

2.800min 1.502 ng/ml

response 3339061

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD122023\  
Data File : PD080200.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 18 Dec 2023 17:52  
Operator : AR\AJ  
Sample : 05794-08DL2 20X  
Misc :  
ALS Vial : 21 Sample Multiplier: 1



Instrument :  
ECD\_D  
ClientSampleId :  
BH3Q2DL2

## Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 12/19/2023  
Supervised By :Ankita Jodhani 12/19/2023

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 19 00:49:41 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD121623CLP.M  
Quant Title : GC Extractables  
QLast Update : Mon Dec 18 00:44:33 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

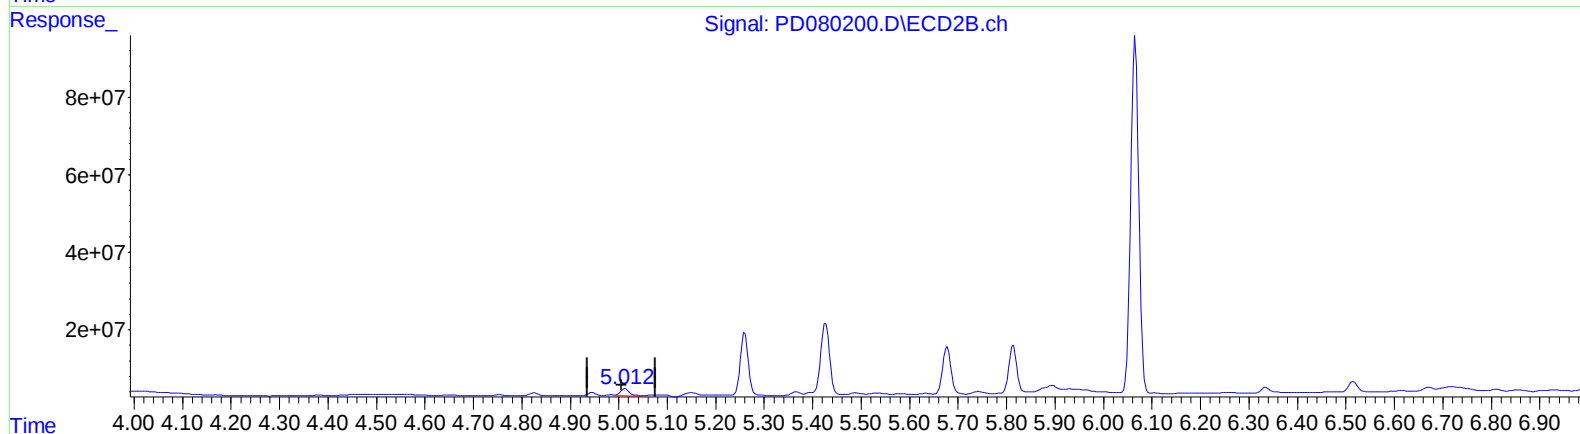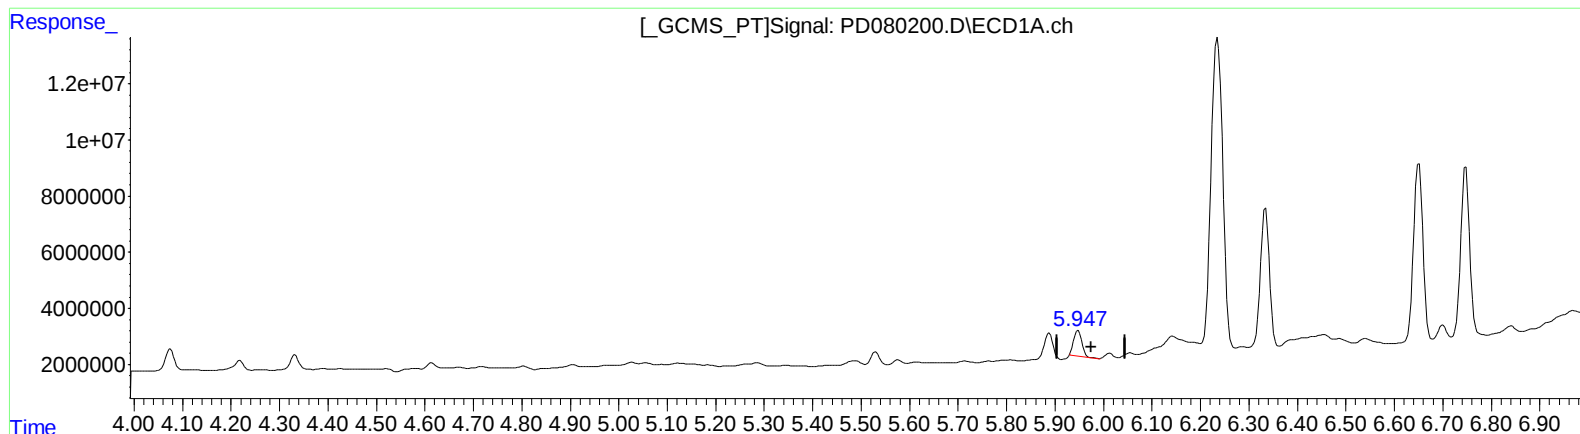

QEdit

(10) trans-Chlordane (B)

5.948min 5.285 ng/ml

response 10845839

(10) trans-Chlordane #2 (B)

5.013min 7.942 ng/ml

response 26144006

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD122023\  
Data File : PD080200.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 18 Dec 2023 17:52  
Operator : AR\AJ  
Sample : 05794-08DL2 20X  
Misc :  
ALS Vial : 21 Sample Multiplier: 1



Instrument :  
ECD\_D  
ClientSampleId :  
BH3Q2DL2

## Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 12/19/2023  
Supervised By :Ankita Jodhani 12/19/2023

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 19 00:49:41 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD121623CLP.M  
Quant Title : GC Extractables  
QLast Update : Mon Dec 18 00:44:33 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

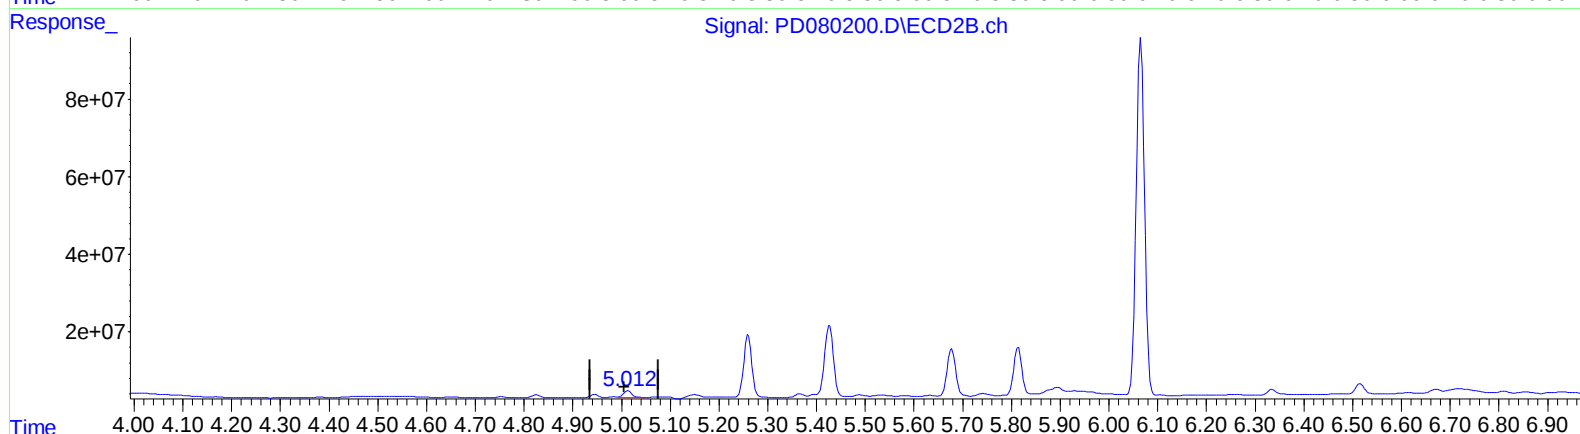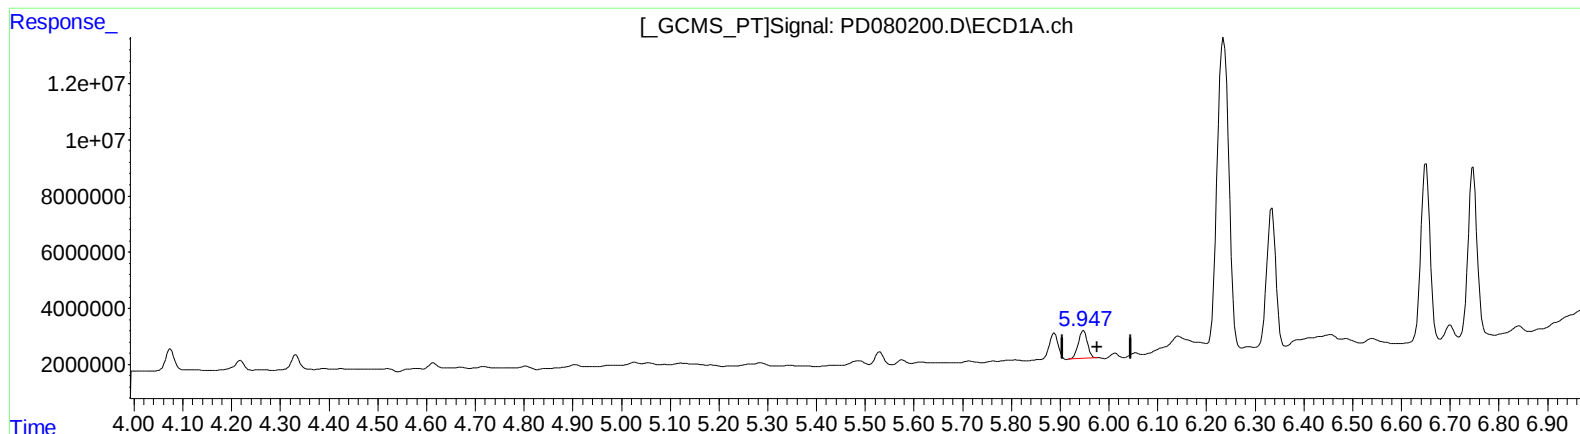

QEdit

(10) trans-Chlordane (B)

5.947min 6.226 ng/ml m

response 12776288

(10) trans-Chlordane #2 (B)

5.012min 6.419 ng/ml m

response 21130542

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD122023\  
Data File : PD080200.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 18 Dec 2023 17:52  
Operator : AR\AJ  
Sample : 05794-08DL2 20X  
Misc :  
ALS Vial : 21 Sample Multiplier: 1


Instrument :  
ECD\_D  
ClientSampleId :  
BH3Q2DL2

## Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 12/19/2023  
Supervised By :Ankita Jodhani 12/19/2023

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 19 00:49:41 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD121623CLP.M  
Quant Title : GC Extractables  
QLast Update : Mon Dec 18 00:44:33 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

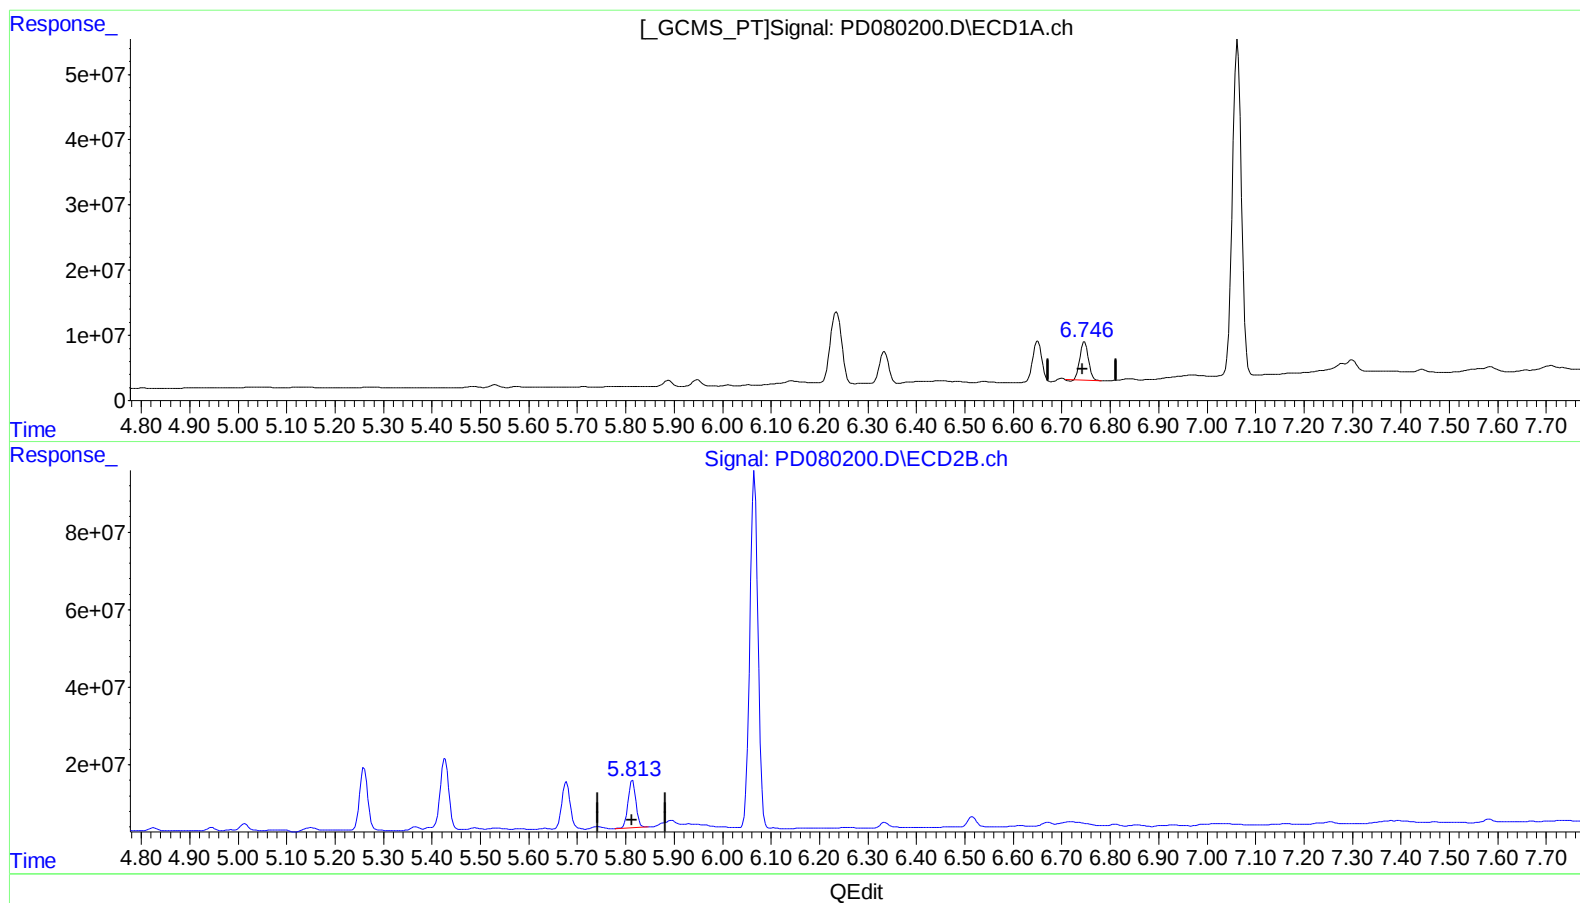

(16) 4,4'-DDD (A)  
6.747min 50.875 ng/ml  
response 70566579

(16) 4,4'-DDD #2 (A)  
5.814min 59.597 ng/ml  
response 137029297

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD122023\  
Data File : PD080200.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 18 Dec 2023 17:52  
Operator : AR\AJ  
Sample : 05794-08DL2 20X  
Misc :  
ALS Vial : 21 Sample Multiplier: 1


Instrument :  
ECD\_D  
ClientSampleId :  
BH3Q2DL2

## Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 12/19/2023  
Supervised By :Ankita Jodhani 12/19/2023

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 19 00:49:41 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD121623CLP.M  
Quant Title : GC Extractables  
QLast Update : Mon Dec 18 00:44:33 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

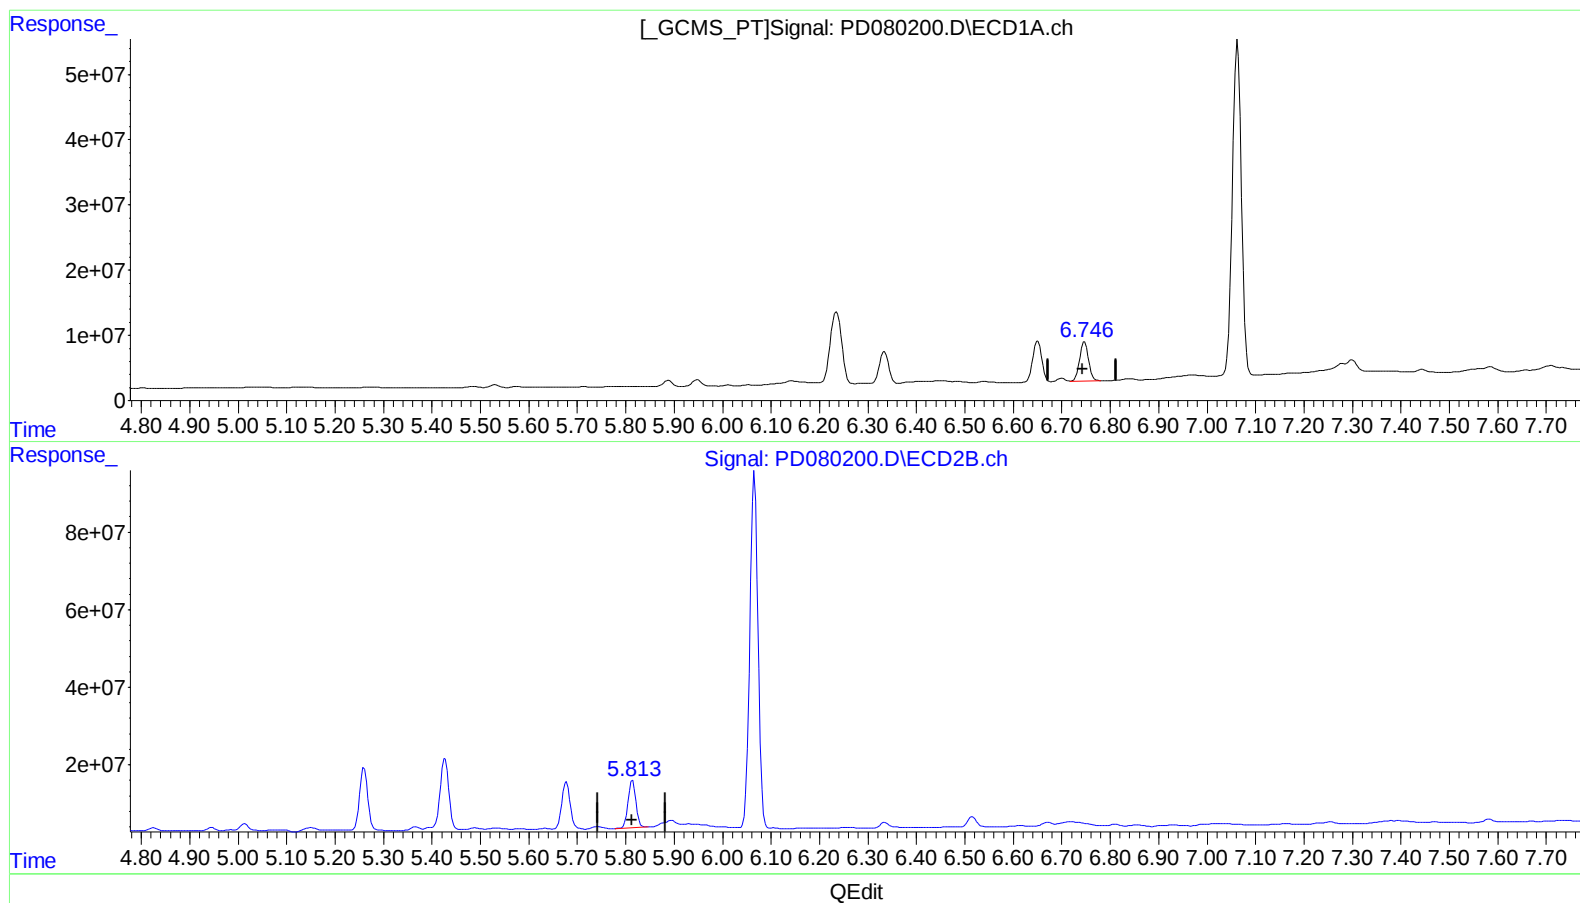

(16) 4,4'-DDD (A)  
6.746min 55.601 ng/ml m  
response 77122424

(16) 4,4'-DDD #2 (A)  
5.814min 59.597 ng/ml  
response 137029297