

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122023\
 Data File : PD080200.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2023 17:52
 Operator : AR\AJ
 Sample : 05794-08DL2 20X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH3Q2DL2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/19/2023
 Supervised By : Ankita Jodhani 12/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 00:49:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 18 00:44:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.567	2.800	1004440	3339061	0.787m	1.502 #
2) SA Decachlor...	9.097	7.942	4886955	3064416	3.040	1.277 #
Target Compounds						
10) B trans-Chl...	5.947	5.012	12776288	21130542	6.226m	6.419m
12) B 4,4'-DDE	6.235	5.260	180.5E6	185.4E6	93.441	59.022 #
16) A 4,4'-DDD	6.746	5.814	77122424	137.0E6	55.601m	59.597
17) MA 4,4'-DDT	7.063	6.066	655.2E6	1079.1E6	443.366	447.535

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122023\
Data File : PD080200.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2023 17:52
Operator : AR\AJ
Sample : 05794-08DL2 20X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 00:49:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Mon Dec 18 00:44:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

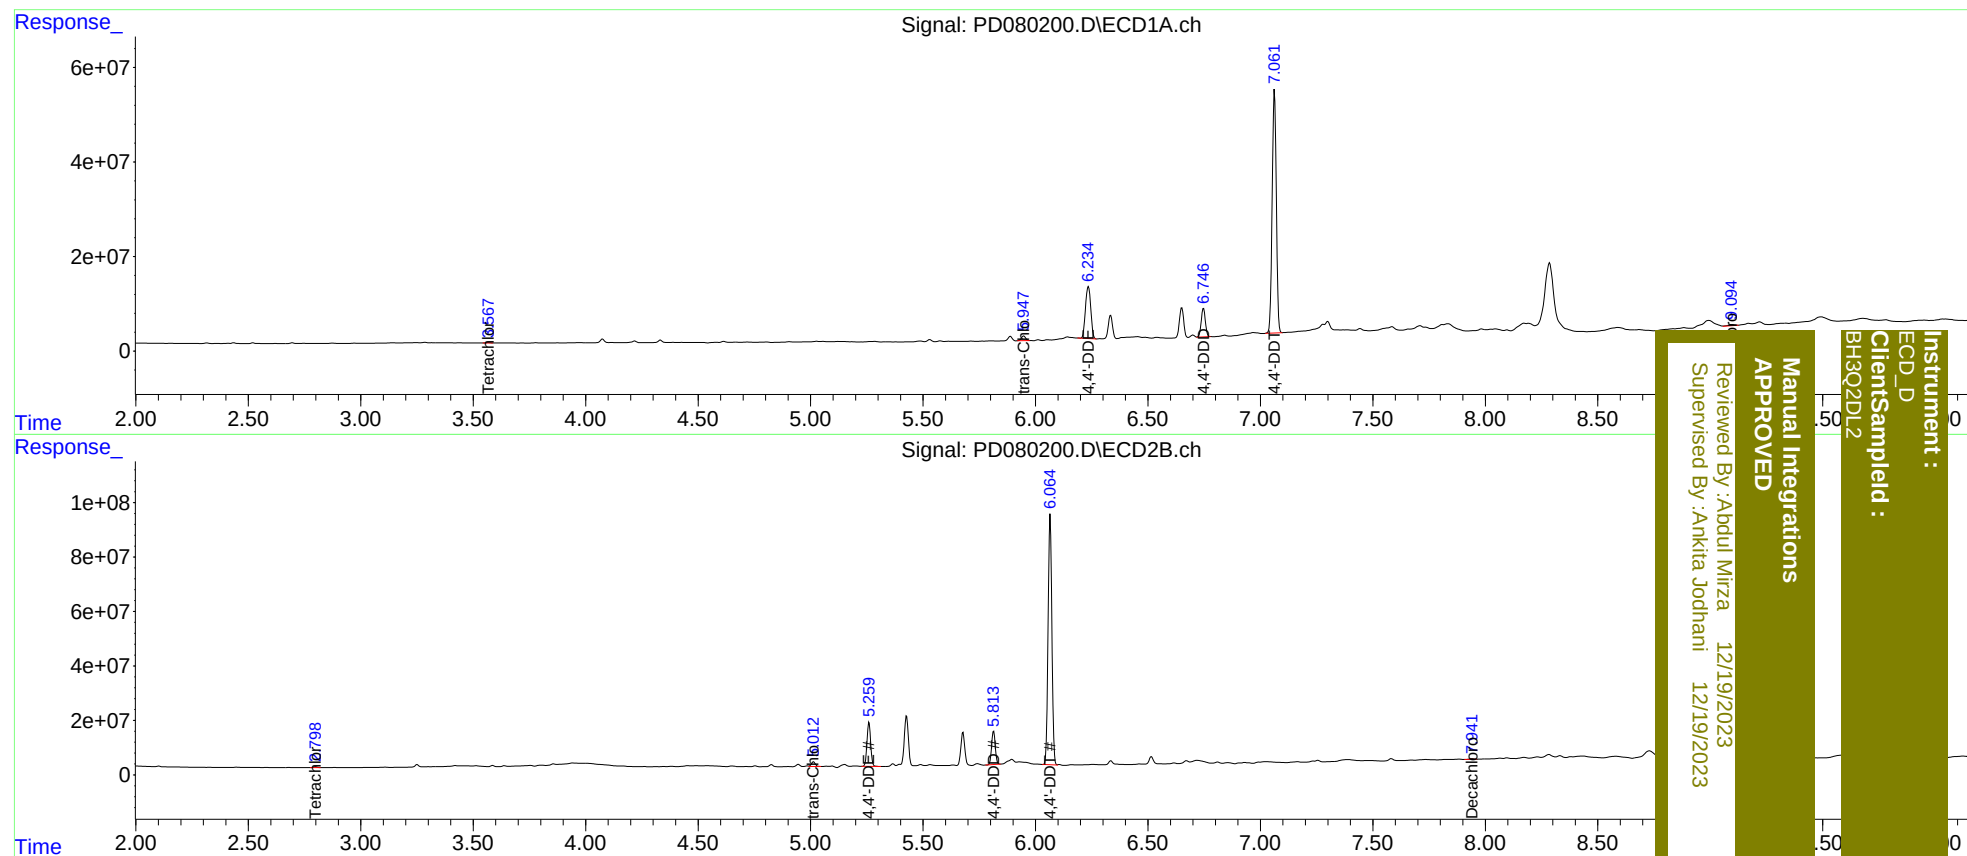

Instrument :
ECD_D
Client Sampled :
BH302DL2

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/19/2023
Supervised By :Ankita Jodhani 12/19/2023