

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122023\
 Data File : PD080202.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2023 18:18
 Operator : AR\AJ
 Sample : 05794-09DL 2X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH3Q3DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/20/2023
 Supervised By : Ankita Jodhani 12/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 00:50:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 18 00:44:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.568	2.801	7922223	23041318	6.205	10.362 #
2)	SA Decachlor...	9.103	7.942	18512592	30269337	11.515	12.611
Target Compounds							
9)	A Endosulfan I	6.139	5.153	43858026	123.8E6	24.620m	45.150m#
12)	B 4,4'-DDE	6.229	5.259	269.6E6	520.0E6	139.538	165.551m
16)	A 4,4'-DDD	6.743	5.813	55069623	63119668	39.702	27.452m#
17)	MA 4,4'-DDT	7.061	6.066	1580.2E6	2338.1E6	1069.316	969.710

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122023\
Data File : PD080202.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2023 18:18
Operator : AR\AJ
Sample : 05794-09DL 2X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 00:50:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Mon Dec 18 00:44:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

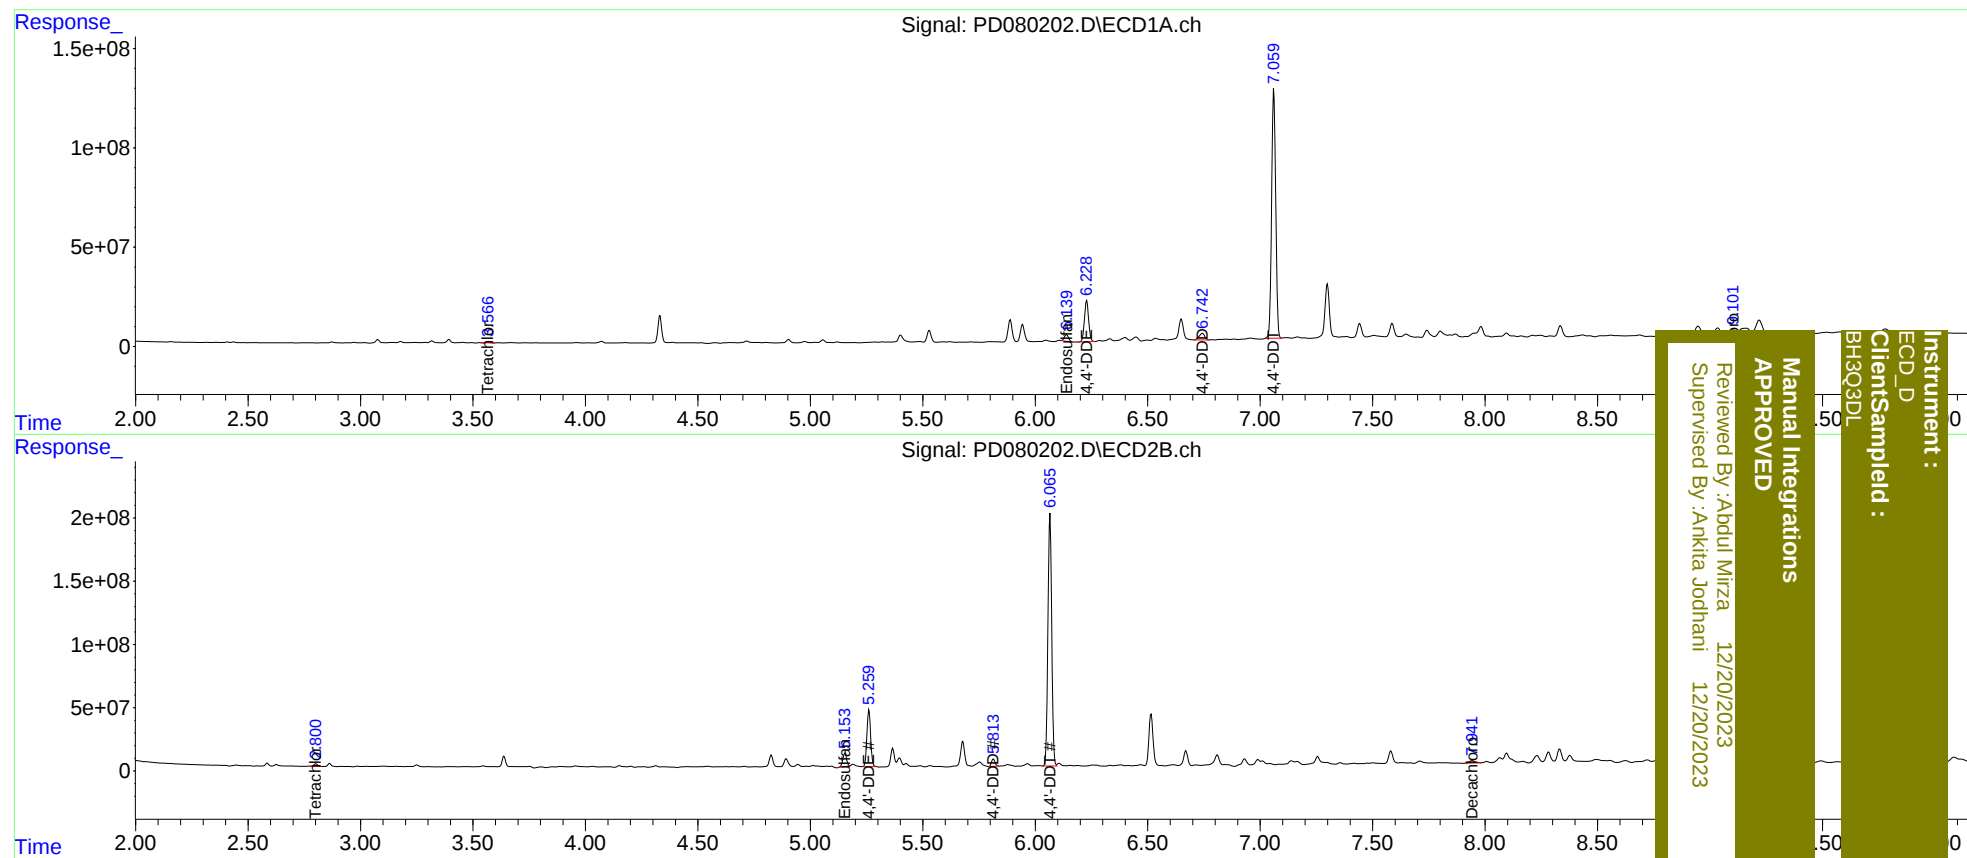

Instrument :
ECD_D
Client Sampled :
BH303DL
Manual Integrations
APPROVED
Reviewed By : Abdul Mirza 12/20/2023
Supervised By : Ankita Jodhani 12/20/2023