

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122024\
 Data File : PD087211.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2024 19:10
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 02:15:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122024CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 20 02:14:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.883	10454529	63201453	5.169	5.470
27)	SA Decachlor...	9.081	8.083	34163984	146.9E6	11.388	11.300
Target Compounds							
2)	A alpha-BHC	4.004	3.396	18256393	94665316	4.638	5.212
3)	MA gamma-BHC...	4.335	3.733	18211953	89390821	4.774	5.306
4)	MA Heptachlor	4.936	4.088	19123521	93654823	4.922	5.434
9)	A Endosulfan I	6.080	5.254	16723609	78937137	5.090	5.462
13)	MA Dieldrin	6.353	5.520	33944833	164.6E6	9.550	10.787
14)	MA Endrin	6.580	5.797	28317247	152.4E6	9.735	11.082
16)	A 4,4'-DDD	6.710	5.938	24259273	130.6E6	9.516	10.742
17)	MA 4,4'-DDT	7.027	6.192	25019360	130.8E6	9.495	10.358
20)	A Methoxychlor	7.499	6.763	75687768	340.8E6	51.353	58.099


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122024\
Data File : PD087211.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2024 19:10
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 02:15:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122024CLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 02:14:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

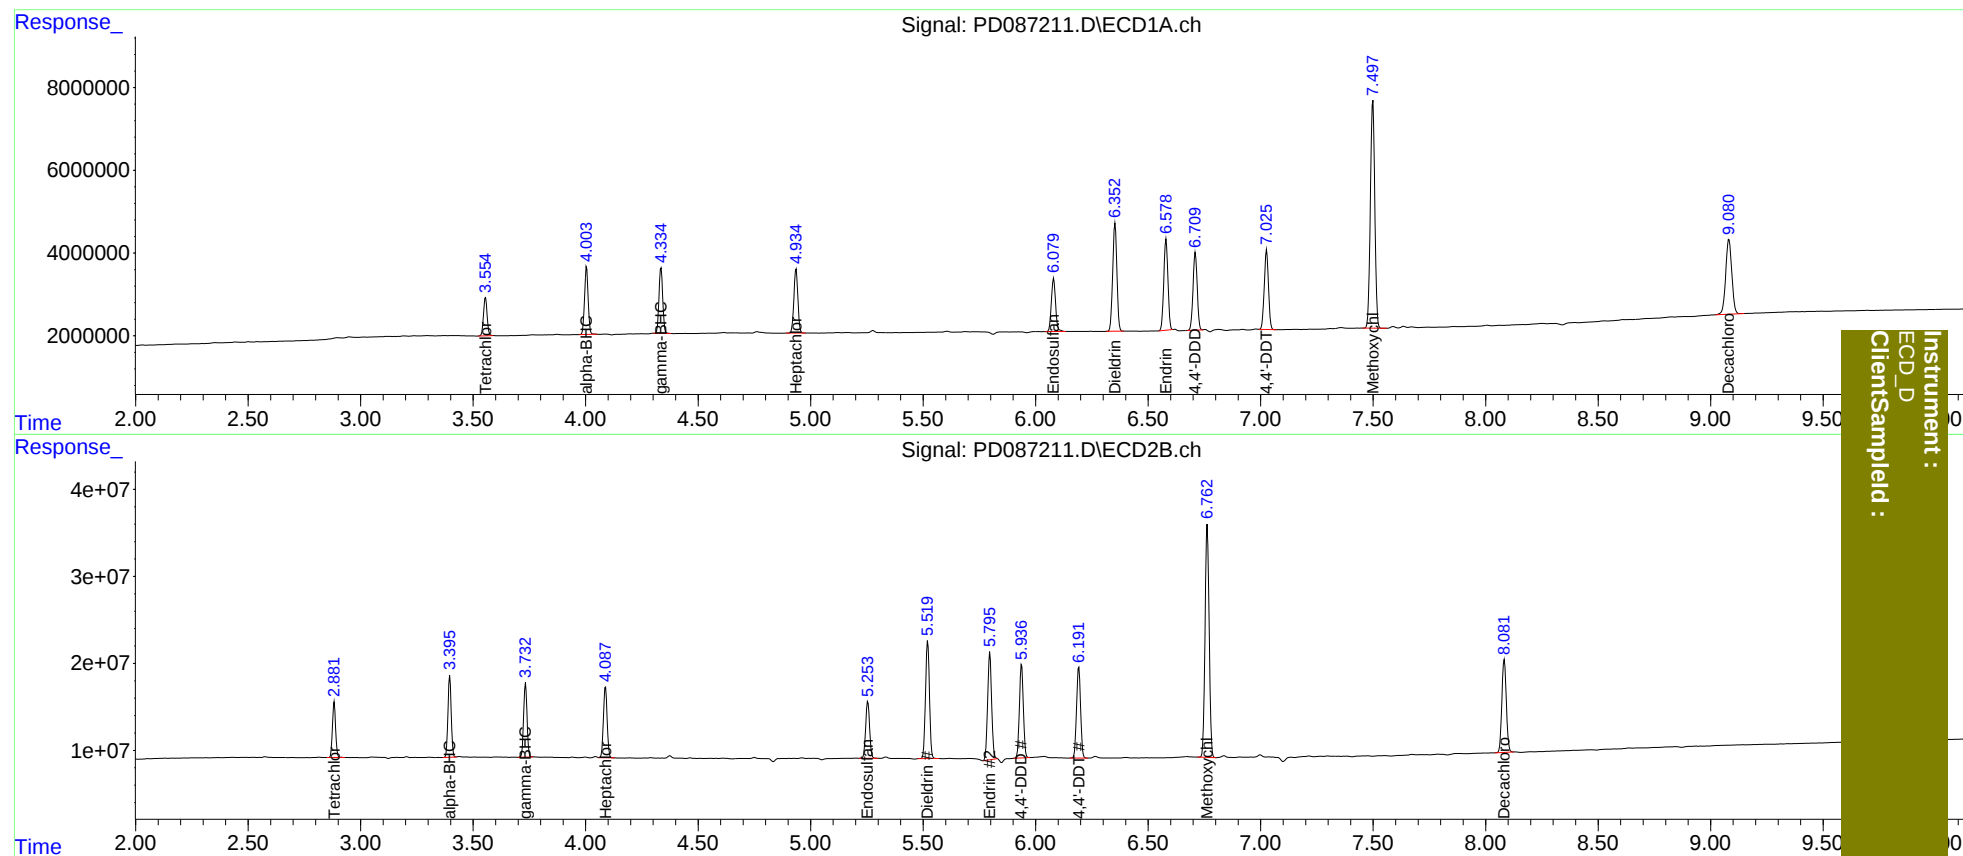


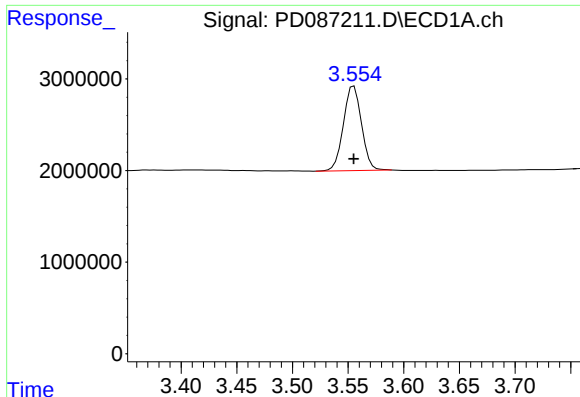

#1 Tetrachloro-m-xylene


R.T.: 3.555 min
Delta R.T.: 0.000 min
Response: 10454529
Conc: 5.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

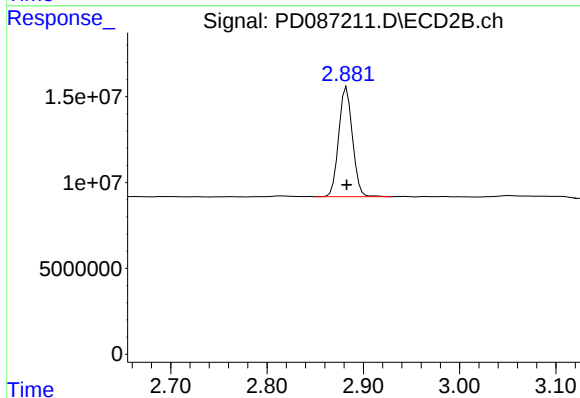


#1 Tetrachloro-m-xylene

R.T.: 2.883 min
Delta R.T.: 0.000 min
Response: 63201453
Conc: 5.47 ng/ml

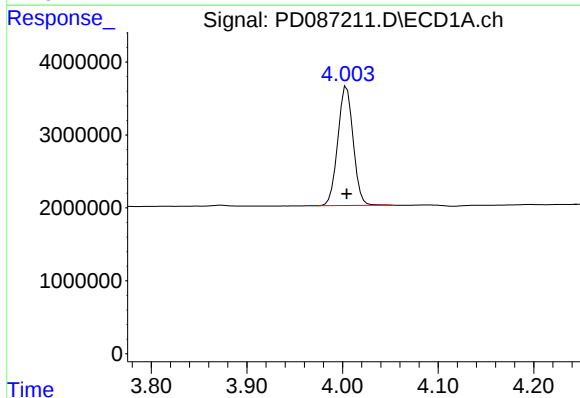


#2 alpha-BHC

R.T.: 4.004 min
Delta R.T.: 0.000 min
Response: 18256393
Conc: 4.64 ng/ml

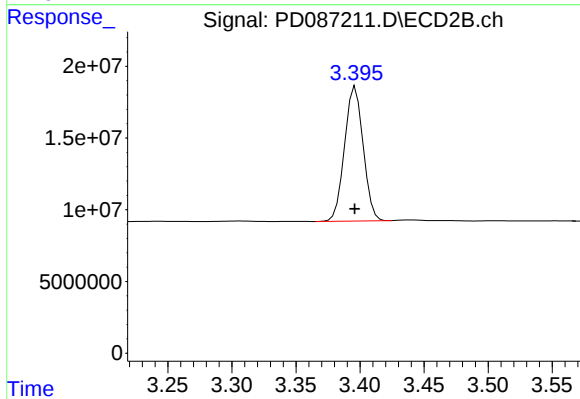

#2 alpha-BHC


R.T.: 3.396 min
Delta R.T.: 0.000 min
Response: 94665316
Conc: 5.21 ng/ml

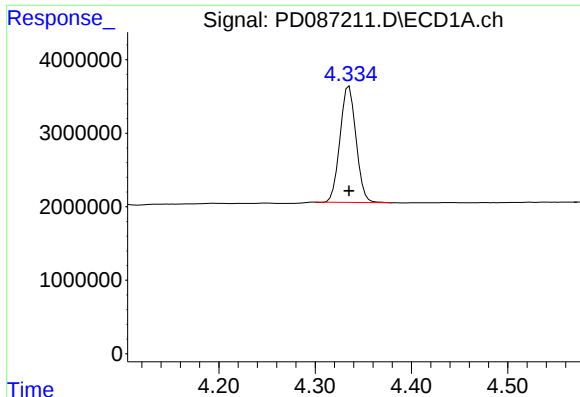

#3 gamma-BHC (Lindane)


R.T.: 4.335 min
Delta R.T.: 0.000 min
Response: 18211953
Conc: 4.77 ng/ml

Instrument :
ECD_D
ClientSampleId :

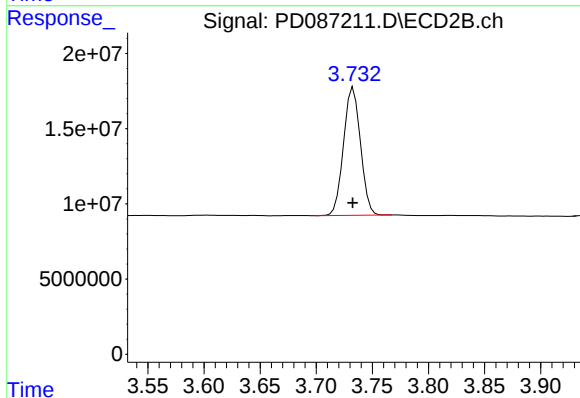


#3 gamma-BHC (Lindane)

R.T.: 3.733 min
Delta R.T.: 0.000 min
Response: 89390821
Conc: 5.31 ng/ml

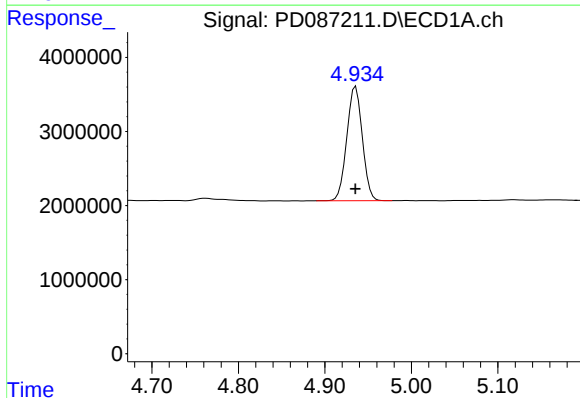


#4 Heptachlor

R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 19123521
Conc: 4.92 ng/ml

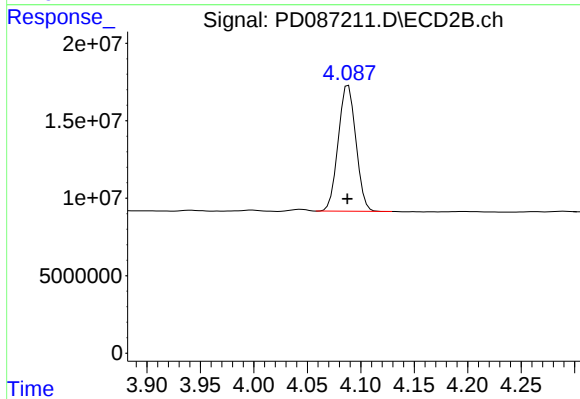

#4 Heptachlor


R.T.: 4.088 min
Delta R.T.: 0.000 min
Response: 93654823
Conc: 5.43 ng/ml

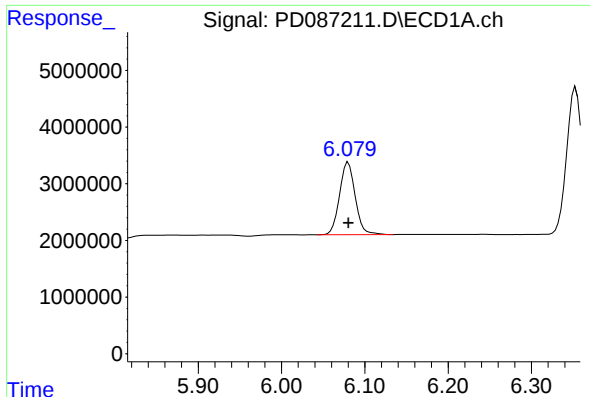

#9 Endosulfan I


R.T.: 6.080 min
Delta R.T.: 0.000 min
Response: 16723609
Conc: 5.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

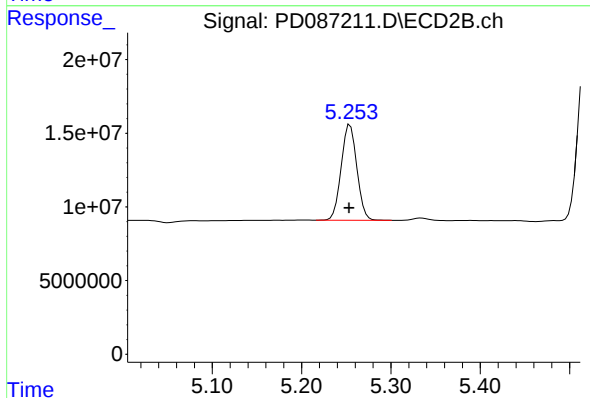


#9 Endosulfan I

R.T.: 5.254 min
Delta R.T.: 0.001 min
Response: 78937137
Conc: 5.46 ng/ml

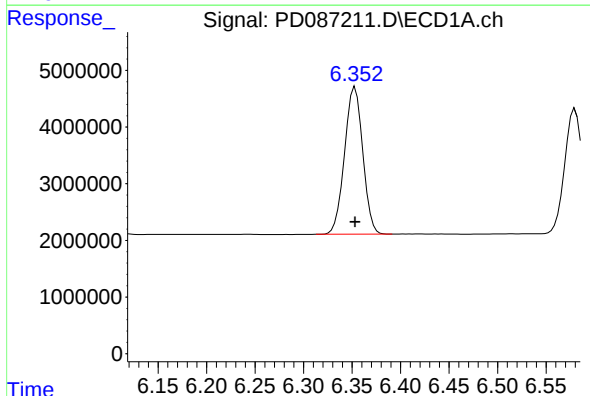


#13 Dieldrin

R.T.: 6.353 min
Delta R.T.: 0.000 min
Response: 33944833
Conc: 9.55 ng/ml

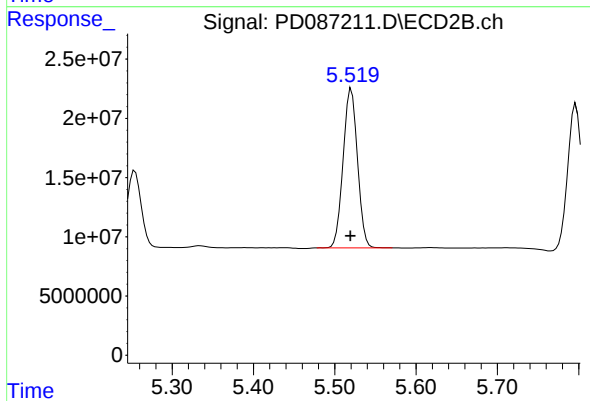

#13 Dieldrin


R.T.: 5.520 min
Delta R.T.: 0.001 min
Response: 164587273
Conc: 10.79 ng/ml

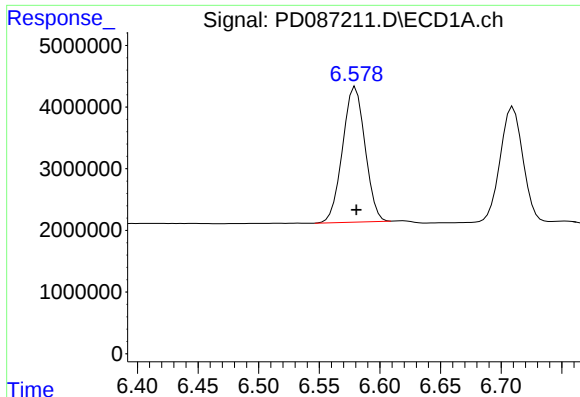

#14 Endrin


R.T.: 6.580 min
Delta R.T.: 0.000 min
Response: 28317247
Conc: 9.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

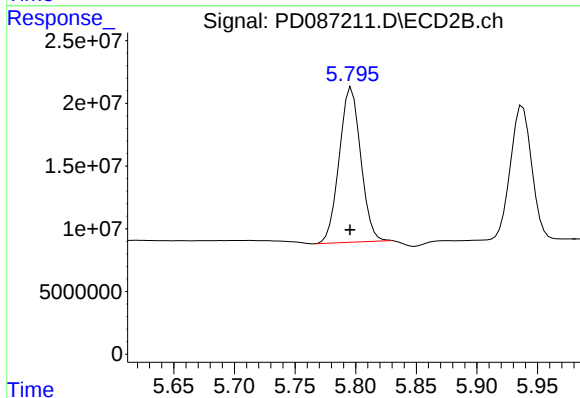


#14 Endrin

R.T.: 5.797 min
Delta R.T.: 0.001 min
Response: 152434773
Conc: 11.08 ng/ml

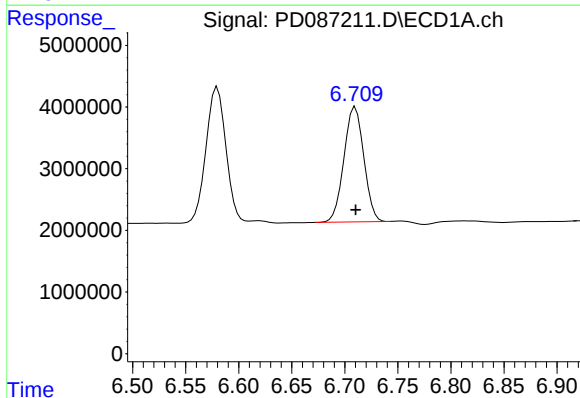


#16 4,4'-DDD

R.T.: 6.710 min
Delta R.T.: 0.000 min
Response: 24259273
Conc: 9.52 ng/ml

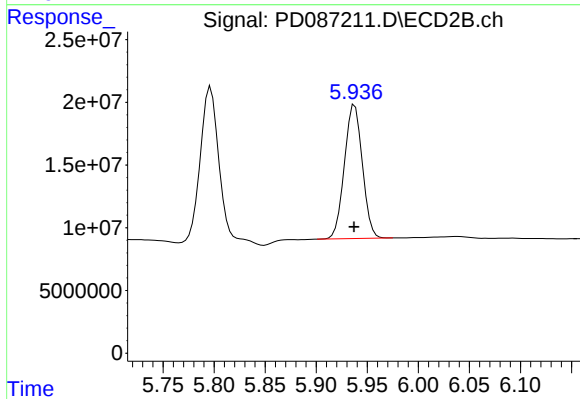

#16 4,4'-DDD


R.T.: 5.938 min
Delta R.T.: 0.000 min
Response: 130563890
Conc: 10.74 ng/ml

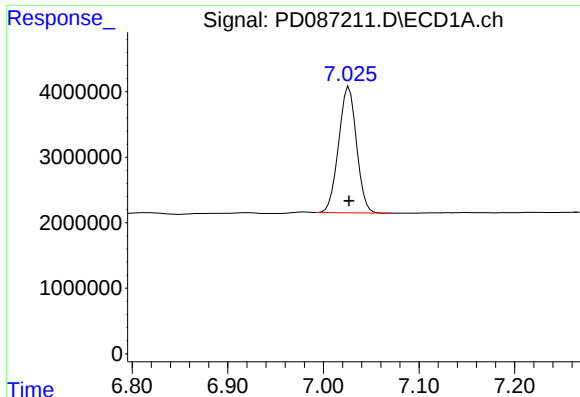

#17 4,4'-DDT


R.T.: 7.027 min
Delta R.T.: 0.000 min
Response: 25019360
Conc: 9.49 ng/ml

Instrument :
ECD_D
ClientSampleId :

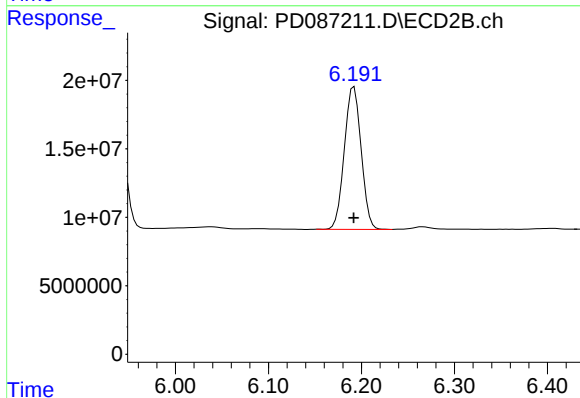


#17 4,4'-DDT

R.T.: 6.192 min
Delta R.T.: 0.000 min
Response: 130799243
Conc: 10.36 ng/ml

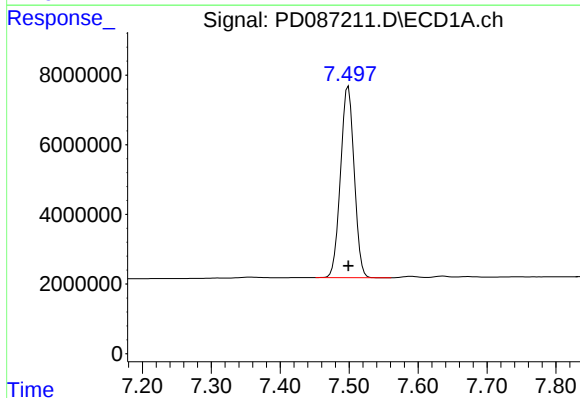


#20 Methoxychlor

R.T.: 7.499 min
Delta R.T.: 0.000 min
Response: 75687768
Conc: 51.35 ng/ml

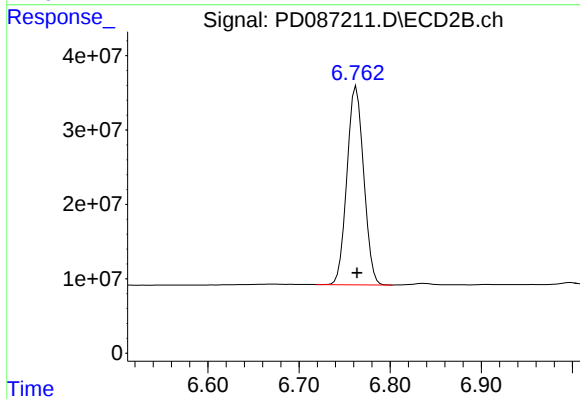

#20 Methoxychlor


R.T.: 6.763 min
Delta R.T.: 0.000 min
Response: 340808910
Conc: 58.10 ng/ml

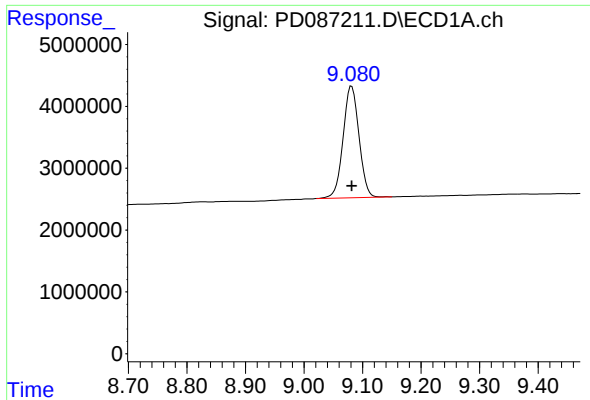

#27 Decachlorobiphenyl

R.T.: 9.081 min
Delta R.T.: 0.000 min
Response: 34163984
Conc: 11.39 ng/ml

Instrument :
ECD_D
ClientSampleId :

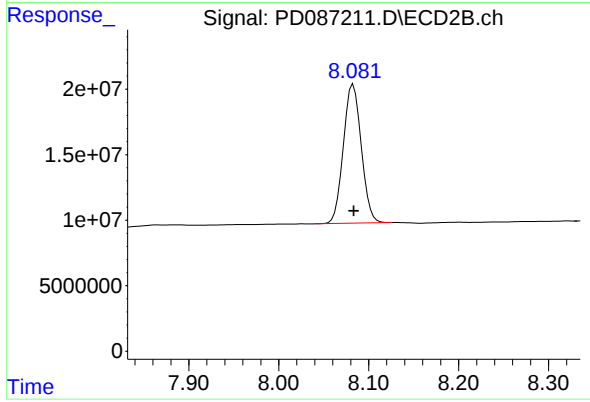

#27 Decachlorobiphenyl

R.T.: 8.083 min
Delta R.T.: 0.000 min
Response: 146861320
Conc: 11.30 ng/ml