

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122024\
 Data File : PD087213.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2024 19:38
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 02:15:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122024CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 20 02:14:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.883	21046384	124.0E6	10.407	10.728
27)	SA Decachlor...	9.081	8.084	64133849	280.6E6	21.377	21.589
Target Compounds							
2)	A alpha-BHC	4.004	3.396	38257081	189.3E6	9.718	10.421
3)	MA gamma-BHC...	4.335	3.733	37717790	176.2E6	9.887	10.461
4)	MA Heptachlor	4.935	4.088	39120420	183.3E6	10.068	10.638
9)	A Endosulfan I	6.081	5.253	33856581	154.5E6	10.306	10.689
13)	MA Dieldrin	6.353	5.520	70588233	323.3E6	19.859	21.190
14)	MA Endrin	6.581	5.796	58409881	294.6E6	20.081	21.420
16)	A 4,4'-DDD	6.711	5.937	50523356	258.2E6	19.819	21.243
17)	MA 4,4'-DDT	7.027	6.192	52134902	263.4E6	19.785	20.858
20)	A Methoxychlor	7.499	6.764	151.6E6	645.6E6	102.888	110.058


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122024\
Data File : PD087213.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2024 19:38
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 02:15:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122024CLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 02:14:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

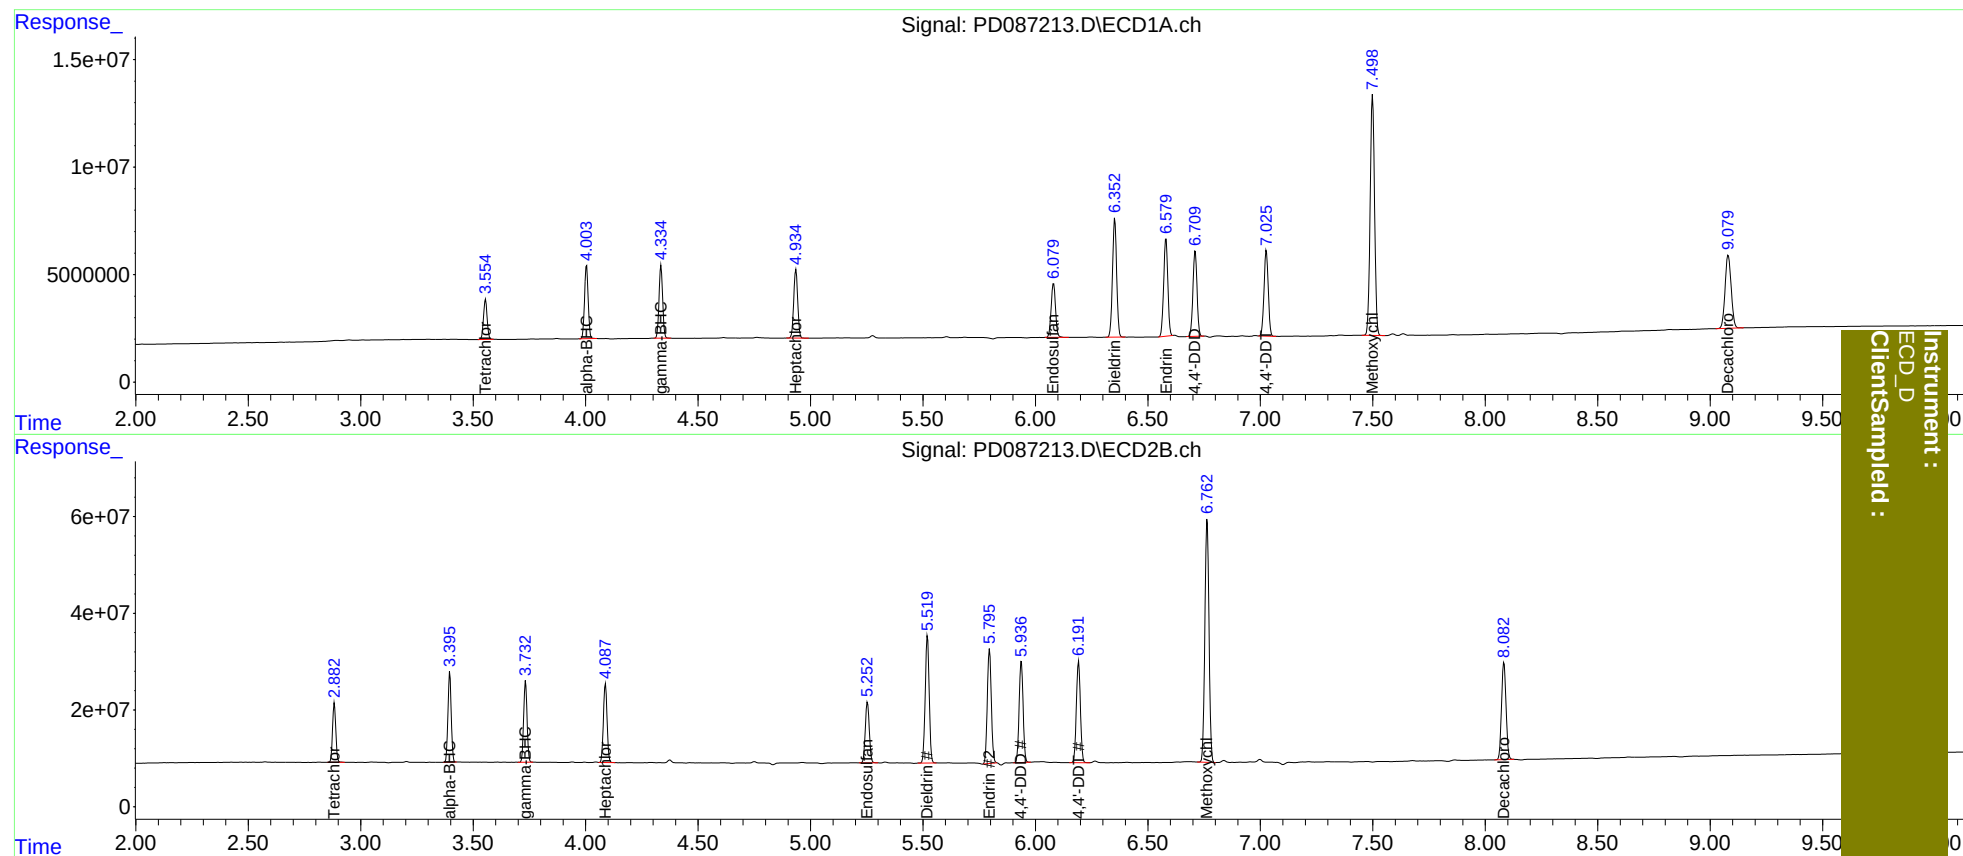


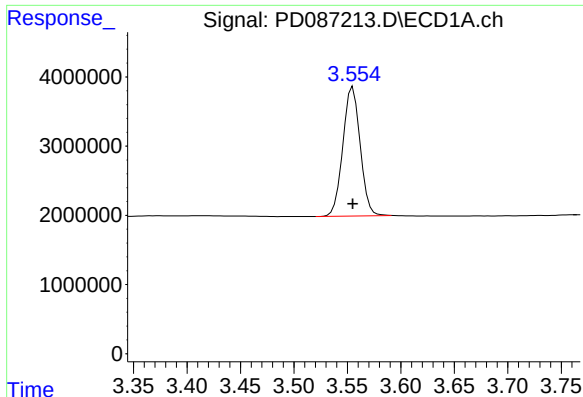

#1 Tetrachloro-m-xylene


R.T.: 3.555 min
Delta R.T.: 0.000 min
Response: 21046384
Conc: 10.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

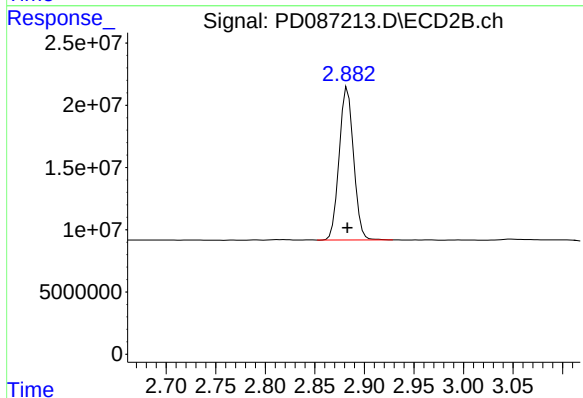


#1 Tetrachloro-m-xylene

R.T.: 2.883 min
Delta R.T.: 0.000 min
Response: 123954742
Conc: 10.73 ng/ml

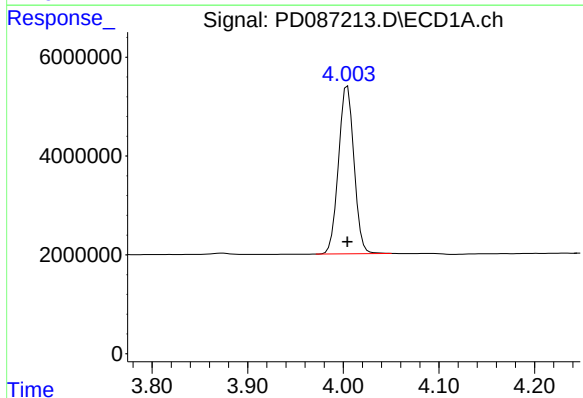


#2 alpha-BHC

R.T.: 4.004 min
Delta R.T.: 0.000 min
Response: 38257081
Conc: 9.72 ng/ml

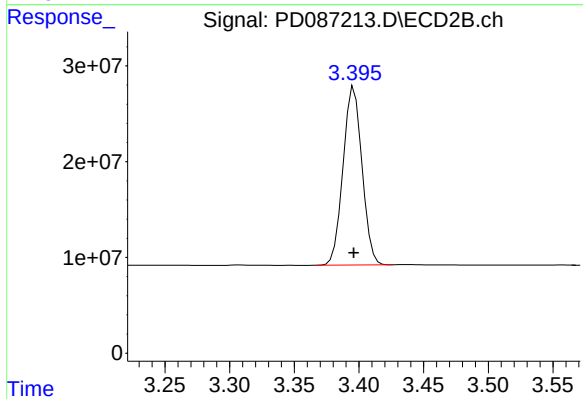

#2 alpha-BHC


R.T.: 3.396 min
Delta R.T.: 0.000 min
Response: 189300530
Conc: 10.42 ng/ml

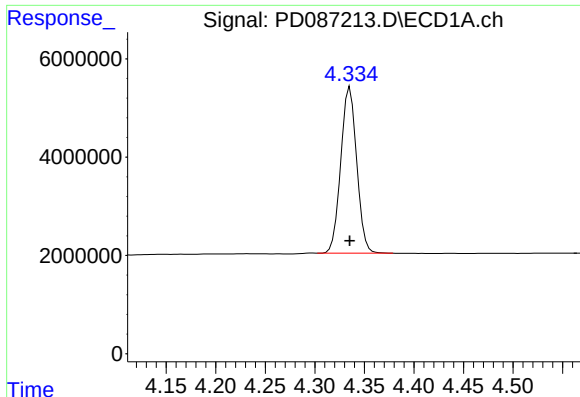

#3 gamma-BHC (Lindane)


R.T.: 4.335 min
Delta R.T.: 0.000 min
Response: 37717790
Conc: 9.89 ng/ml

Instrument :
ECD_D
ClientSampleId :

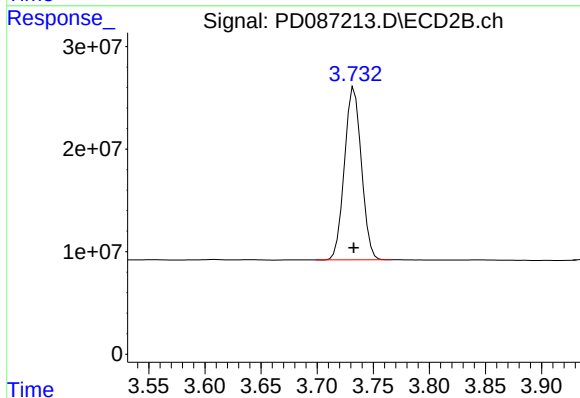


#3 gamma-BHC (Lindane)

R.T.: 3.733 min
Delta R.T.: 0.000 min
Response: 176240288
Conc: 10.46 ng/ml

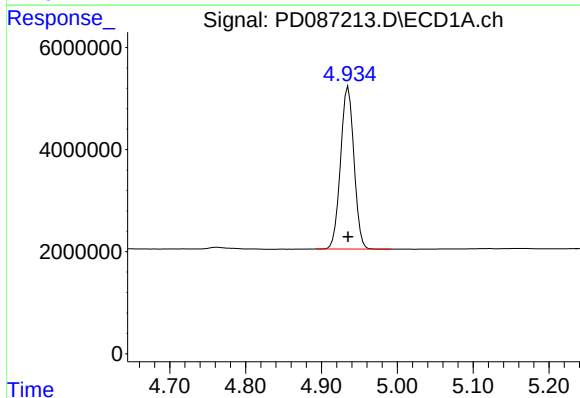


#4 Heptachlor

R.T.: 4.935 min
Delta R.T.: 0.000 min
Response: 39120420
Conc: 10.07 ng/ml

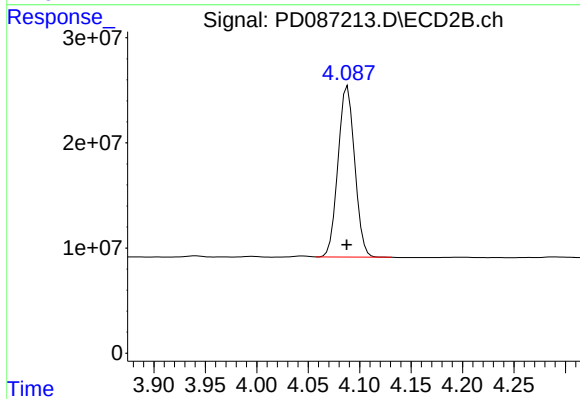

#4 Heptachlor


R.T.: 4.088 min
Delta R.T.: 0.000 min
Response: 183348316
Conc: 10.64 ng/ml

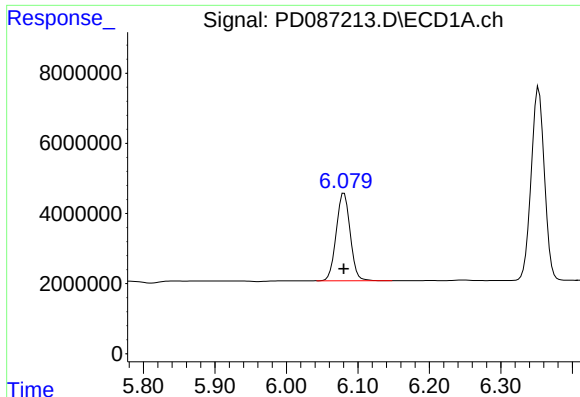

#9 Endosulfan I


R.T.: 6.081 min
Delta R.T.: 0.000 min
Response: 33856581
Conc: 10.31 ng/ml

Instrument :
ECD_D
ClientSampleId :

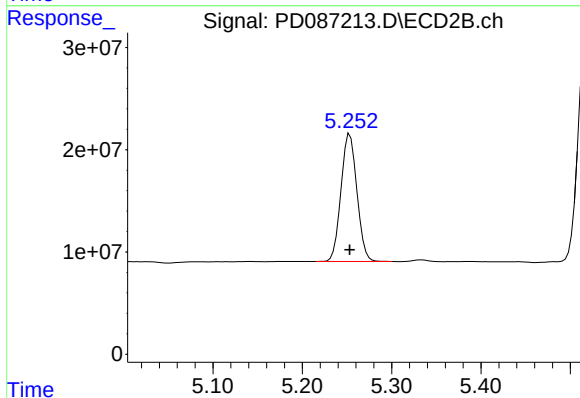


#9 Endosulfan I

R.T.: 5.253 min
Delta R.T.: 0.000 min
Response: 154460665
Conc: 10.69 ng/ml

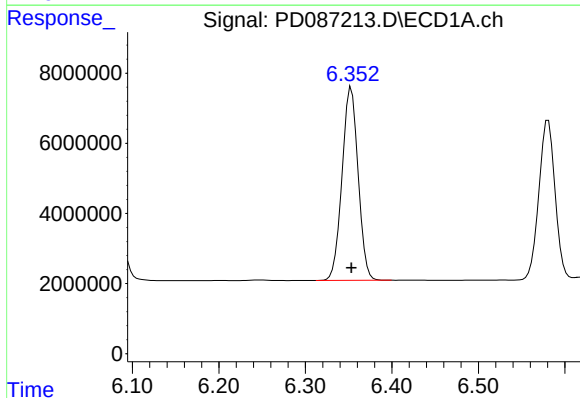


#13 Dieldrin

R.T.: 6.353 min
Delta R.T.: 0.000 min
Response: 70588233
Conc: 19.86 ng/ml

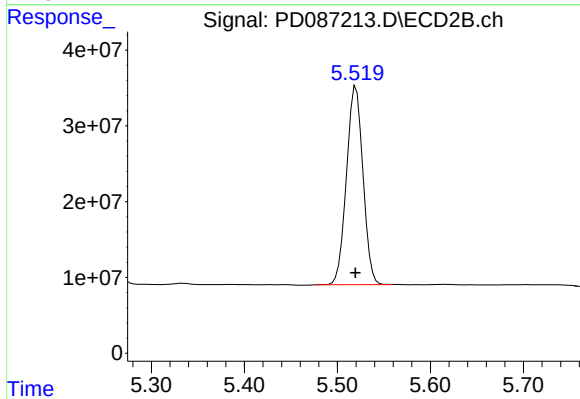

#13 Dieldrin


R.T.: 5.520 min
Delta R.T.: 0.000 min
Response: 323315153
Conc: 21.19 ng/ml

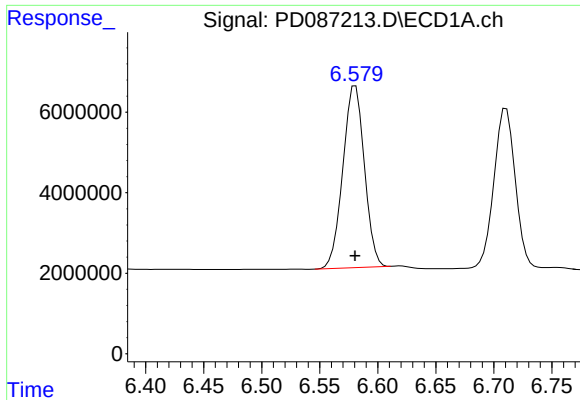

#14 Endrin


R.T.: 6.581 min
Delta R.T.: 0.000 min
Response: 58409881
Conc: 20.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

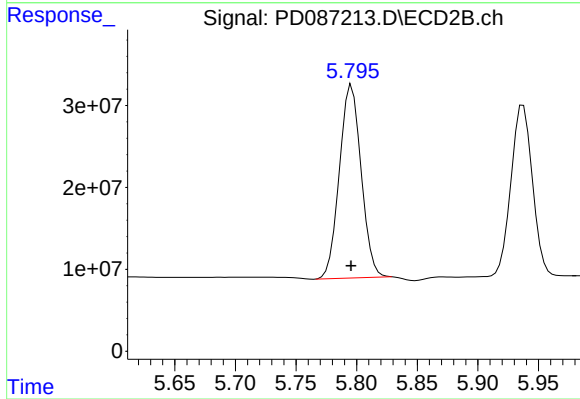


#14 Endrin

R.T.: 5.796 min
Delta R.T.: 0.000 min
Response: 294636378
Conc: 21.42 ng/ml

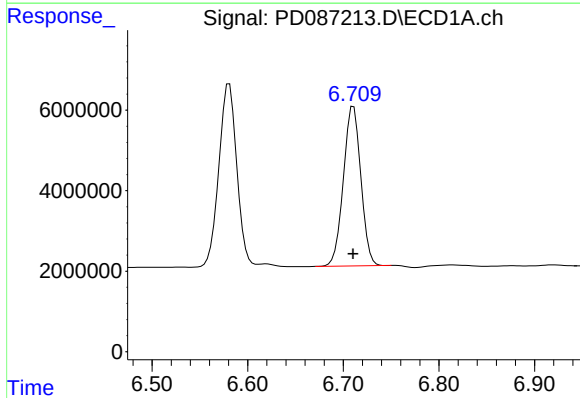


#16 4,4'-DDD

R.T.: 6.711 min
Delta R.T.: 0.000 min
Response: 50523356
Conc: 19.82 ng/ml

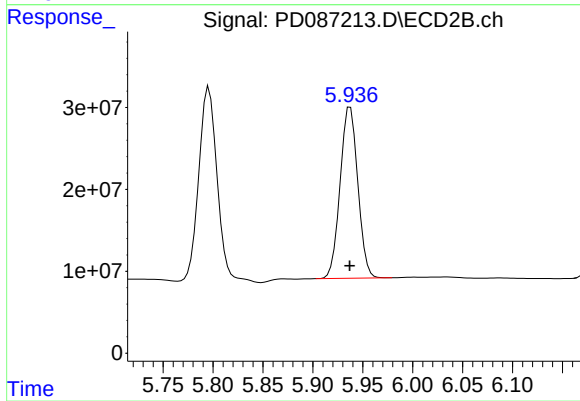

#16 4,4'-DDD


R.T.: 5.937 min
Delta R.T.: 0.000 min
Response: 258189455
Conc: 21.24 ng/ml

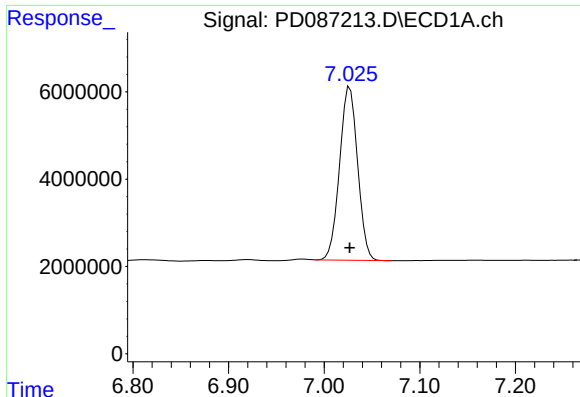

#17 4,4'-DDT


R.T.: 7.027 min
Delta R.T.: 0.000 min
Response: 52134902
Conc: 19.78 ng/ml

Instrument :
ECD_D
ClientSampleId :

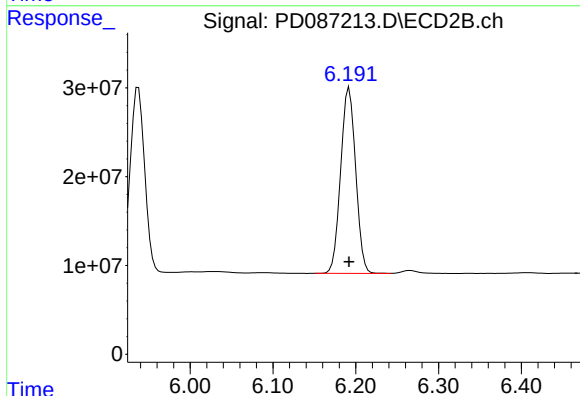


#17 4,4'-DDT

R.T.: 6.192 min
Delta R.T.: 0.000 min
Response: 263388983
Conc: 20.86 ng/ml

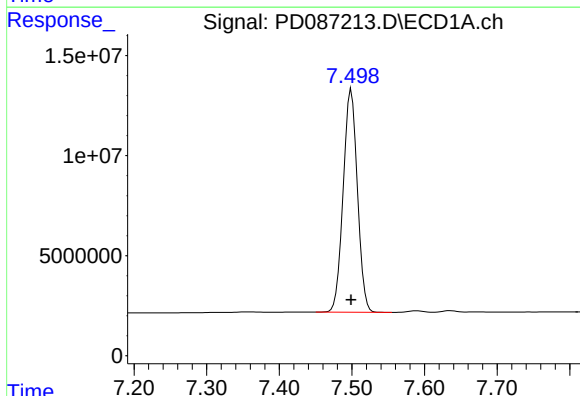


#20 Methoxychlor

R.T.: 7.499 min
Delta R.T.: 0.000 min
Response: 151644285
Conc: 102.89 ng/ml

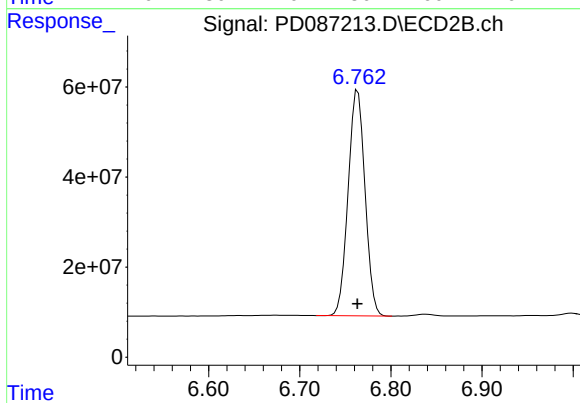

#20 Methoxychlor


R.T.: 6.764 min
Delta R.T.: 0.000 min
Response: 645602815
Conc: 110.06 ng/ml

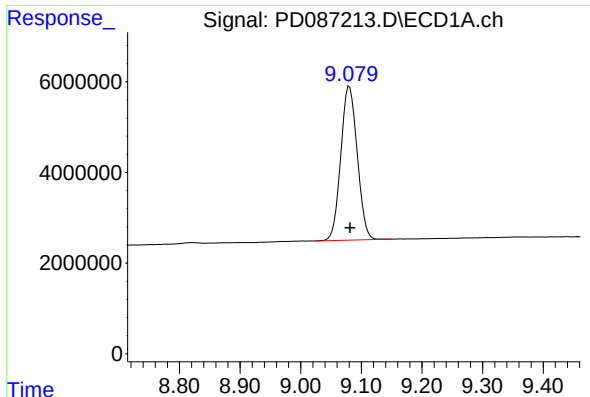

#27 Decachlorobiphenyl

R.T.: 9.081 min
Delta R.T.: 0.000 min
Response: 64133849
Conc: 21.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

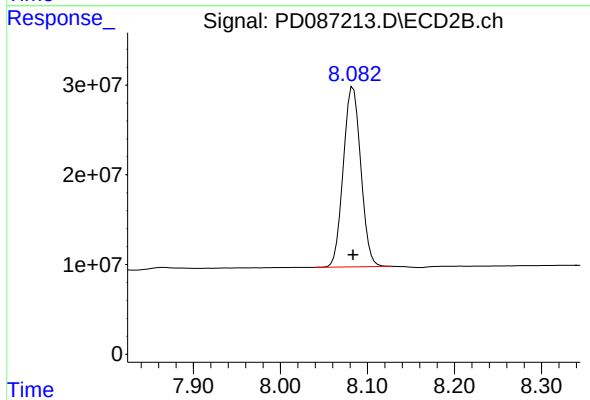

#27 Decachlorobiphenyl

R.T.: 8.084 min
Delta R.T.: 0.000 min
Response: 280574098
Conc: 21.59 ng/ml