

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122024\
 Data File : PD087215.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2024 20:06
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 02:15:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122024CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 20 02:14:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.883	40448447	231.1E6	20.000	20.000
27)	SA Decachlor...	9.081	8.084	120.0E6	519.9E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	4.004	3.396	78732434	363.3E6	20.000	20.000
3)	MA gamma-BHC...	4.335	3.733	76299718	336.9E6	20.000	20.000
4)	MA Heptachlor	4.935	4.087	77711372	344.7E6	20.000	20.000
9)	A Endosulfan I	6.080	5.253	65705654	289.0E6	20.000	20.000
13)	MA Dieldrin	6.353	5.519	142.2E6	610.3E6	40.000	40.000
14)	MA Endrin	6.581	5.796	116.3E6	550.2E6	40.000	40.000
16)	A 4,4'-DDD	6.710	5.937	102.0E6	486.2E6	40.000	40.000
17)	MA 4,4'-DDT	7.027	6.192	105.4E6	505.1E6	40.000	40.000
20)	A Methoxychlor	7.499	6.763	294.8E6	1173.2E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122024\
Data File : PD087215.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2024 20:06
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 02:15:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122024CLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 02:14:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

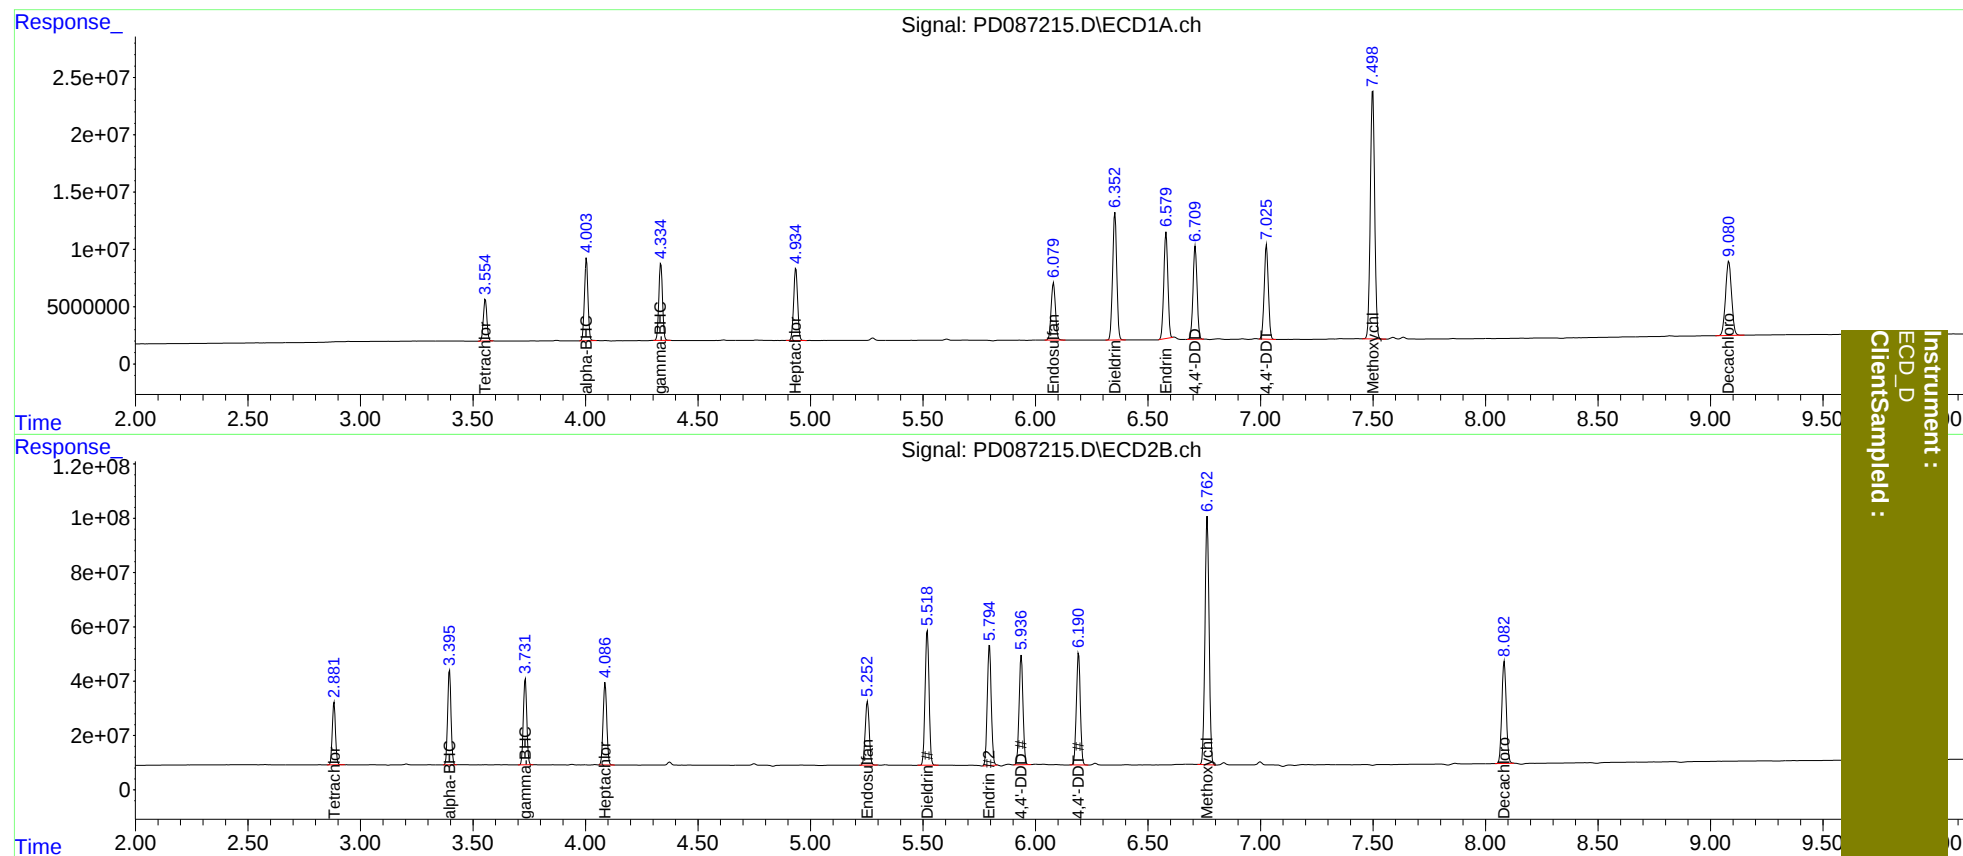


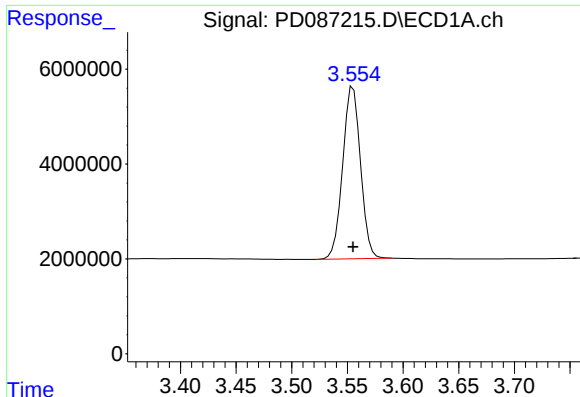

#1 Tetrachloro-m-xylene


R.T.: 3.555 min
Delta R.T.: 0.000 min
Response: 40448447
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

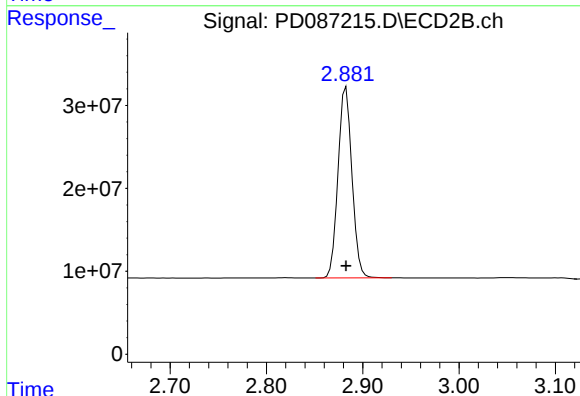


#1 Tetrachloro-m-xylene

R.T.: 2.883 min
Delta R.T.: 0.000 min
Response: 231086864
Conc: 20.00 ng/ml

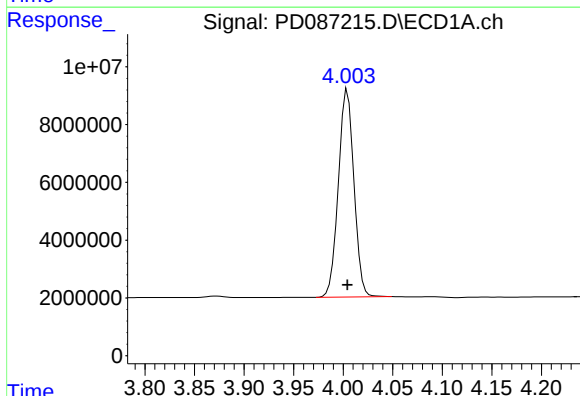


#2 alpha-BHC

R.T.: 4.004 min
Delta R.T.: 0.000 min
Response: 78732434
Conc: 20.00 ng/ml

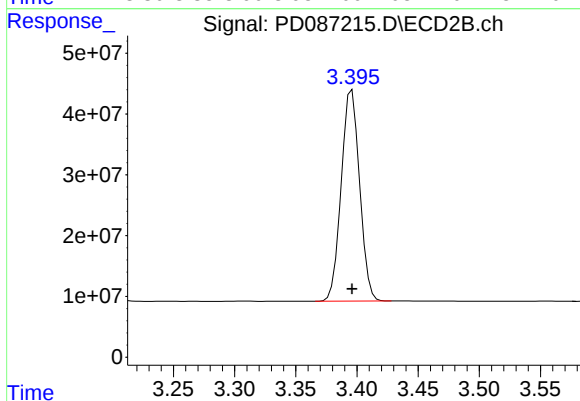

#2 alpha-BHC


R.T.: 3.396 min
Delta R.T.: 0.000 min
Response: 363293861
Conc: 20.00 ng/ml

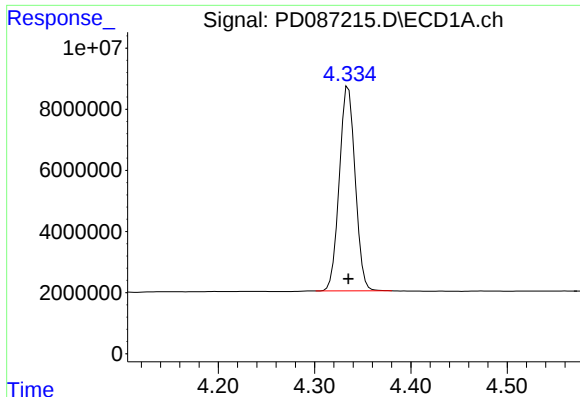

#3 gamma-BHC (Lindane)


R.T.: 4.335 min
Delta R.T.: 0.000 min
Response: 76299718
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

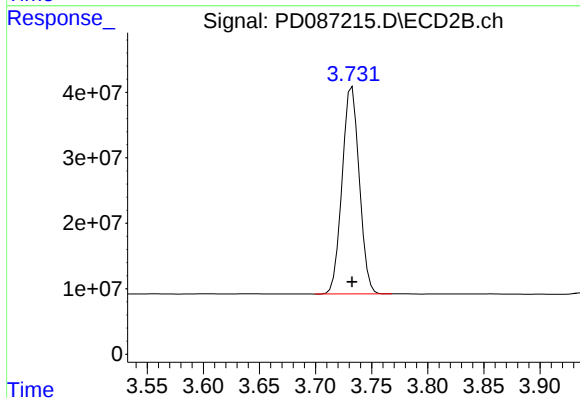


#3 gamma-BHC (Lindane)

R.T.: 3.733 min
Delta R.T.: 0.000 min
Response: 336933496
Conc: 20.00 ng/ml

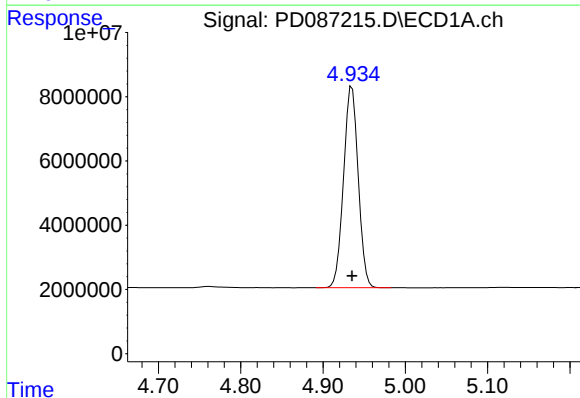


#4 Heptachlor

R.T.: 4.935 min
Delta R.T.: 0.000 min
Response: 77711372
Conc: 20.00 ng/ml

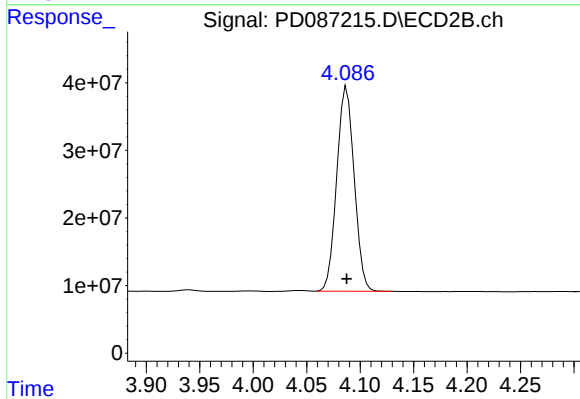

#4 Heptachlor


R.T.: 4.087 min
Delta R.T.: 0.000 min
Response: 344688520
Conc: 20.00 ng/ml

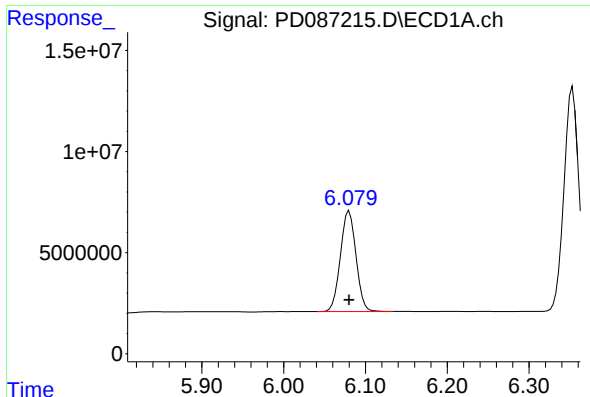

#9 Endosulfan I


R.T.: 6.080 min
Delta R.T.: 0.000 min
Response: 65705654
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

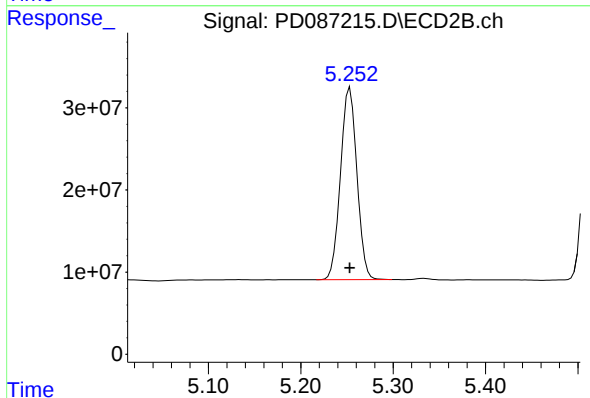


#9 Endosulfan I

R.T.: 5.253 min
Delta R.T.: 0.000 min
Response: 289020702
Conc: 20.00 ng/ml

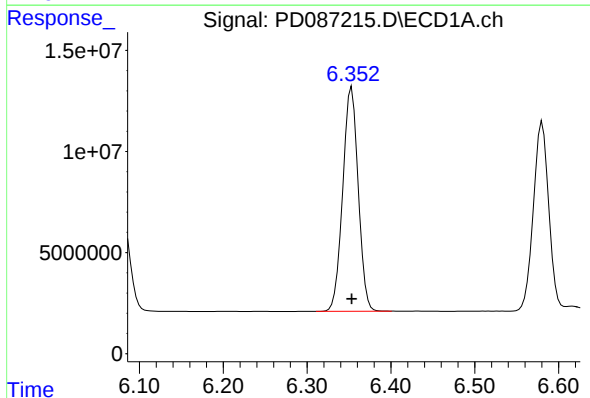


#13 Dieldrin

R.T.: 6.353 min
Delta R.T.: 0.000 min
Response: 142175651
Conc: 40.00 ng/ml

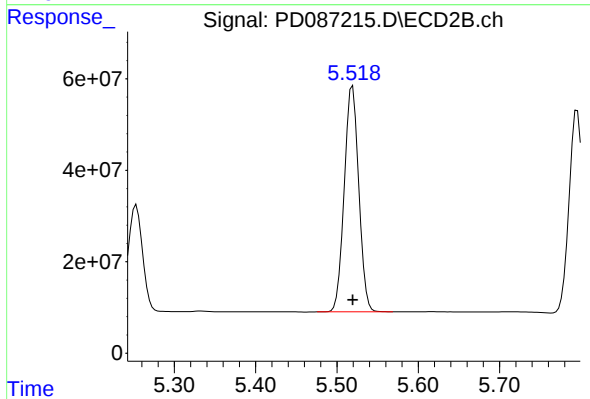

#13 Dieldrin


R.T.: 5.519 min
Delta R.T.: 0.000 min
Response: 610310270
Conc: 40.00 ng/ml

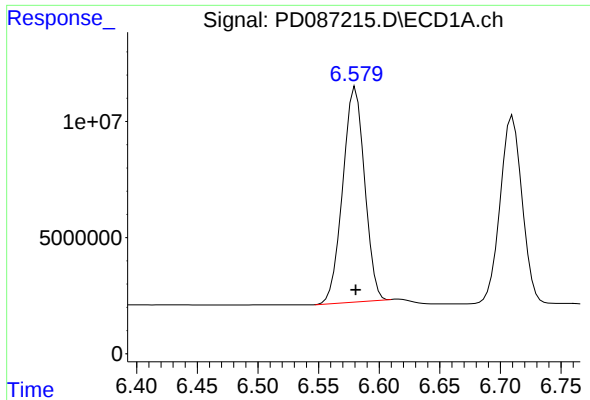

#14 Endrin


R.T.: 6.581 min
Delta R.T.: 0.000 min
Response: 116347802
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

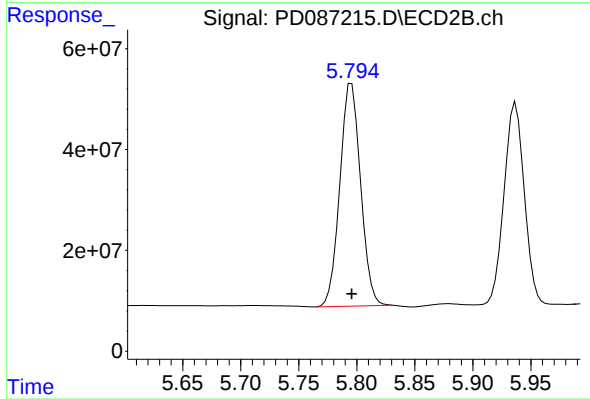


#14 Endrin

R.T.: 5.796 min
Delta R.T.: 0.000 min
Response: 550202683
Conc: 40.00 ng/ml

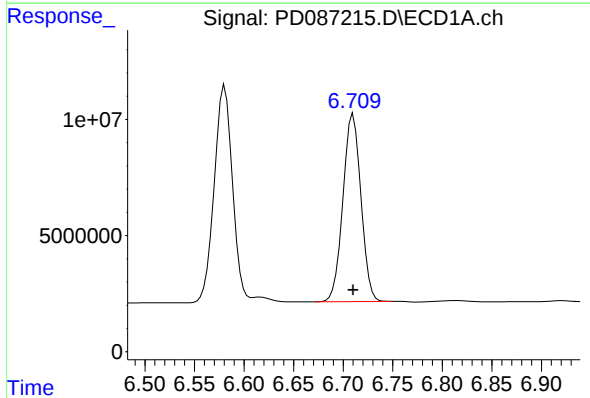


#16 4,4'-DDD

R.T.: 6.710 min
Delta R.T.: 0.000 min
Response: 101967233
Conc: 40.00 ng/ml

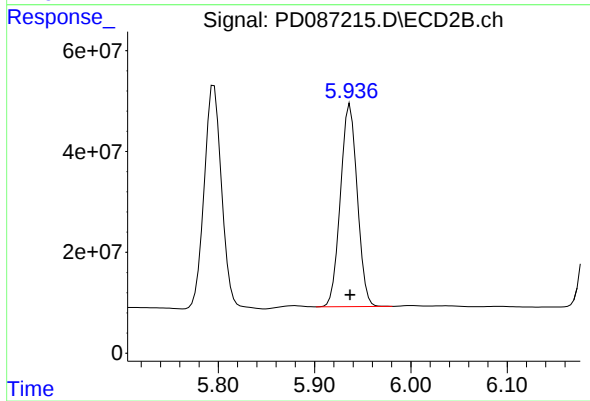

#16 4,4'-DDD


R.T.: 5.937 min
Delta R.T.: 0.000 min
Response: 486169790
Conc: 40.00 ng/ml

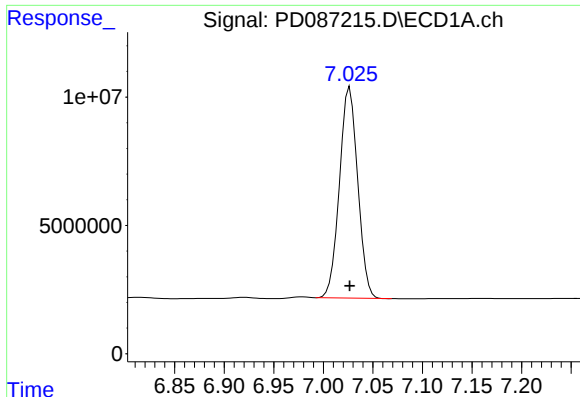

#17 4,4'-DDT


R.T.: 7.027 min
Delta R.T.: 0.000 min
Response: 105403810
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

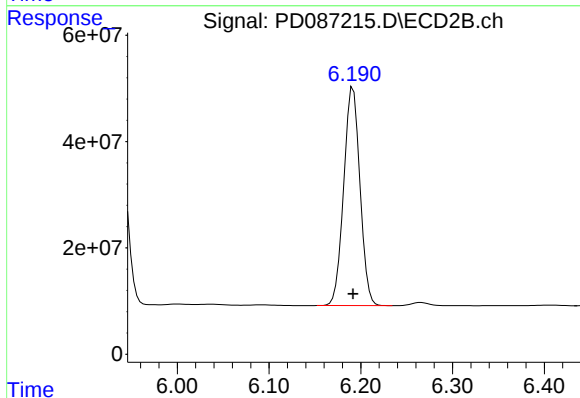


#17 4,4'-DDT

R.T.: 6.192 min
Delta R.T.: 0.000 min
Response: 505102801
Conc: 40.00 ng/ml

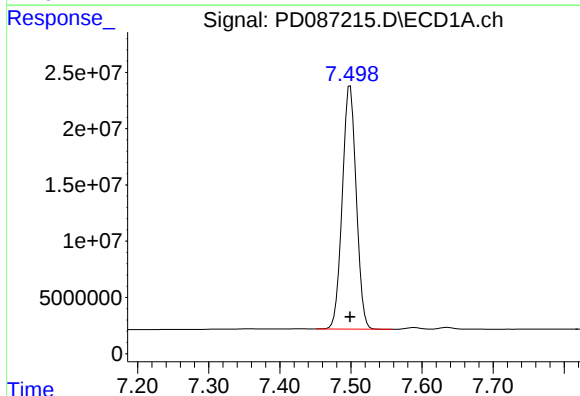


#20 Methoxychlor

R.T.: 7.499 min
Delta R.T.: 0.000 min
Response: 294774729
Conc: 200.00 ng/ml

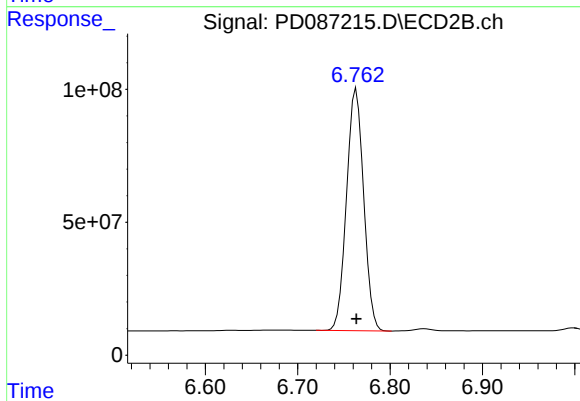

#20 Methoxychlor


R.T.: 6.763 min
Delta R.T.: 0.000 min
Response: 1173200758
Conc: 200.00 ng/ml

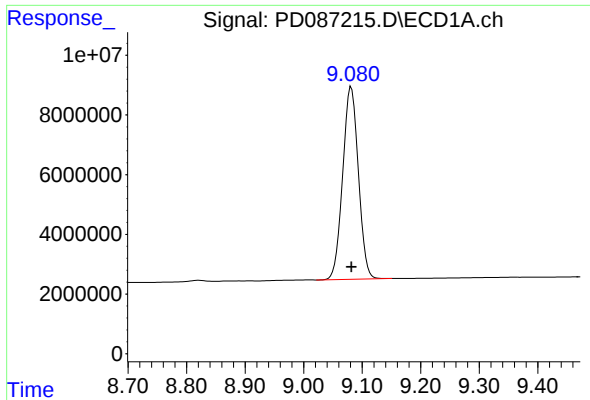

#27 Decachlorobiphenyl

R.T.: 9.081 min
Delta R.T.: 0.000 min
Response: 120004199
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

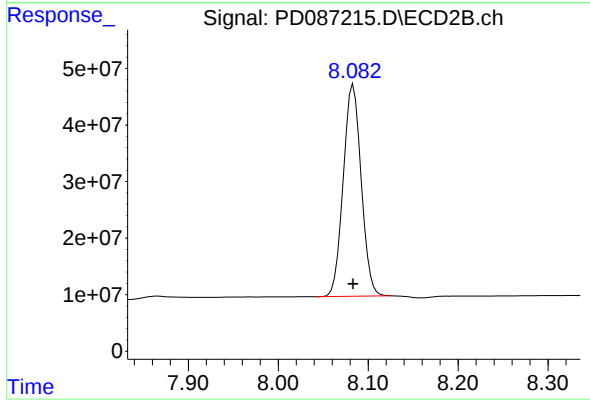

#27 Decachlorobiphenyl

R.T.: 8.084 min
Delta R.T.: 0.000 min
Response: 519850923
Conc: 40.00 ng/ml