

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122024\
 Data File : PD087217.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2024 20:34
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 02:15:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122024CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 20 02:14:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.556	2.883	79891536	439.8E6	39.503	38.066
27)	SA Decachlor...	9.082	8.084	229.2E6	977.0E6	76.410	75.175
Target Compounds							
2)	A alpha-BHC	4.005	3.397	167.8E6	707.3E6	42.622	38.940
3)	MA gamma-BHC...	4.336	3.734	160.3E6	650.9E6	42.031	38.634
4)	MA Heptachlor	4.936	4.089	159.9E6	657.1E6	41.144	38.130
9)	A Endosulfan I	6.081	5.254	131.7E6	548.1E6	40.096	37.929
13)	MA Dieldrin	6.354	5.520	296.5E6	1170.8E6	83.417	76.732
14)	MA Endrin	6.581	5.796	244.6E6	1049.0E6	84.080	76.264
16)	A 4,4'-DDD	6.711	5.938	212.7E6	931.6E6	83.448	76.645
17)	MA 4,4'-DDT	7.027	6.192	220.1E6	982.4E6	83.536	77.796
20)	A Methoxychlor	7.500	6.764	587.8E6	2129.6E6	398.820	363.047


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122024\
Data File : PD087217.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2024 20:34
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 02:15:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122024CLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 02:14:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

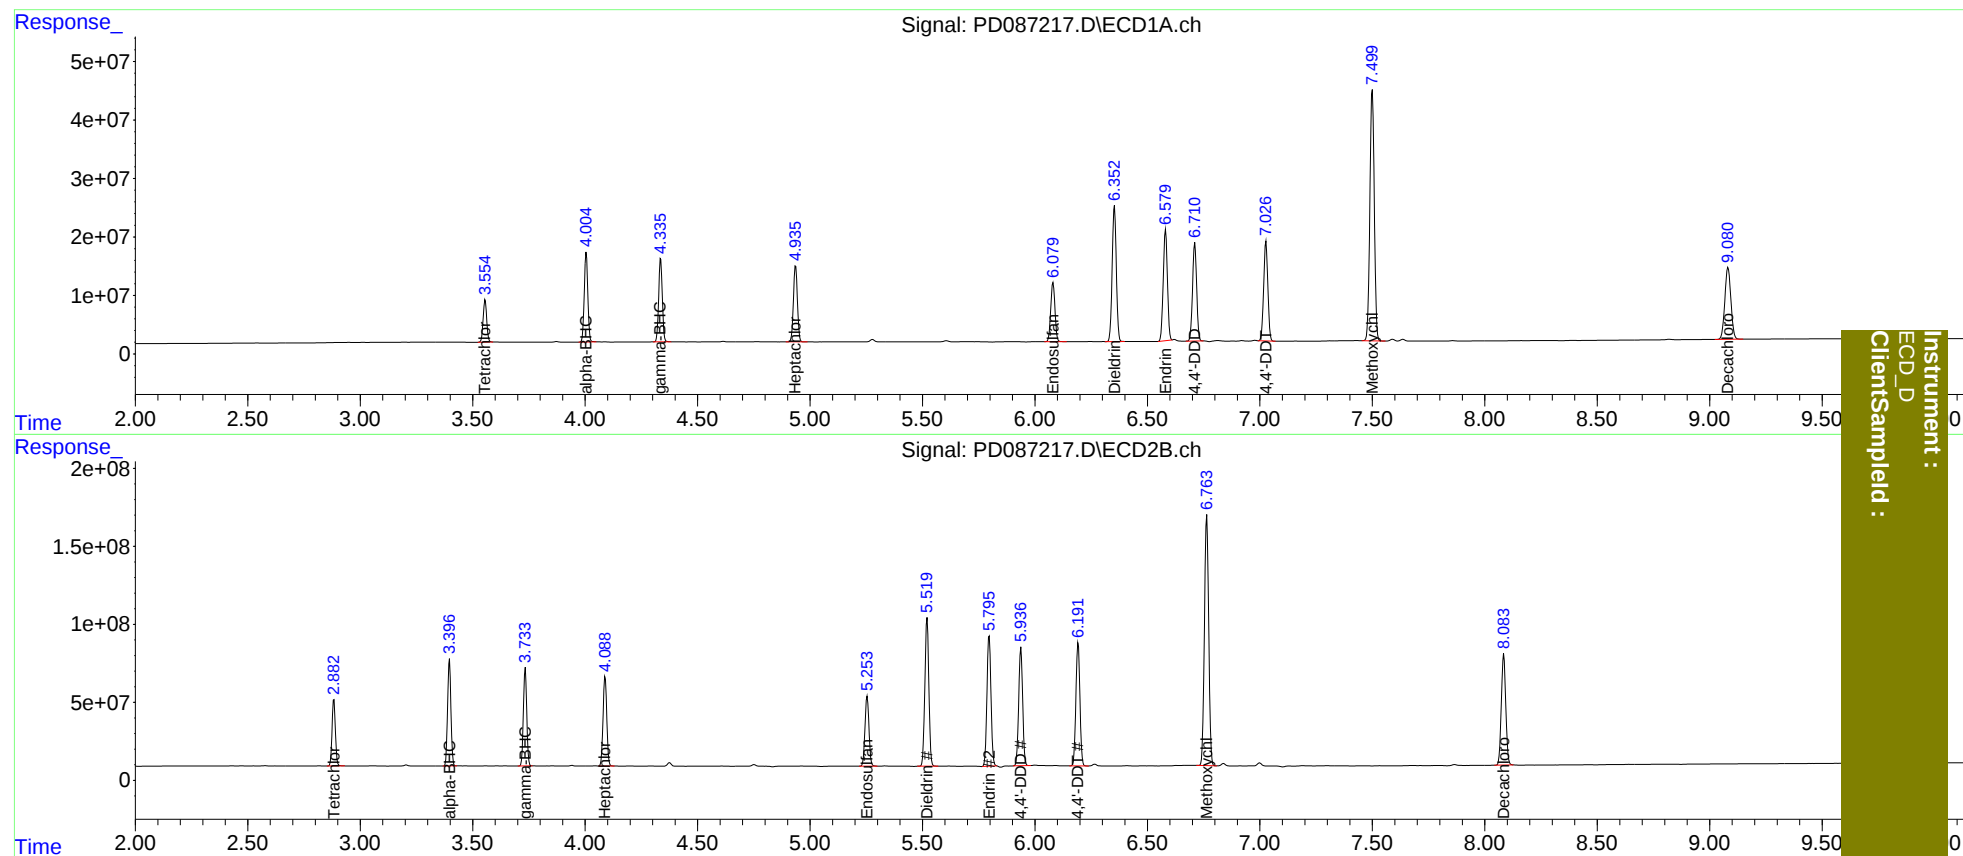


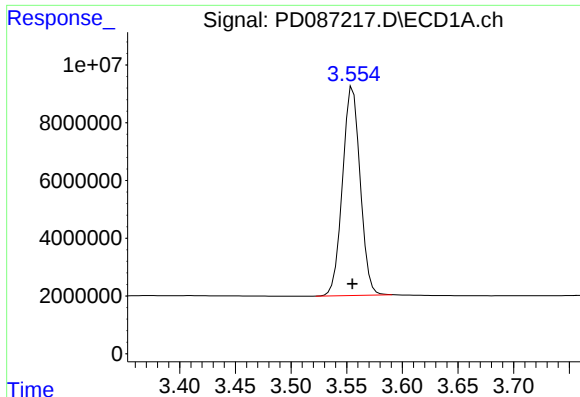

#1 Tetrachloro-m-xylene


R.T.: 3.556 min
Delta R.T.: 0.000 min
Response: 79891536
Conc: 39.50 ng/ml

Instrument :
ECD_D
ClientSampleId :

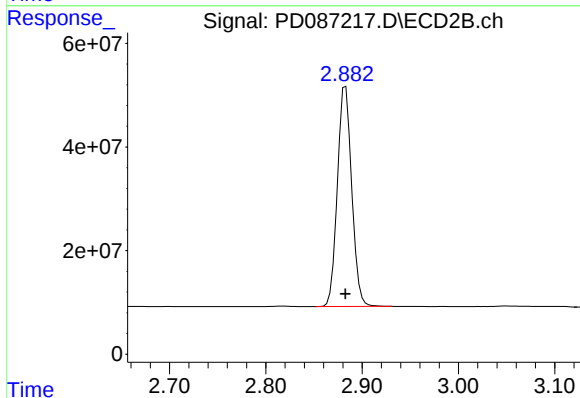


#1 Tetrachloro-m-xylene

R.T.: 2.883 min
Delta R.T.: 0.000 min
Response: 439830409
Conc: 38.07 ng/ml

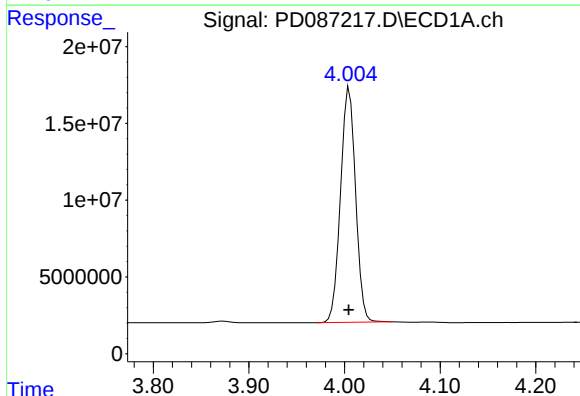


#2 alpha-BHC

R.T.: 4.005 min
Delta R.T.: 0.000 min
Response: 167787395
Conc: 42.62 ng/ml

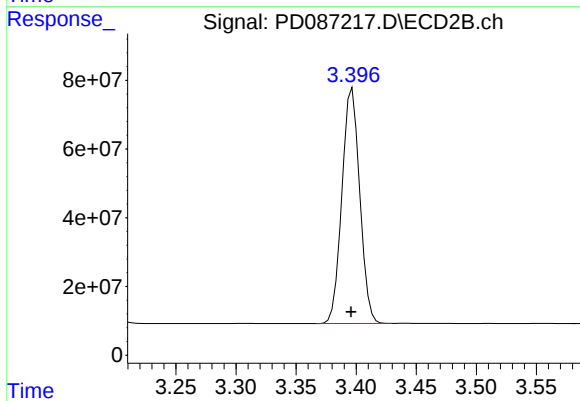

#2 alpha-BHC


R.T.: 3.397 min
Delta R.T.: 0.000 min
Response: 707327389
Conc: 38.94 ng/ml

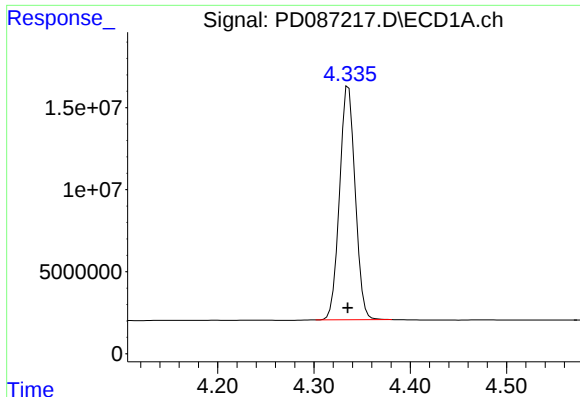

#3 gamma-BHC (Lindane)


R.T.: 4.336 min
Delta R.T.: 0.000 min
Response: 160347288
Conc: 42.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

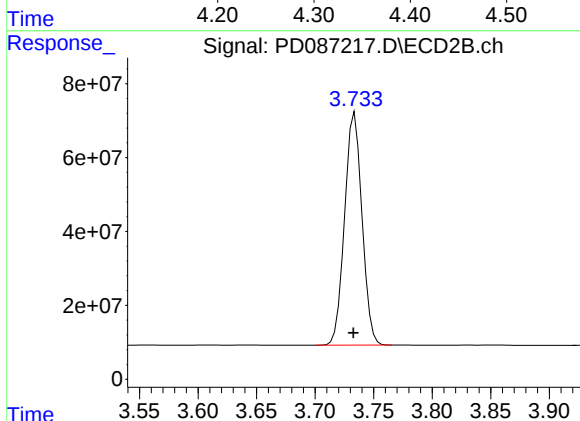


#3 gamma-BHC (Lindane)

R.T.: 3.734 min
Delta R.T.: 0.001 min
Response: 650858080
Conc: 38.63 ng/ml

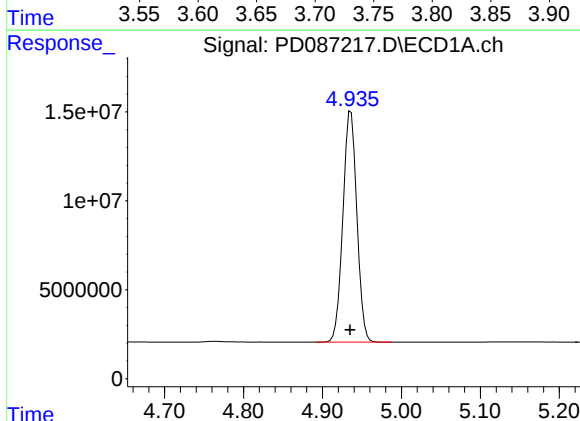


#4 Heptachlor

R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 159866946
Conc: 41.14 ng/ml

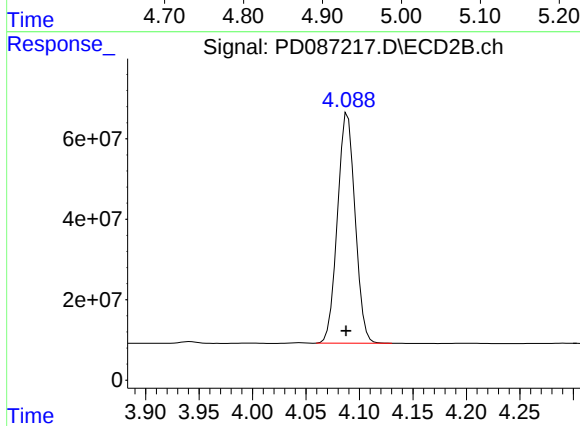

#4 Heptachlor


R.T.: 4.089 min
Delta R.T.: 0.002 min
Response: 657145017
Conc: 38.13 ng/ml

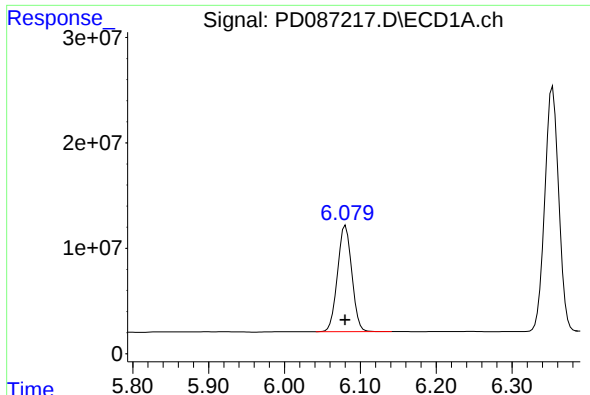

#9 Endosulfan I


R.T.: 6.081 min
Delta R.T.: 0.000 min
Response: 131725403
Conc: 40.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

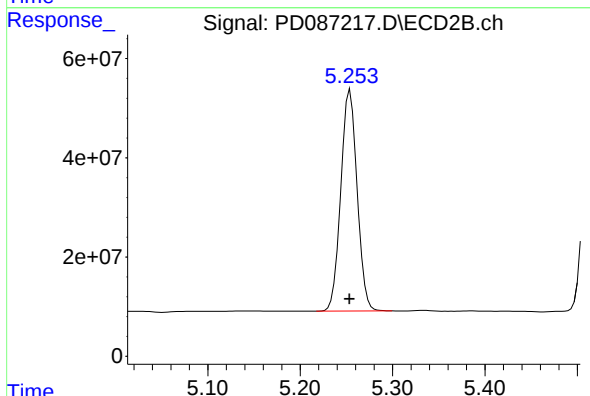


#9 Endosulfan I

R.T.: 5.254 min
Delta R.T.: 0.000 min
Response: 548118468
Conc: 37.93 ng/ml

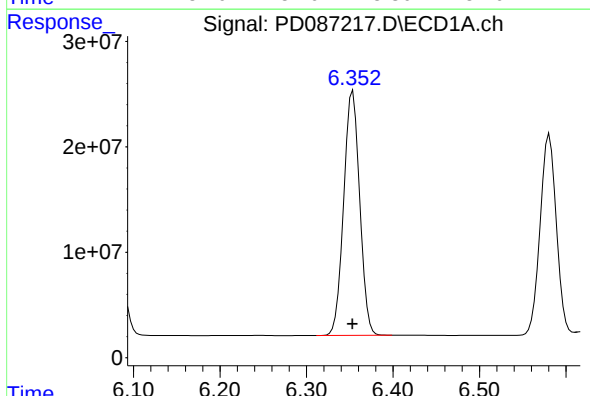


#13 Dieldrin

R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 296496317
Conc: 83.42 ng/ml

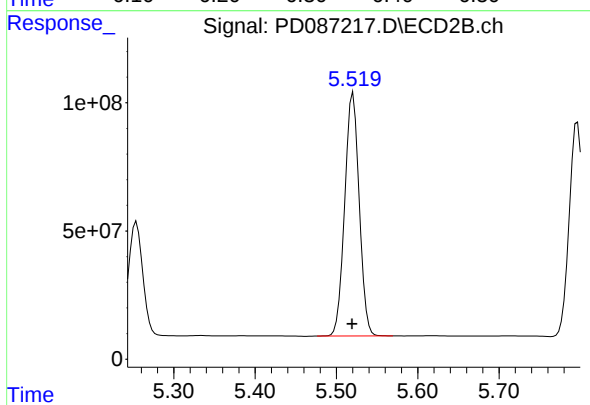

#13 Dieldrin


R.T.: 5.520 min
Delta R.T.: 0.001 min
Response: 1170756392
Conc: 76.73 ng/ml

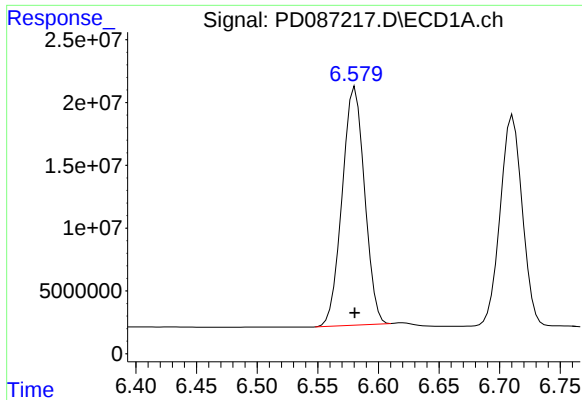

#14 Endrin


R.T.: 6.581 min
Delta R.T.: 0.000 min
Response: 244564346
Conc: 84.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

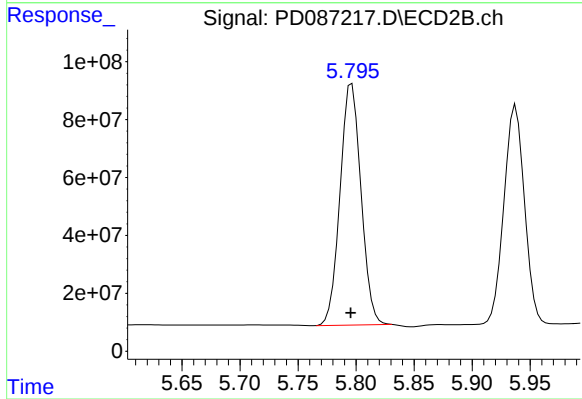


#14 Endrin

R.T.: 5.796 min
Delta R.T.: 0.000 min
Response: 1049013782
Conc: 76.26 ng/ml

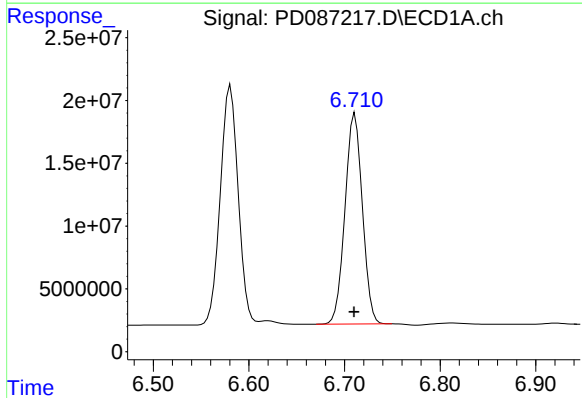


#16 4,4'-DDD

R.T.: 6.711 min
Delta R.T.: 0.000 min
Response: 212723114
Conc: 83.45 ng/ml

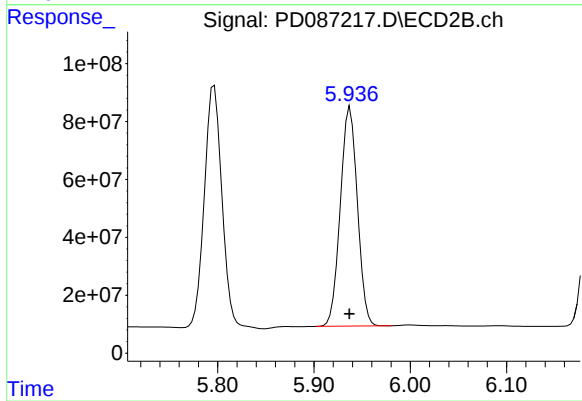

#16 4,4'-DDD


R.T.: 5.938 min
Delta R.T.: 0.000 min
Response: 931564871
Conc: 76.65 ng/ml

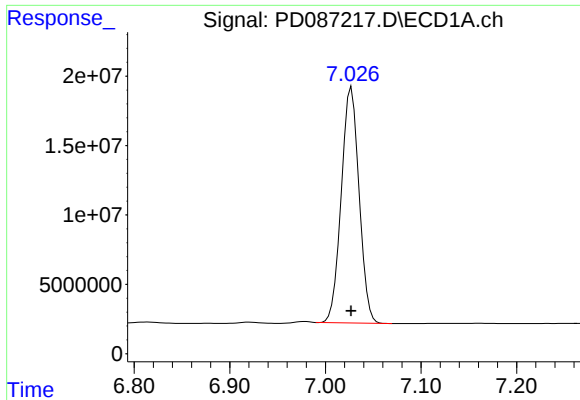

#17 4,4'-DDT


R.T.: 7.027 min
Delta R.T.: 0.000 min
Response: 220124627
Conc: 83.54 ng/ml

Instrument :
ECD_D
ClientSampleId :

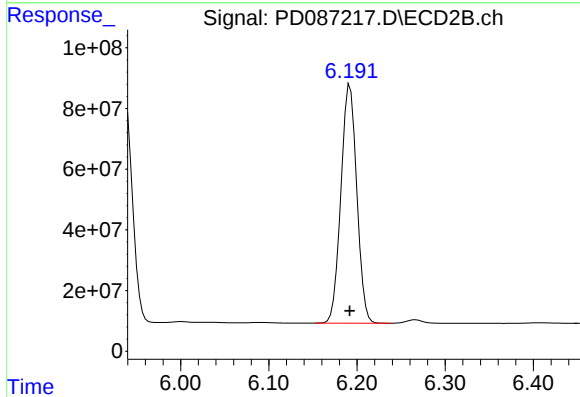


#17 4,4'-DDT

R.T.: 6.192 min
Delta R.T.: 0.000 min
Response: 982370982
Conc: 77.80 ng/ml

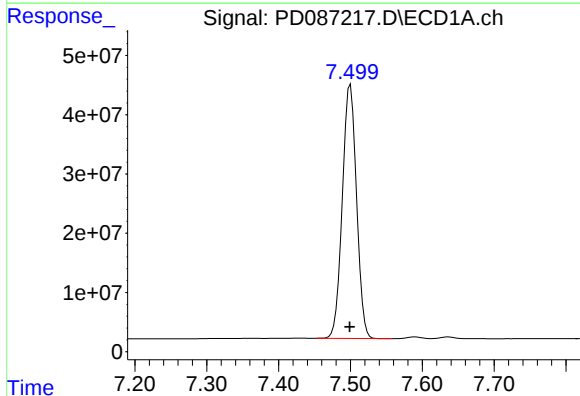


#20 Methoxychlor

R.T.: 7.500 min
Delta R.T.: 0.001 min
Response: 587810531
Conc: 398.82 ng/ml

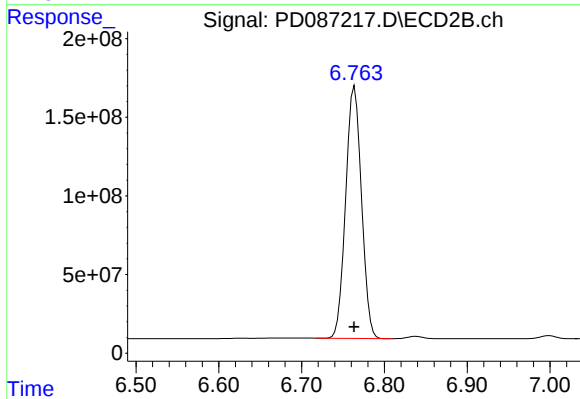

#20 Methoxychlor

R.T.: 6.764 min
Delta R.T.: 0.000 min
Response: 2129632553
Conc: 363.05 ng/ml

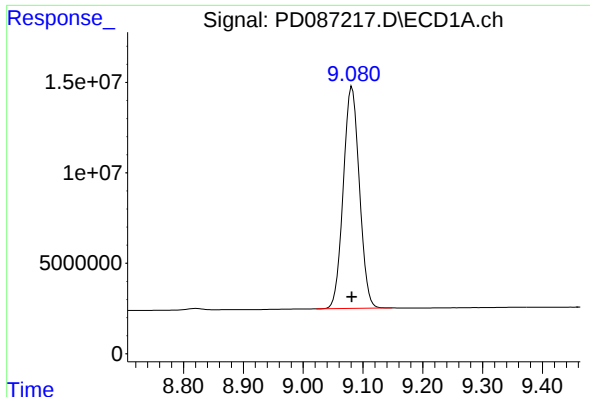

#27 Decachlorobiphenyl


R.T.: 9.082 min

Delta R.T.: 0.000 min

Response: 229238201

Conc: 76.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

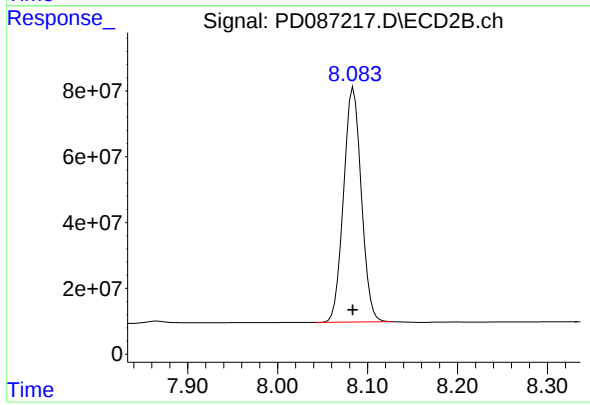

#27 Decachlorobiphenyl

R.T.: 8.084 min

Delta R.T.: 0.000 min

Response: 976992541

Conc: 75.17 ng/ml