

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122024\
 Data File : PD087219.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2024 21:02
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 02:16:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122024CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 20 02:14:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.883	161.7E6	847.9E6	79.969	73.383
27)	SA Decachlor...	9.081	8.083	445.2E6	1866.7E6	148.380	143.634
Target Compounds							
2)	A alpha-BHC	4.005	3.396	365.2E6	1394.3E6	92.769	76.760
3)	MA gamma-BHC...	4.336	3.732	343.2E6	1278.1E6	89.967	75.864
4)	MA Heptachlor	4.936	4.088	337.9E6	1264.3E6	86.952	73.356
9)	A Endosulfan I	6.080	5.254	271.5E6	1048.4E6	82.649	72.548
13)	MA Dieldrin	6.353	5.520	623.8E6	2244.5E6	175.493	147.107
14)	MA Endrin	6.581	5.796	515.1E6	1993.9E6	177.088	144.955
16)	A 4,4'-DDD	6.711	5.937	448.2E6	1779.0E6	175.813	146.366
17)	MA 4,4'-DDT	7.027	6.191	465.5E6	1901.1E6	176.653	150.549
20)	A Methoxychlor	7.499	6.763	1172.0E6	3750.1E6	795.181	639.302


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122024\
Data File : PD087219.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2024 21:02
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 02:16:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122024CLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 02:14:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

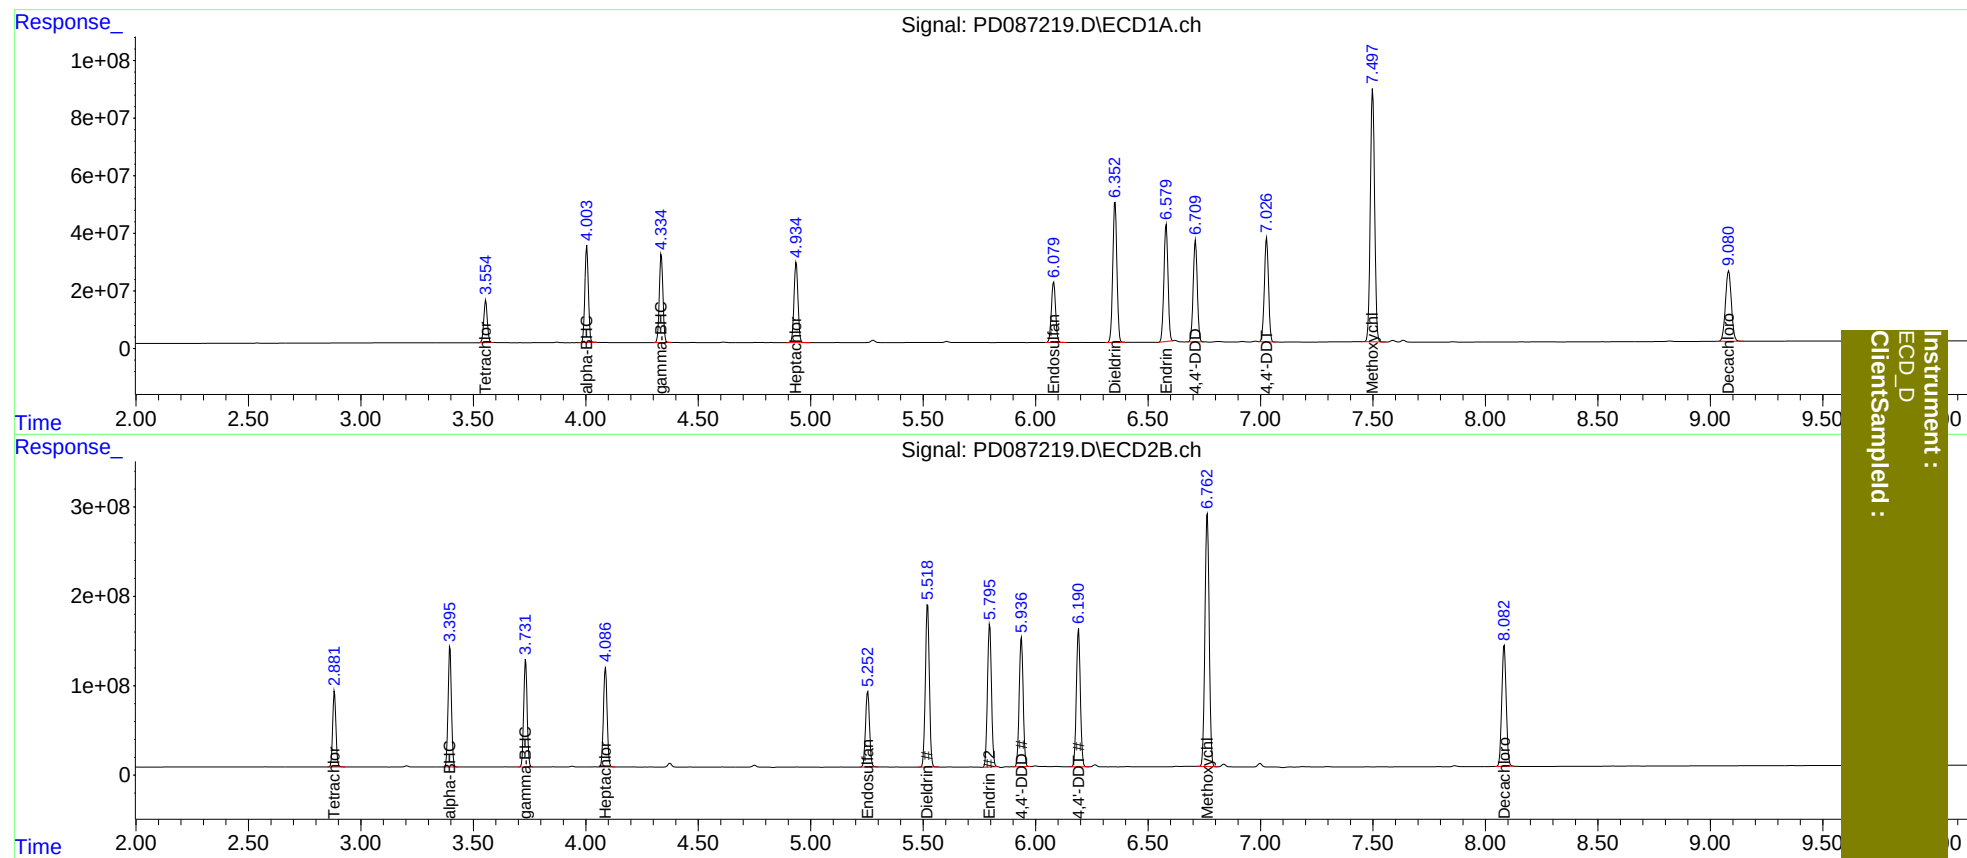


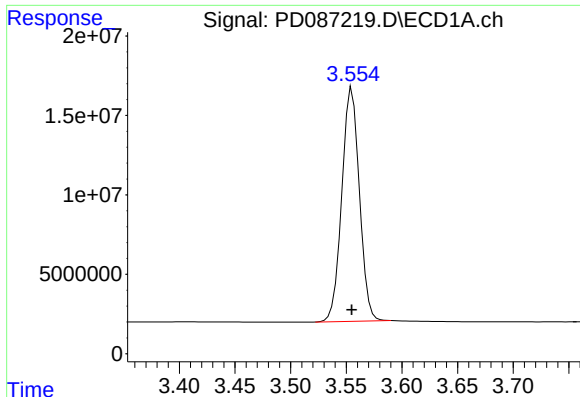

#1 Tetrachloro-m-xylene


R.T.: 3.555 min
Delta R.T.: 0.000 min
Response: 161731651
Conc: 79.97 ng/ml

Instrument :
ECD_D
ClientSampleId :

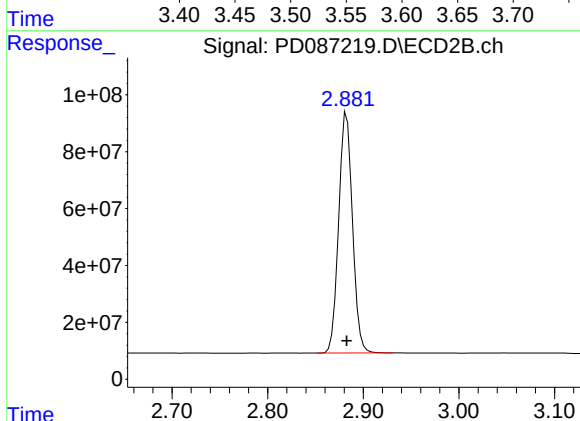


#1 Tetrachloro-m-xylene

R.T.: 2.883 min
Delta R.T.: 0.000 min
Response: 847889141
Conc: 73.38 ng/ml

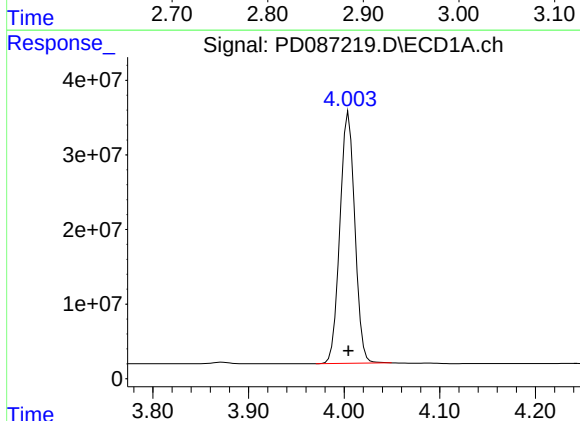


#2 alpha-BHC

R.T.: 4.005 min
Delta R.T.: 0.000 min
Response: 365195495
Conc: 92.77 ng/ml

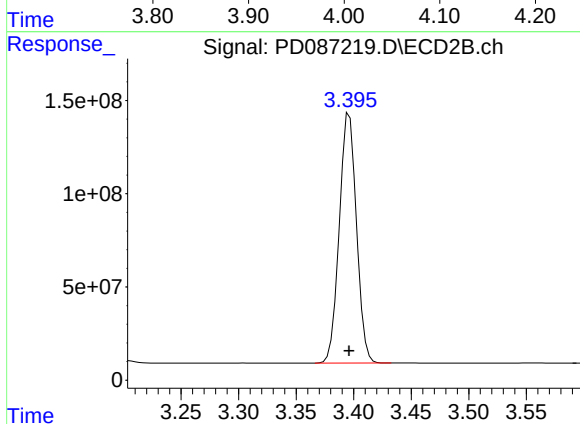

#2 alpha-BHC


R.T.: 3.396 min
Delta R.T.: 0.000 min
Response: 1394330011
Conc: 76.76 ng/ml

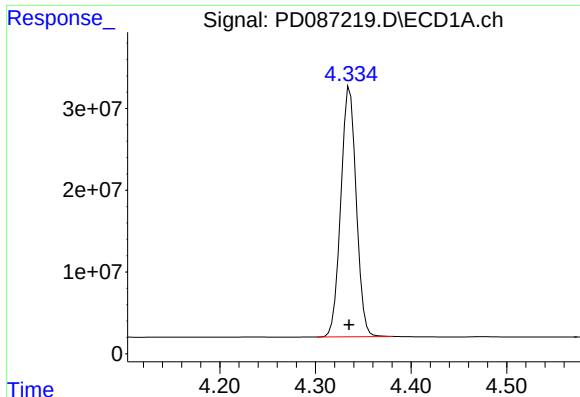

#3 gamma-BHC (Lindane)


R.T.: 4.336 min
Delta R.T.: 0.000 min
Response: 343222464
Conc: 89.97 ng/ml

Instrument :
ECD_D
ClientSampleId :

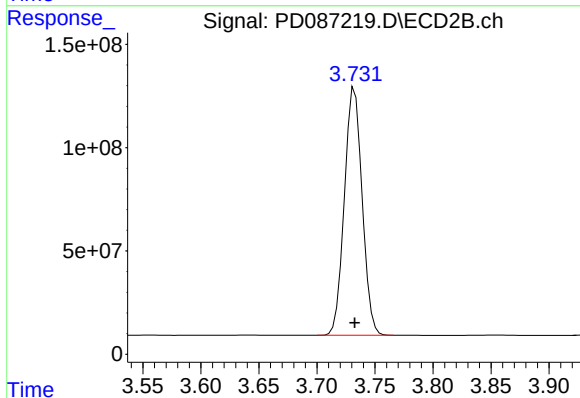


#3 gamma-BHC (Lindane)

R.T.: 3.732 min
Delta R.T.: 0.000 min
Response: 1278058244
Conc: 75.86 ng/ml

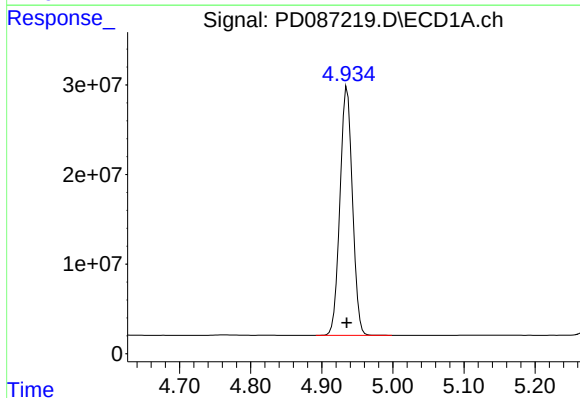


#4 Heptachlor

R.T.: 4.936 min
Delta R.T.: 0.000 min
Response: 337856079
Conc: 86.95 ng/ml

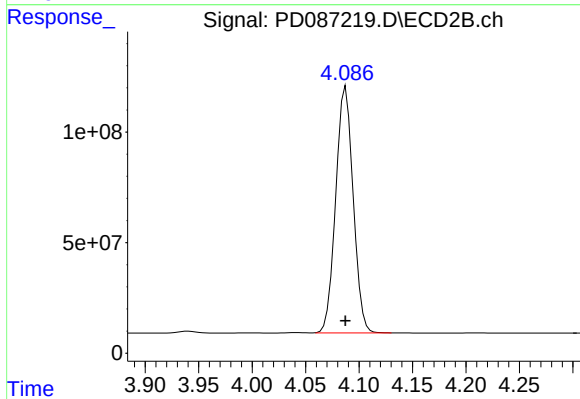

#4 Heptachlor


R.T.: 4.088 min
Delta R.T.: 0.000 min
Response: 1264250509
Conc: 73.36 ng/ml

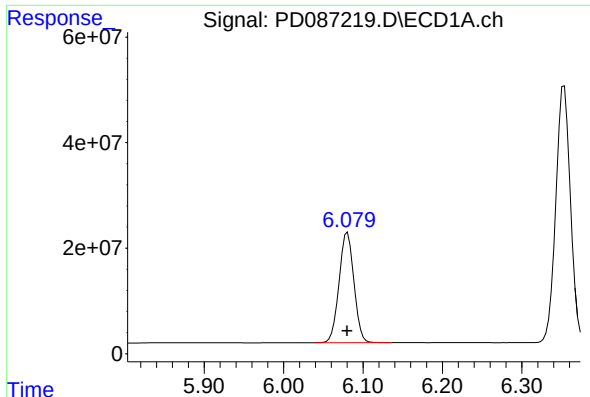

#9 Endosulfan I


R.T.: 6.080 min
Delta R.T.: 0.000 min
Response: 271523837
Conc: 82.65 ng/ml

Instrument :
ECD_D
ClientSampleId :

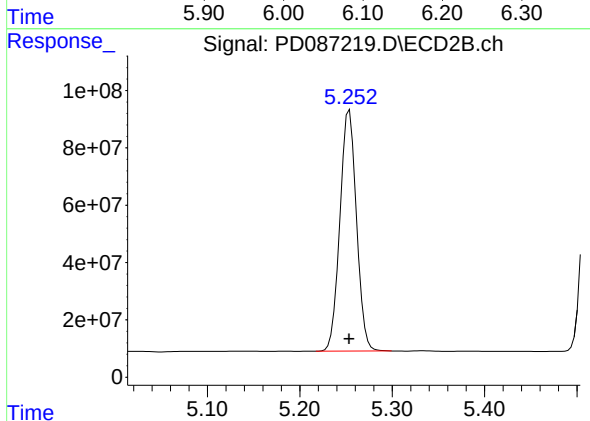


#9 Endosulfan I

R.T.: 5.254 min
Delta R.T.: 0.000 min
Response: 1048393620
Conc: 72.55 ng/ml

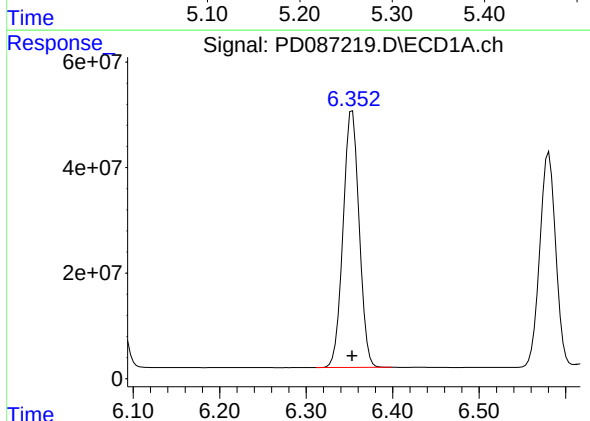


#13 Dieldrin

R.T.: 6.353 min
Delta R.T.: 0.000 min
Response: 623769743
Conc: 175.49 ng/ml

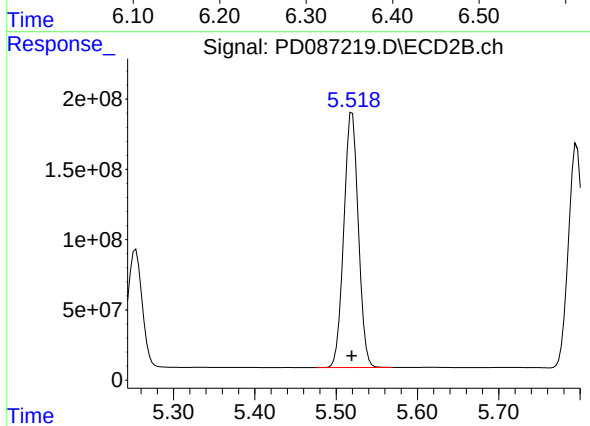

#13 Dieldrin


R.T.: 5.520 min
Delta R.T.: 0.000 min
Response: 2244516241
Conc: 147.11 ng/ml

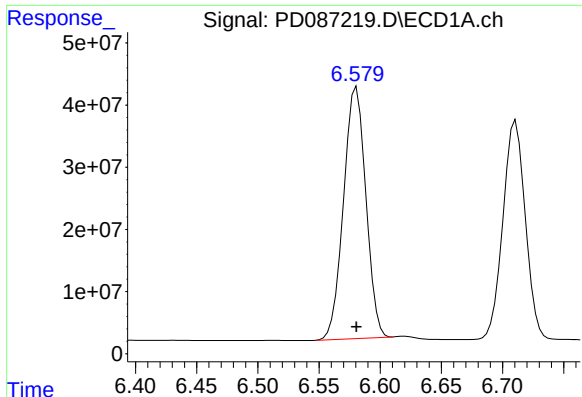

#14 Endrin


R.T.: 6.581 min
Delta R.T.: 0.000 min
Response: 515095153
Conc: 177.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

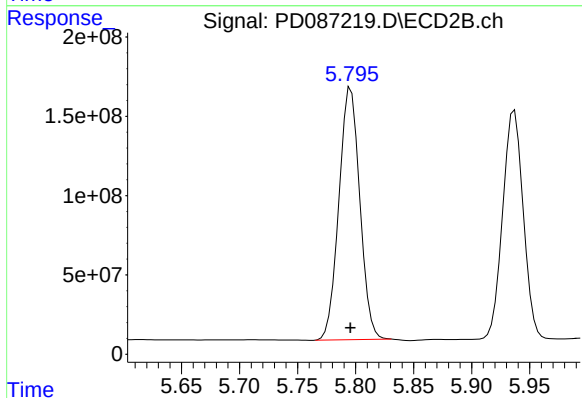


#14 Endrin

R.T.: 5.796 min
Delta R.T.: 0.000 min
Response: 1993867564
Conc: 144.96 ng/ml

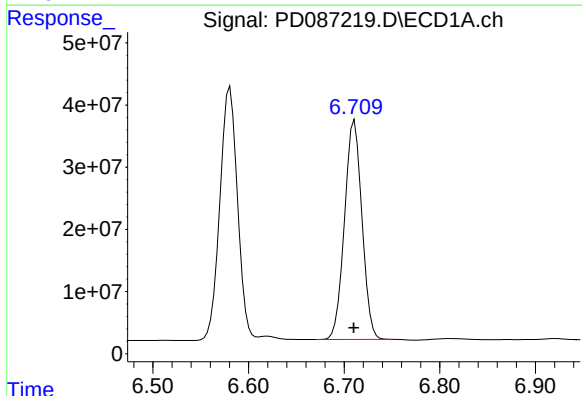


#16 4,4'-DDD

R.T.: 6.711 min
Delta R.T.: 0.000 min
Response: 448178960
Conc: 175.81 ng/ml

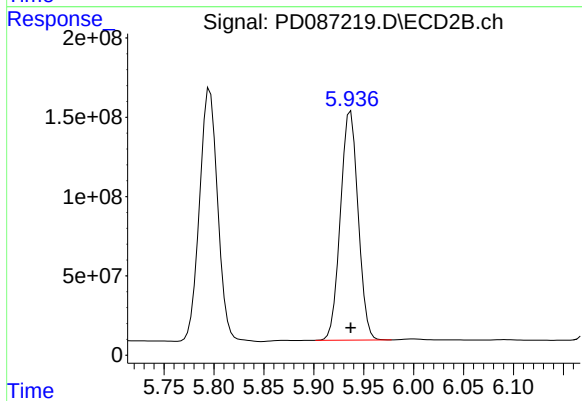

#16 4,4'-DDD


R.T.: 5.937 min
Delta R.T.: 0.000 min
Response: 1778972939
Conc: 146.37 ng/ml

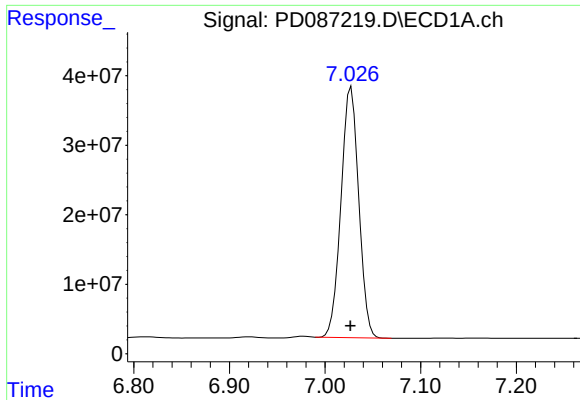

#17 4,4'-DDT


R.T.: 7.027 min
Delta R.T.: 0.000 min
Response: 465496751
Conc: 176.65 ng/ml

Instrument :
ECD_D
ClientSampleId :

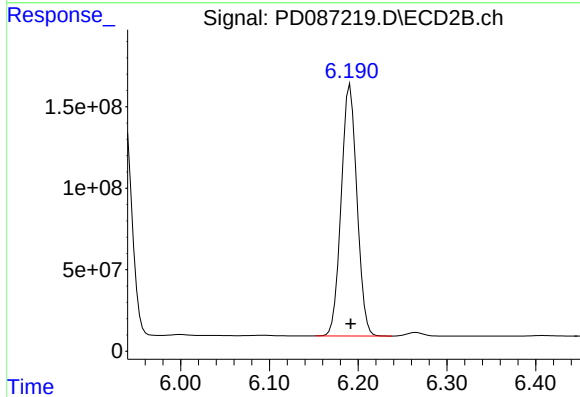


#17 4,4'-DDT

R.T.: 6.191 min
Delta R.T.: 0.000 min
Response: 1901073350
Conc: 150.55 ng/ml

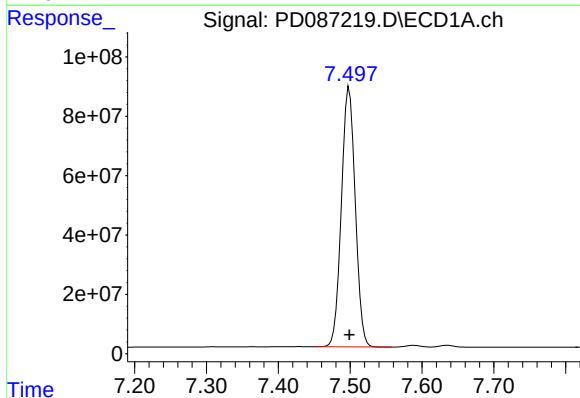


#20 Methoxychlor

R.T.: 7.499 min
Delta R.T.: 0.000 min
Response: 1171997038
Conc: 795.18 ng/ml

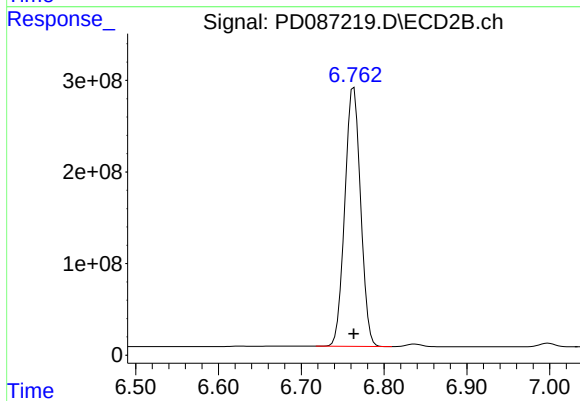

#20 Methoxychlor


R.T.: 6.763 min
Delta R.T.: 0.000 min
Response: 3750149225
Conc: 639.30 ng/ml

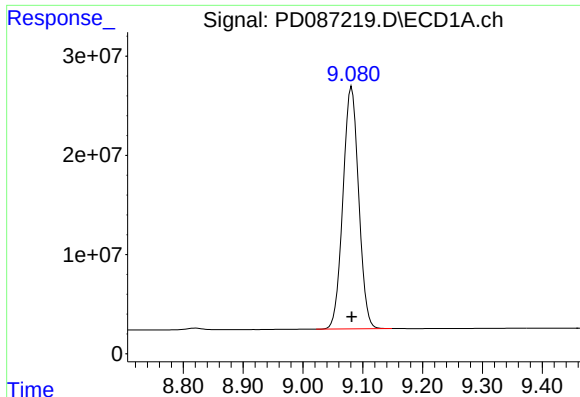

#27 Decachlorobiphenyl

R.T.: 9.081 min
Delta R.T.: 0.000 min
Response: 445155395
Conc: 148.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

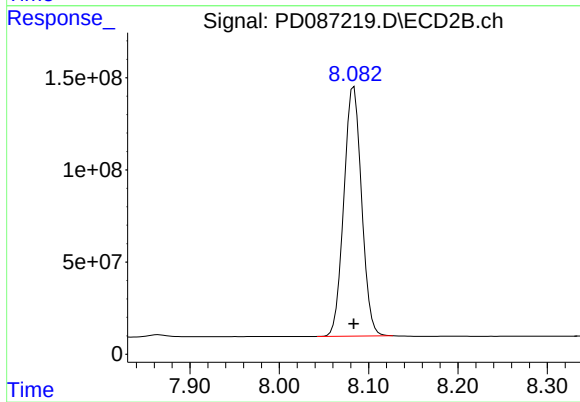

#27 Decachlorobiphenyl

R.T.: 8.083 min
Delta R.T.: 0.000 min
Response: 1866711454
Conc: 143.63 ng/ml