

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD122118\  
Data File : PD050858.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Dec 2018 11:21  
Operator : AJ\SJ  
Sample : J6485-06  
Misc :  
ALS Vial : 11 Sample Multiplier: 1



Instrument :  
ECD\_D  
ClientSampleId :  
ETO85

Manual Integrations  
APPROVED

Sohil  
12/26/2018 9:11:16 AM

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 21 22:27:32 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD120318CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Dec 04 00:43:01 2018  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

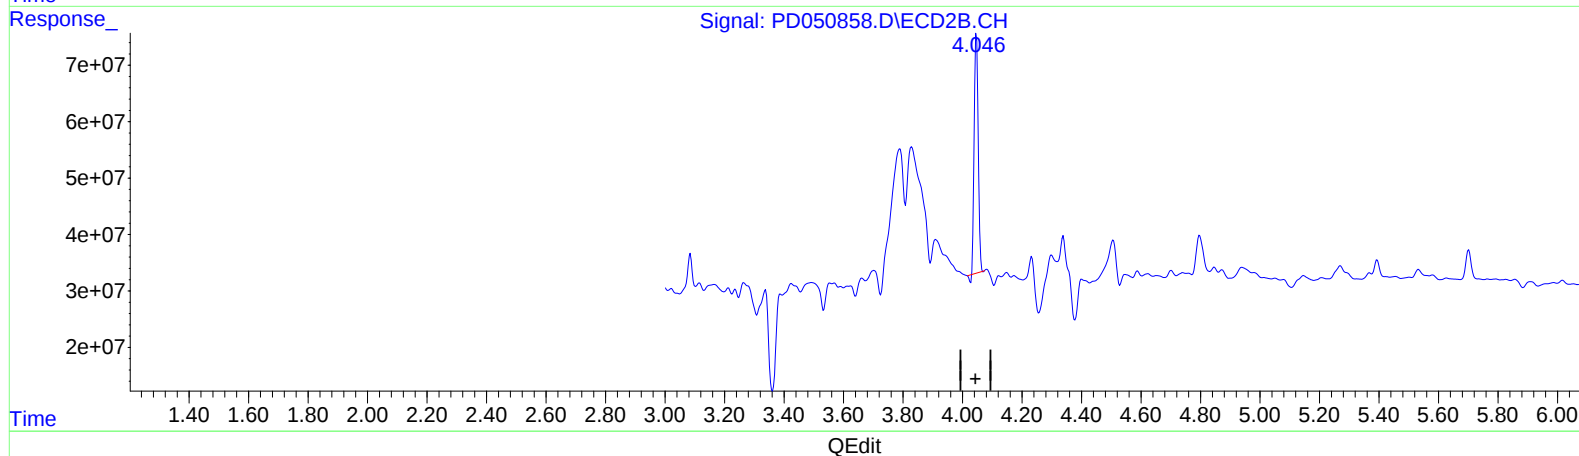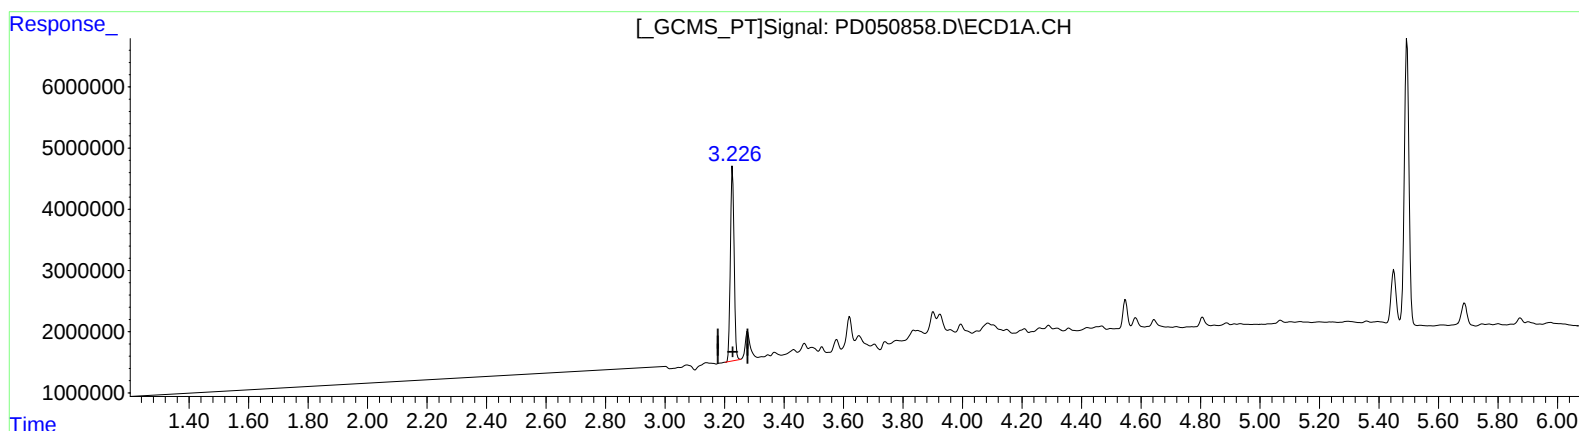

(1) Tetrachloro-m-xylene (SA)

3.227min 18.007 ng/ml

response 27463903

(1) Tetrachloro-m-xylene #2 (SA)

4.047min 13.977 ng/ml

response 396279486

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD122118\  
Data File : PD050858.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Dec 2018 11:21  
Operator : AJ\SJ  
Sample : J6485-06  
Misc :  
ALS Vial : 11 Sample Multiplier: 1



Instrument :  
ECD\_D  
ClientSampleId :  
ETO85

Manual Integrations  
APPROVED

Sohil  
12/26/2018 9:11:16 AM

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 21 22:27:32 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD120318CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Dec 04 00:43:01 2018  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

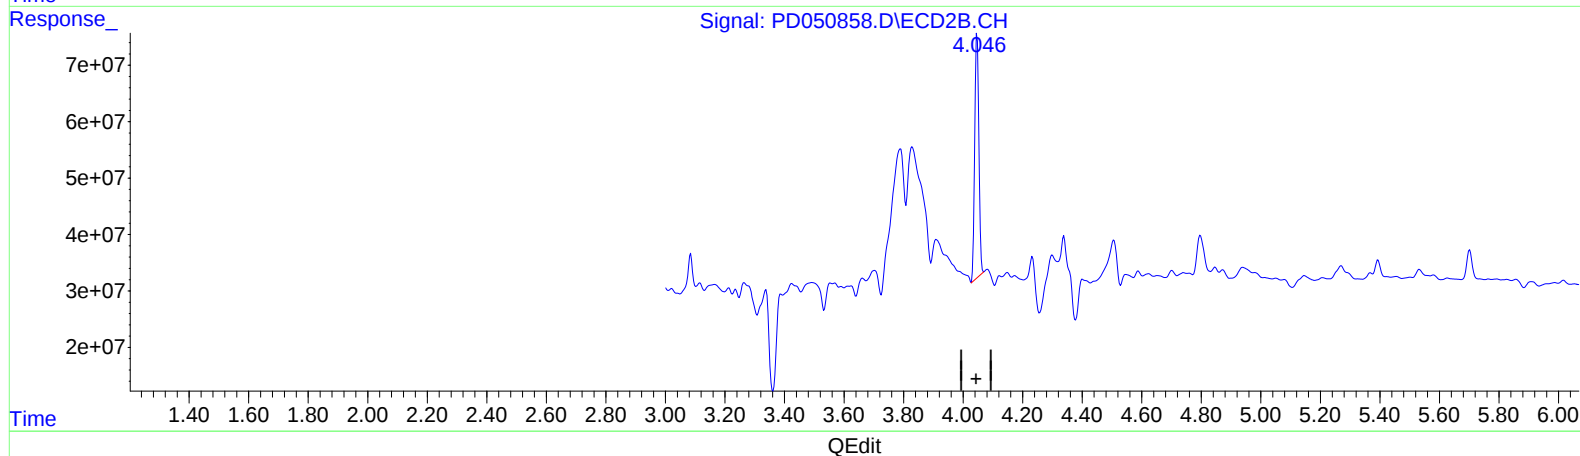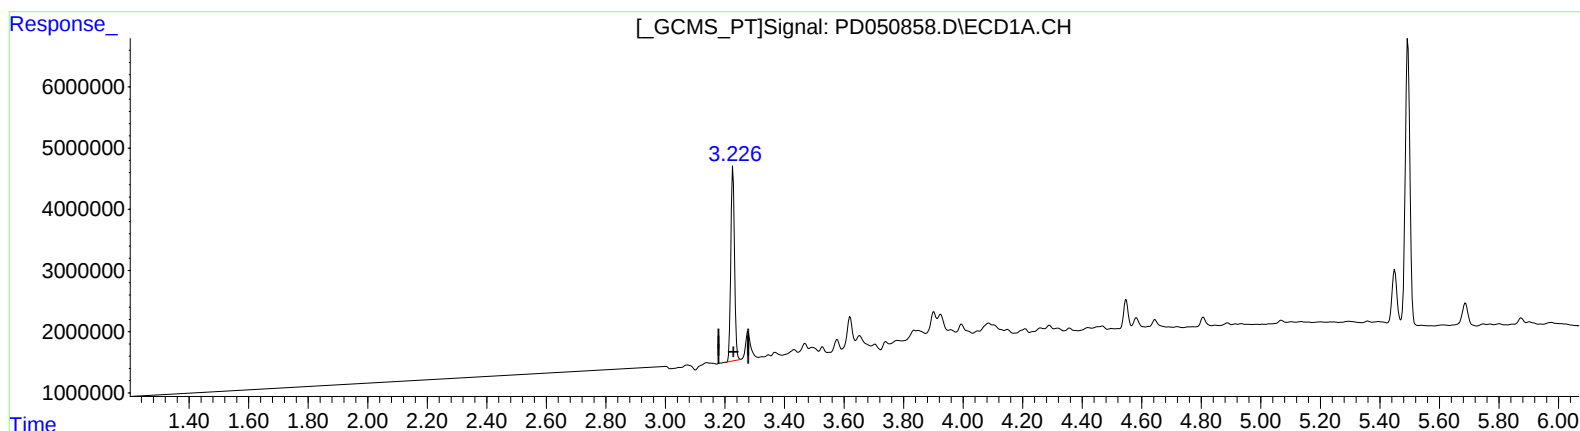

(1) Tetrachloro-m-xylene (SA)

3.227min 18.007 ng/ml

response 27463903

(1) Tetrachloro-m-xylene #2 (SA)

4.046min 14.804 ng/ml m

response 419709454

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD122118\  
 Data File : PD050858.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 21 Dec 2018 11:21  
 Operator : AJ\SJ  
 Sample : J6485-06  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Dec 21 22:27:32 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD120318CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Tue Dec 04 00:43:01 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

| Compound                    | RT#1  | RT#2  | Resp#1   | Resp#2  | ng/ml  | ng/ml   |
|-----------------------------|-------|-------|----------|---------|--------|---------|
| -----                       |       |       |          |         |        |         |
| System Monitoring Compounds |       |       |          |         |        |         |
| 1) SA Tetrachlo...          | 3.227 | 4.046 | 27463903 | 419.7E6 | 18.007 | 14.804m |
| 27) SA Decachlor...         | 7.834 | 9.161 | 56023970 | 648.6E6 | 34.057 | 29.969  |

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :  
 ECD\_D  
 ClientSampleID :  
 ETO85

Manual Integrations  
 APPROVED

Sohil  
 12/26/2018 9:11:16 AM

> SJ  
 12/28/18