

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122120\
 Data File : PD060793.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2020 12:48
 Operator : DD\AJ
 Sample : L5134-02MS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFN58MS

Manual Integrations
 APPROVED

Ankita
 12/22/2020 9:25:40 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 13:12:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 04 03:58:39 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.501	4.022	8855217	33029007	7.580	8.397
27)	SA Decachlor...	8.287	9.108	154.7E6	601.8E6	103.763	185.913m#
Target Compounds							
3)	MA gamma-BHC...	4.233	4.692	255.0E6	194.4E6	158.075	36.258m#
4)	MA Heptachlor	4.534	5.210	54008688	188.6E6	32.162	35.858
5)	MB Aldrin	4.785	5.517	47054841	198.3E6	29.255	39.827 #
9)	A Endosulfan I	5.594	6.265	410.1E6	89717772	282.269	20.960m#
10)	B trans-Chl...	5.463	6.120	2909168	2790.4E6	1.839m	592.080m#
11)	B cis-Chlor...	5.525	6.209	5041864	63091594	3.237	13.991m#
12)	B 4,4'-DDE	5.682	6.361	4232453	39270699	2.812m	8.892m#
13)	MA Dieldrin	5.816	6.519	253.7E6	390.0E6	159.750m	83.507m#
14)	MA Endrin	6.076	6.737	106.3E6	346.5E6	82.142	94.005m
16)	A 4,4'-DDD	6.200	6.854	63584065	367.1E6	49.486m	99.618 #
17)	MA 4,4'-DDT	6.443	7.157	93340346	359.2E6	71.666m	100.100 #
20)	A Methoxychlor	6.978	7.595	12926168	203.7E6	19.006m	112.920 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122120\
Data File : PD060793.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2020 12:48
Operator : DD\AJ
Sample : L5134-02MS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 13:12:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 04 03:58:39 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

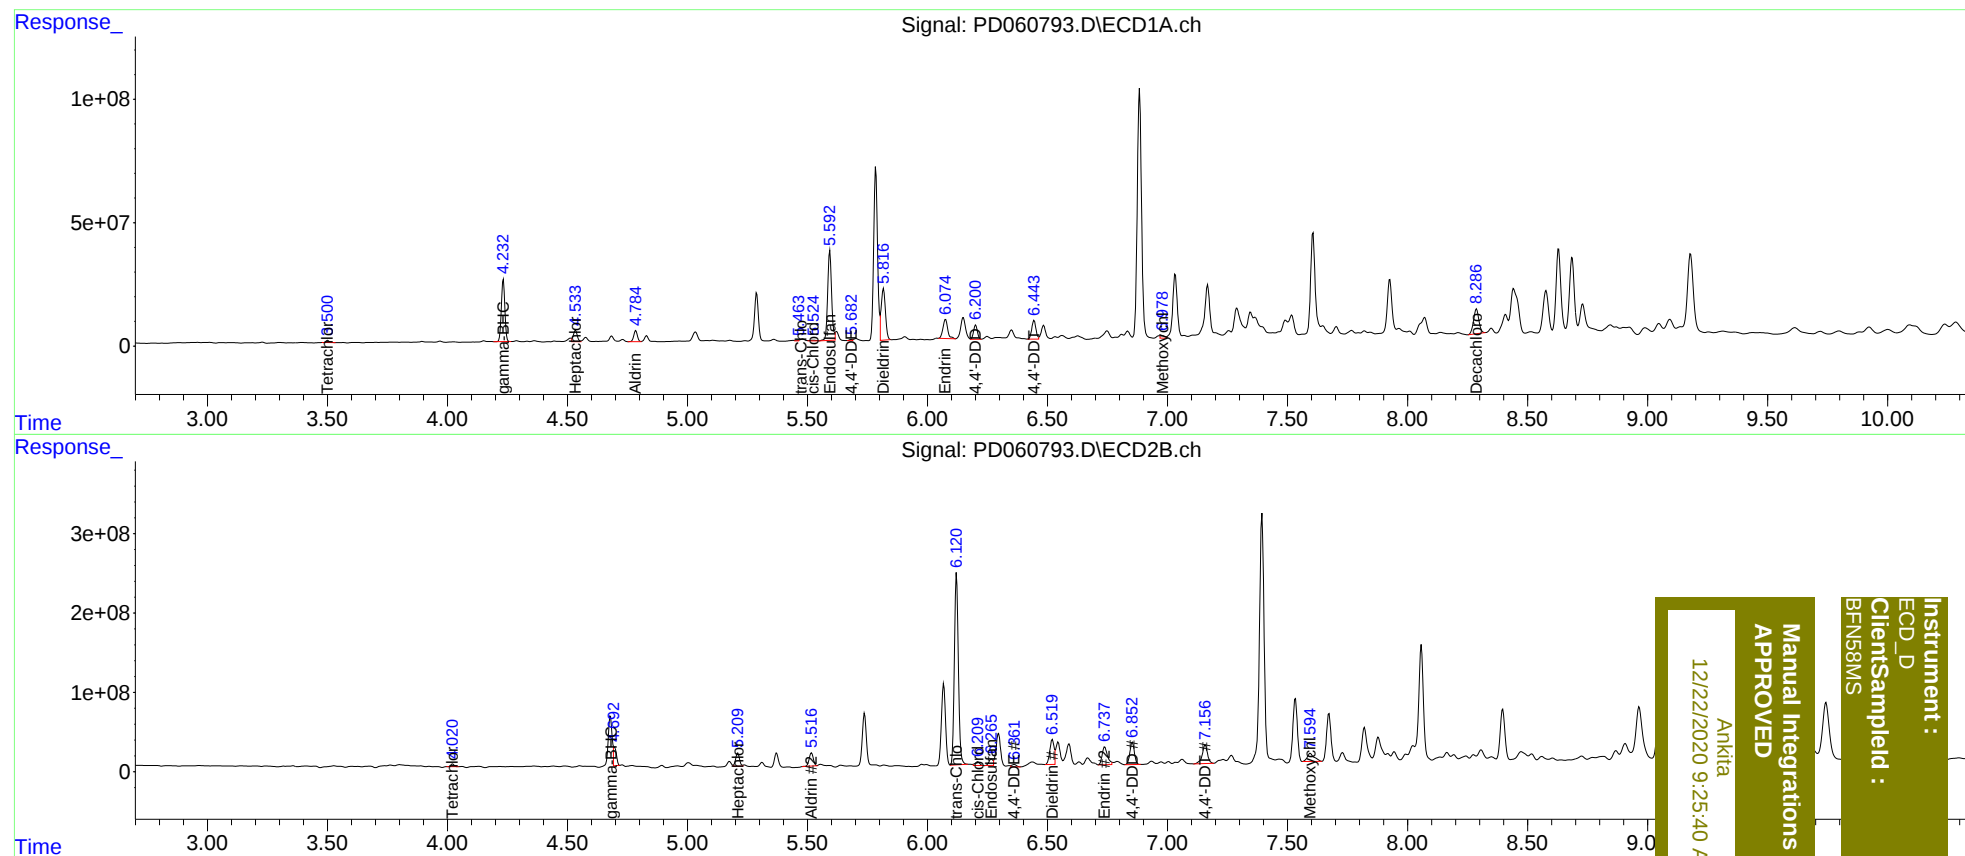

12/22/2020 9:25:40 AM
Ankita

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sample :
BFN58MS