

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122122\
 Data File : PD073392.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2022 13:20
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 03:48:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122122CLP.M
 Quant Title : GC Extractables
 QLast Update : Sun Dec 25 03:42:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.694	3.454	10795308	388.7E6	5.454	6.118
27)	SA Decachlor...	7.818	8.900	27045133	209.3E6	11.254	11.049
Target Compounds							
2)	A alpha-BHC	3.196	3.918	14775470	530.8E6	4.810	6.366 #
3)	MA gamma-BHC...	3.525	4.251	13340613	453.7E6	4.795	6.548 #
4)	MA Heptachlor	3.857	4.817	15224512	341.4E6	5.125	6.111
9)	A Endosulfan I	5.009	5.972	13991586	216.6E6	5.276	5.704
13)	MA Dieldrin	5.275	6.248	28436125	452.8E6	9.708	11.274
14)	MA Endrin	5.551	6.480	25718100	404.7E6	9.943	12.211
16)	A 4,4'-DDD	5.698	6.614	22434351	339.6E6	9.752	11.361
17)	MA 4,4'-DDT	5.947	6.922	21744759	311.4E6	9.452	10.862
20)	A Methoxychlor	6.530	7.401	67858188	698.1E6	52.428	56.868


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122122\
Data File : PD073392.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2022 13:20
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 03:48:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122122CLP.M
Quant Title : GC Extractables
QLast Update : Sun Dec 25 03:42:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

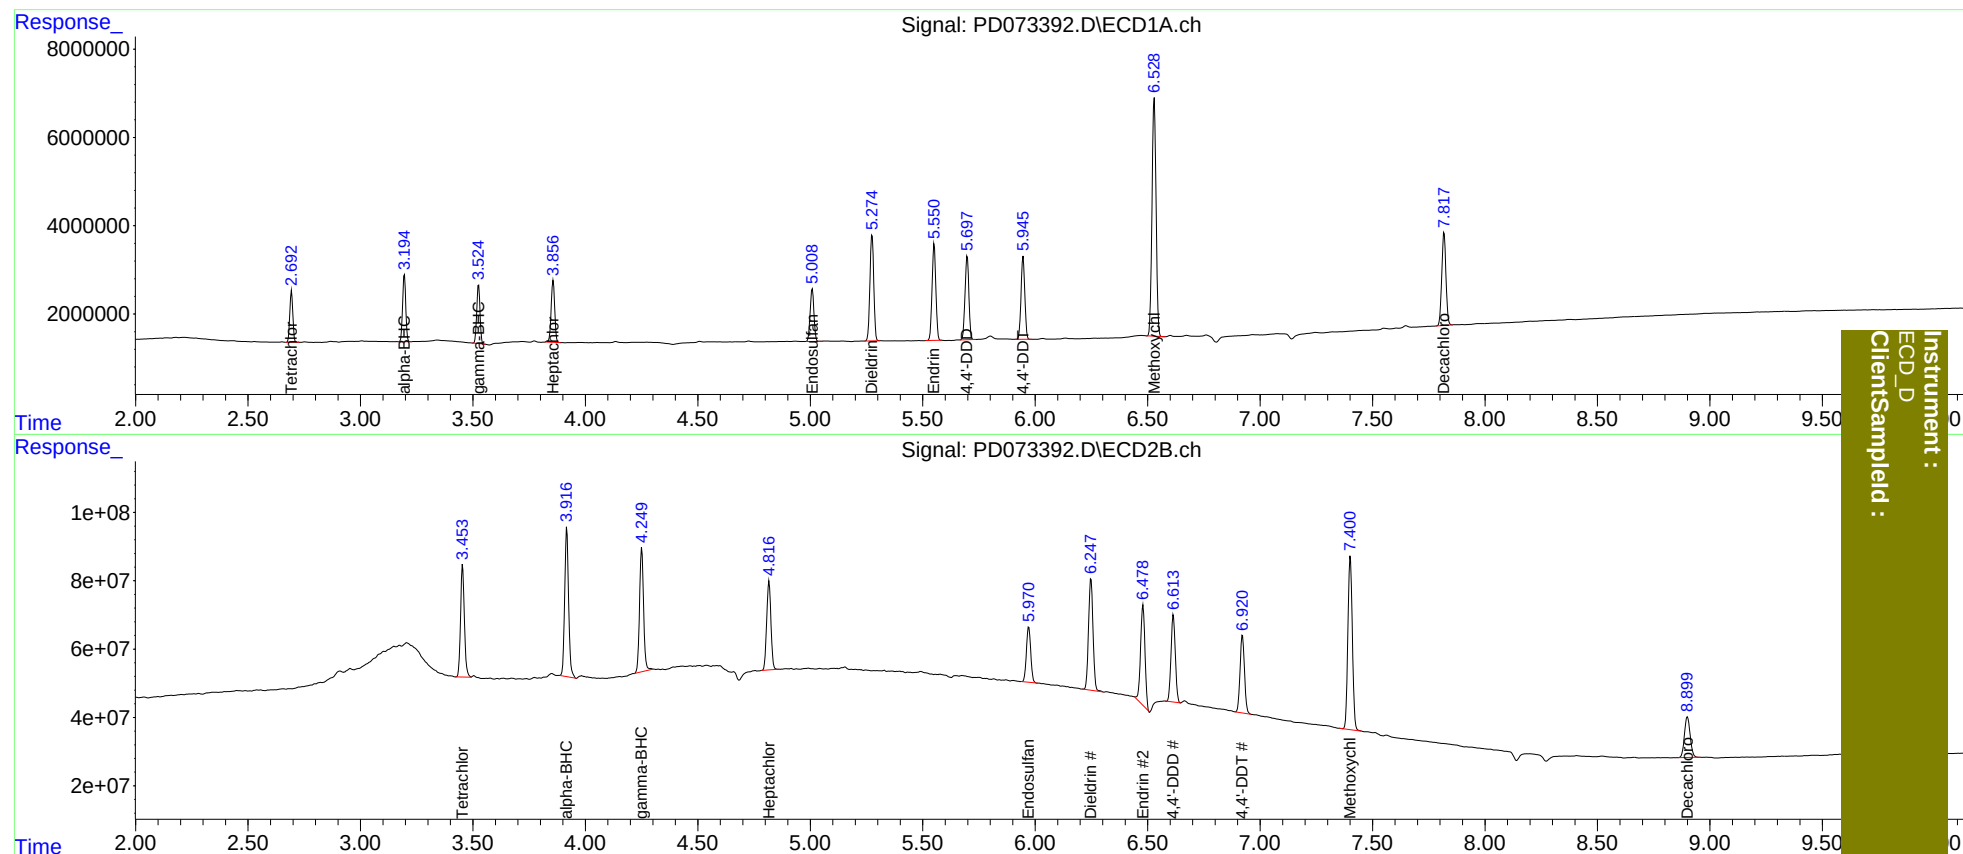


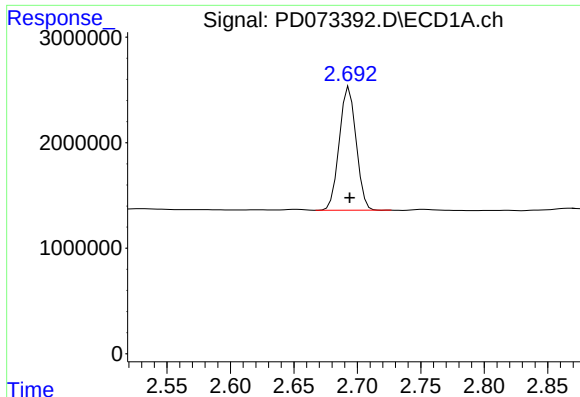

#1 Tetrachloro-m-xylene


R.T.: 2.694 min
Delta R.T.: 0.000 min
Response: 10795308
Conc: 5.45 ng/ml

Instrument :
ECD_D
ClientSampleId :

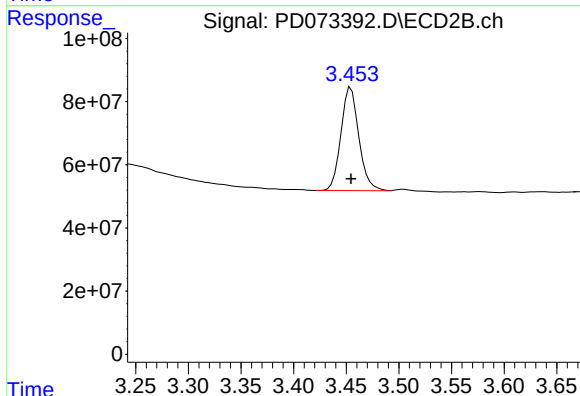


#1 Tetrachloro-m-xylene

R.T.: 3.454 min
Delta R.T.: 0.000 min
Response: 388741118
Conc: 6.12 ng/ml

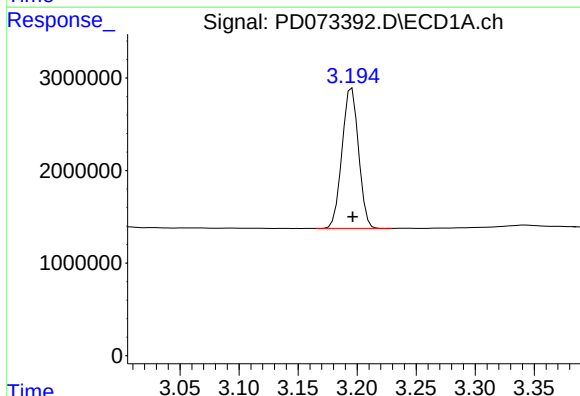


#2 alpha-BHC

R.T.: 3.196 min
Delta R.T.: 0.000 min
Response: 14775470
Conc: 4.81 ng/ml

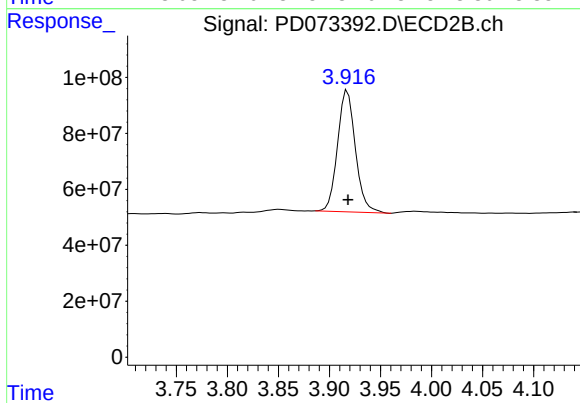

#2 alpha-BHC


R.T.: 3.918 min
Delta R.T.: 0.000 min
Response: 530785285
Conc: 6.37 ng/ml

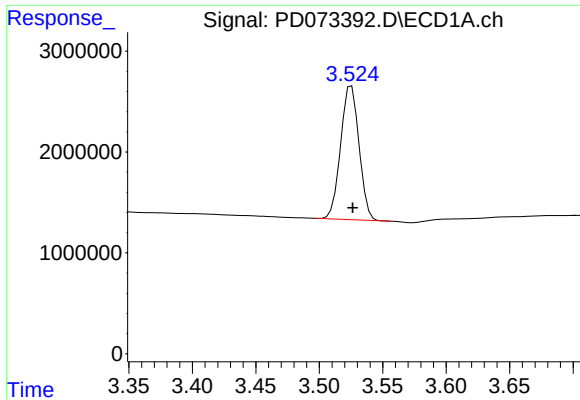

#3 gamma-BHC (Lindane)


R.T.: 3.525 min
Delta R.T.: 0.000 min
Response: 13340613
Conc: 4.80 ng/ml

Instrument :
ECD_D
ClientSampleId :

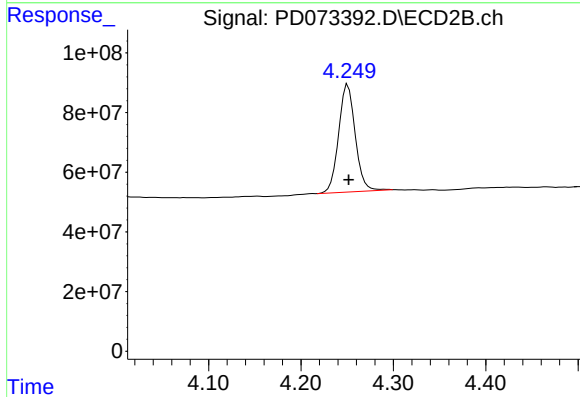


#3 gamma-BHC (Lindane)

R.T.: 4.251 min
Delta R.T.: 0.000 min
Response: 453651329
Conc: 6.55 ng/ml

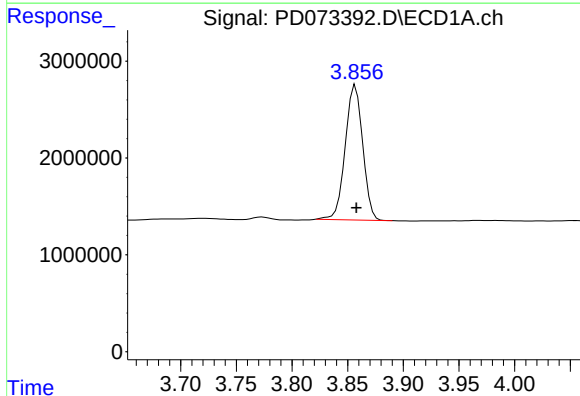


#4 Heptachlor

R.T.: 3.857 min
Delta R.T.: 0.000 min
Response: 15224512
Conc: 5.12 ng/ml

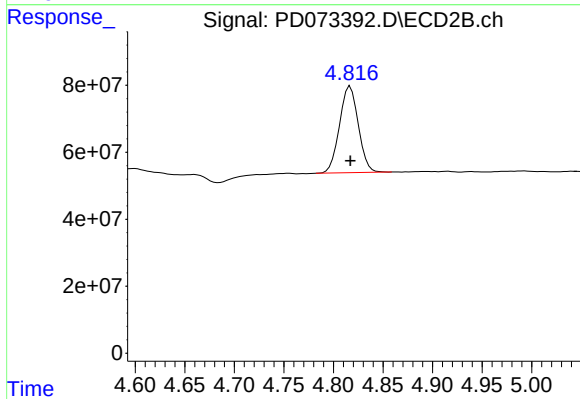

#4 Heptachlor


R.T.: 4.817 min
Delta R.T.: 0.000 min
Response: 341365005
Conc: 6.11 ng/ml

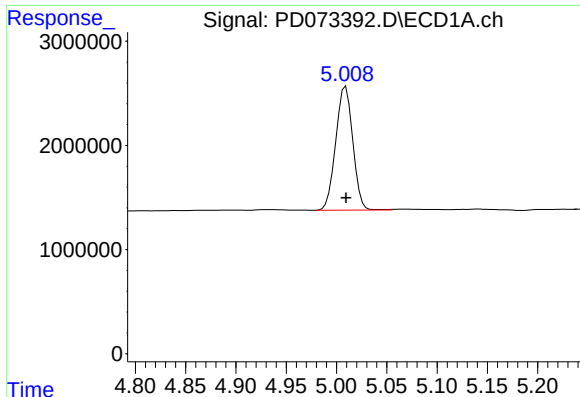

#9 Endosulfan I


R.T.: 5.009 min
Delta R.T.: 0.000 min
Response: 13991586
Conc: 5.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

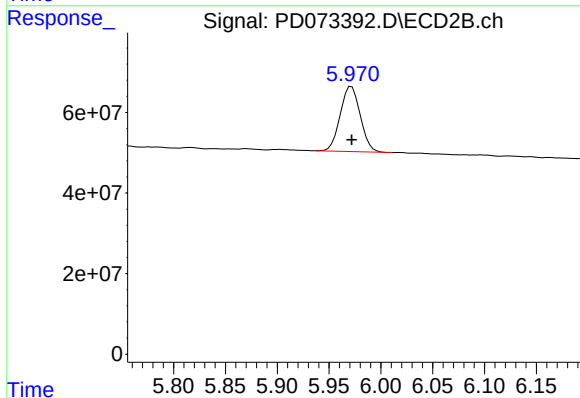


#9 Endosulfan I

R.T.: 5.972 min
Delta R.T.: 0.000 min
Response: 216619179
Conc: 5.70 ng/ml

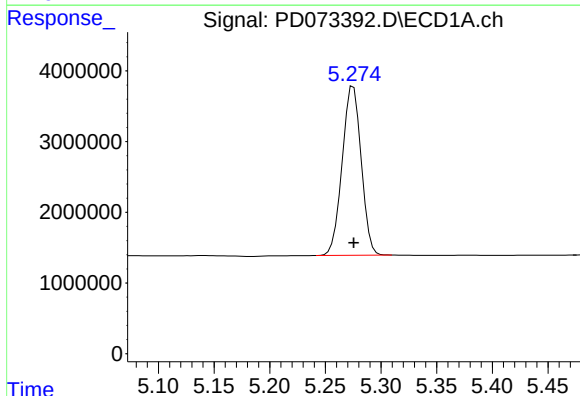


#13 Dieldrin

R.T.: 5.275 min
Delta R.T.: 0.000 min
Response: 28436125
Conc: 9.71 ng/ml

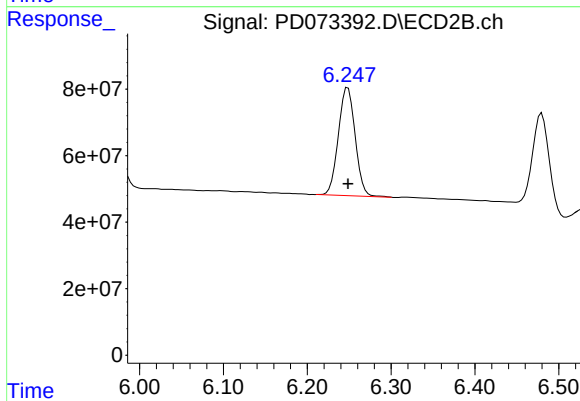

#13 Dieldrin


R.T.: 6.248 min
Delta R.T.: 0.000 min
Response: 452788605
Conc: 11.27 ng/ml

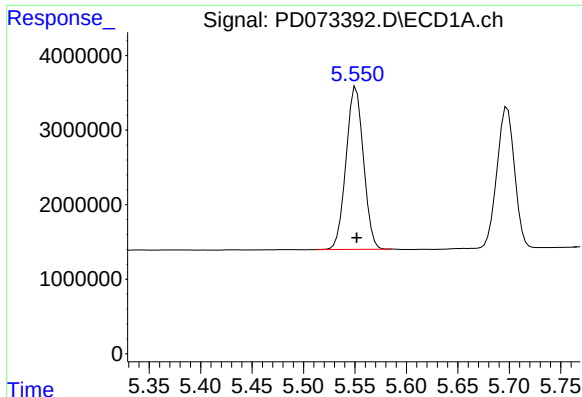

#14 Endrin


R.T.: 5.551 min
Delta R.T.: 0.000 min
Response: 25718100
Conc: 9.94 ng/ml

Instrument :
ECD_D
ClientSampleId :

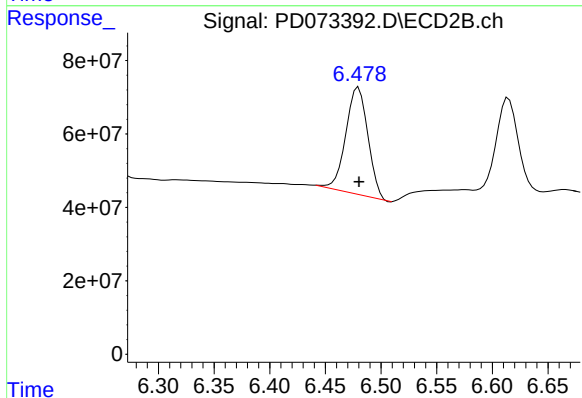


#14 Endrin

R.T.: 6.480 min
Delta R.T.: 0.000 min
Response: 404743565
Conc: 12.21 ng/ml

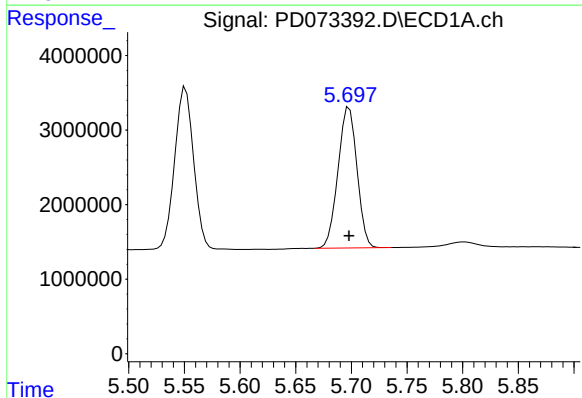


#16 4,4'-DDD

R.T.: 5.698 min
Delta R.T.: 0.000 min
Response: 22434351
Conc: 9.75 ng/ml

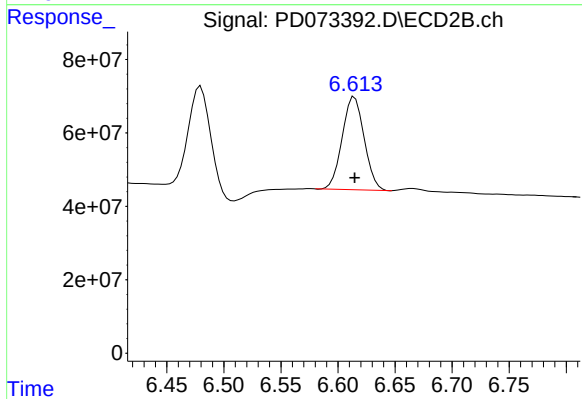

#16 4,4'-DDD


R.T.: 6.614 min
Delta R.T.: 0.000 min
Response: 339640789
Conc: 11.36 ng/ml

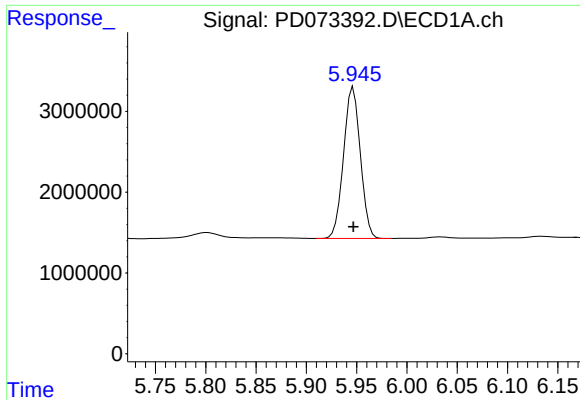

#17 4,4'-DDT


R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 21744759
Conc: 9.45 ng/ml

Instrument :
ECD_D
ClientSampleId :

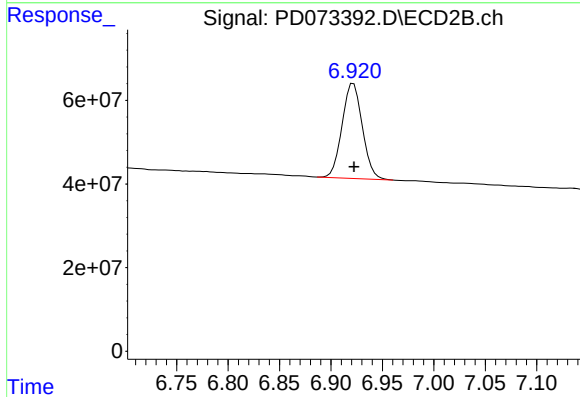


#17 4,4'-DDT

R.T.: 6.922 min
Delta R.T.: 0.000 min
Response: 311401095
Conc: 10.86 ng/ml

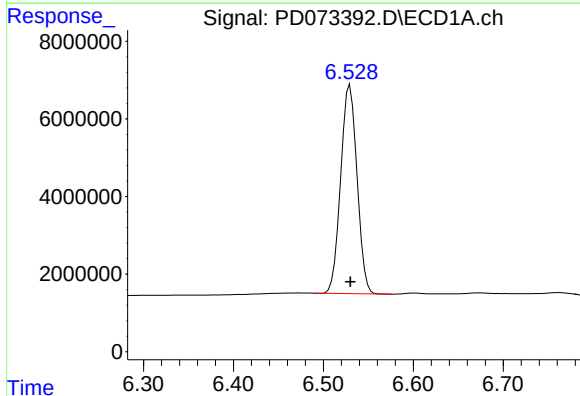


#20 Methoxychlor

R.T.: 6.530 min
Delta R.T.: 0.000 min
Response: 67858188
Conc: 52.43 ng/ml

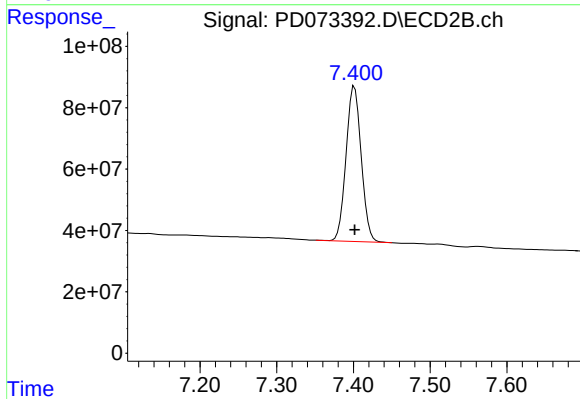

#20 Methoxychlor


R.T.: 7.401 min
Delta R.T.: 0.000 min
Response: 698115261
Conc: 56.87 ng/ml

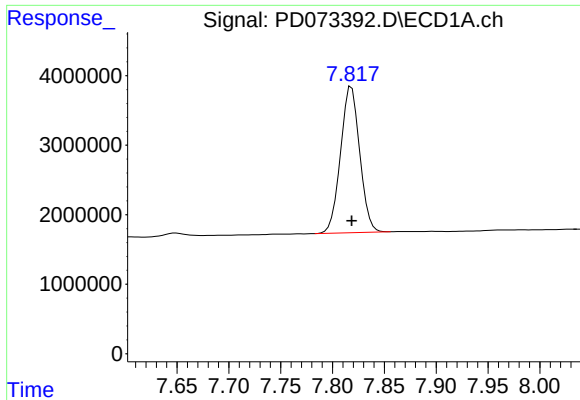

#27 Decachlorobiphenyl

R.T.: 7.818 min
Delta R.T.: 0.000 min
Response: 27045133
Conc: 11.25 ng/ml

Instrument :
ECD_D
ClientSampleId :

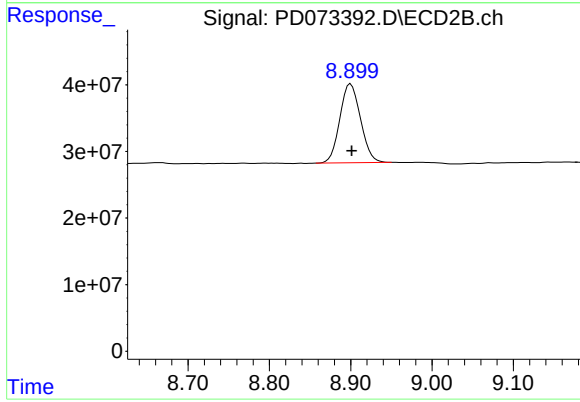

#27 Decachlorobiphenyl

R.T.: 8.900 min
Delta R.T.: -0.001 min
Response: 209275184
Conc: 11.05 ng/ml