

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122122\
 Data File : PD073394.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2022 13:47
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 03:49:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122122CLP.M
 Quant Title : GC Extractables
 QLast Update : Sun Dec 25 03:42:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.694	3.455	20915716	727.0E6	10.566	11.442
27)	SA Decachlor...	7.818	8.902	51109729	401.7E6	21.268	21.209
Target Compounds							
2)	A alpha-BHC	3.196	3.918	30210711	987.8E6	9.835	11.848
3)	MA gamma-BHC...	3.526	4.251	27315233	812.5E6	9.818	11.727
4)	MA Heptachlor	3.858	4.817	30072987	620.9E6	10.123	11.115
9)	A Endosulfan I	5.009	5.972	26934207	406.0E6	10.157	10.691
13)	MA Dieldrin	5.275	6.249	57130934	858.6E6	19.503	21.379
14)	MA Endrin	5.552	6.480	51306459	723.6E6	19.836	21.831
16)	A 4,4'-DDD	5.699	6.614	43160796	635.7E6	18.761	21.263
17)	MA 4,4'-DDT	5.947	6.922	44025301	601.0E6	19.136	20.961
20)	A Methoxychlor	6.530	7.402	132.7E6	1322.8E6	102.543	107.753


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122122\
Data File : PD073394.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2022 13:47
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 03:49:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122122CLP.M
Quant Title : GC Extractables
QLast Update : Sun Dec 25 03:42:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

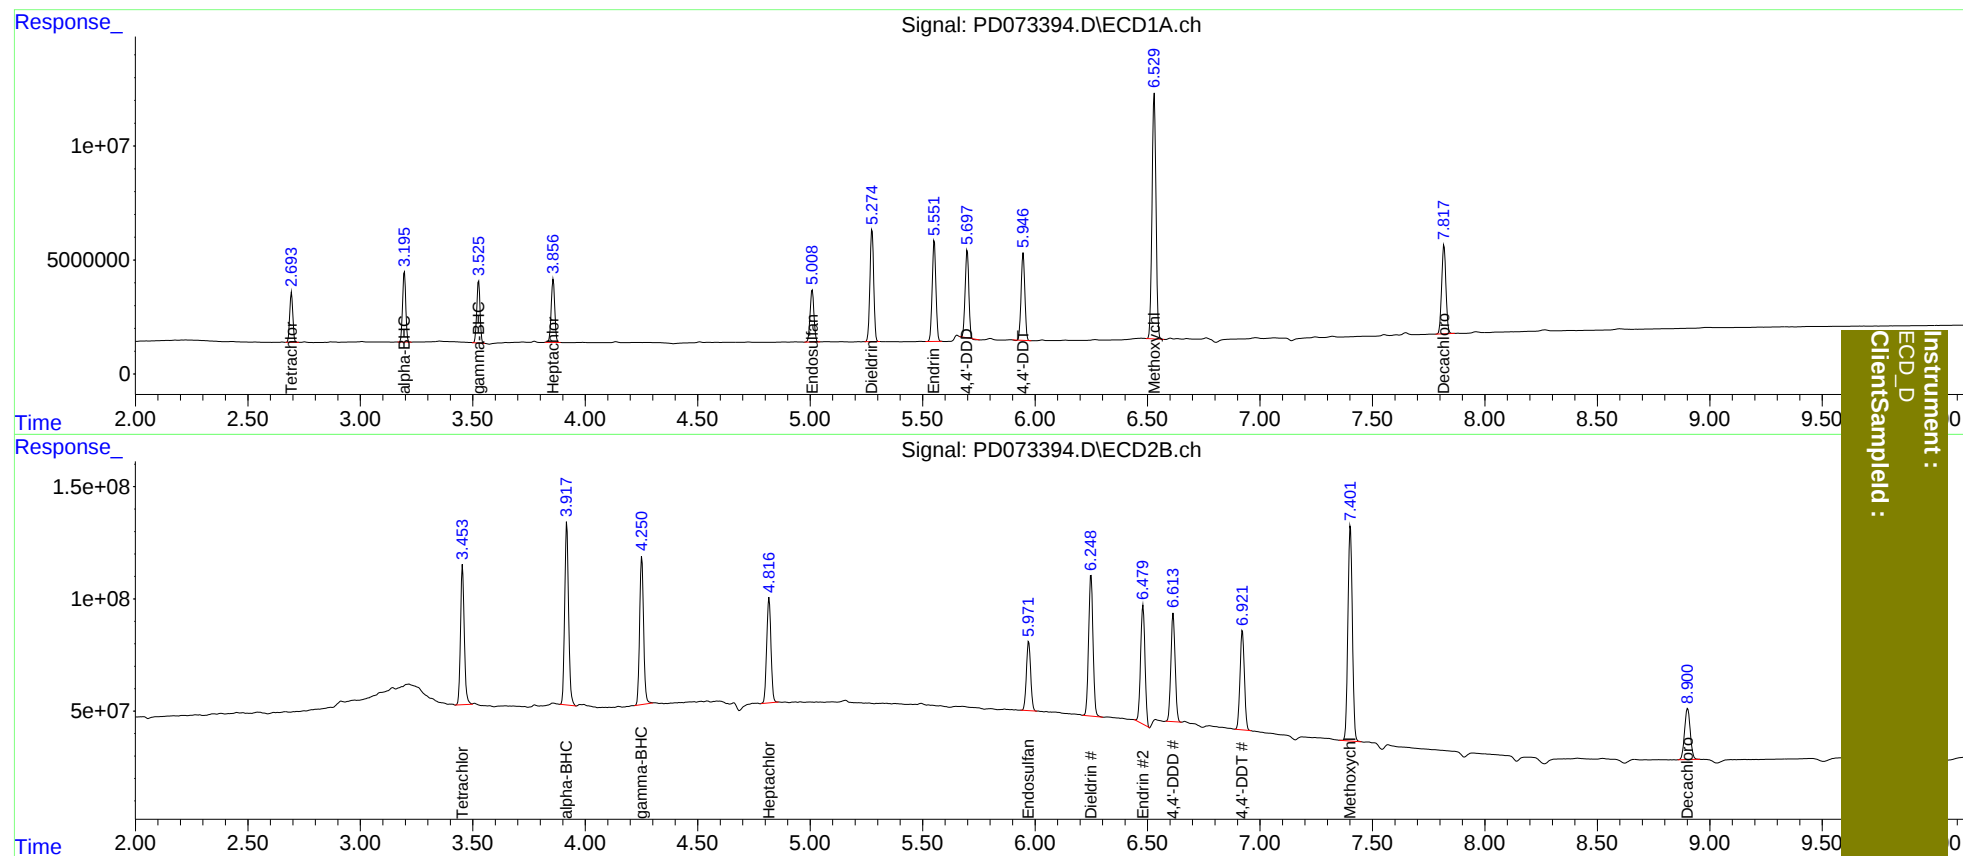


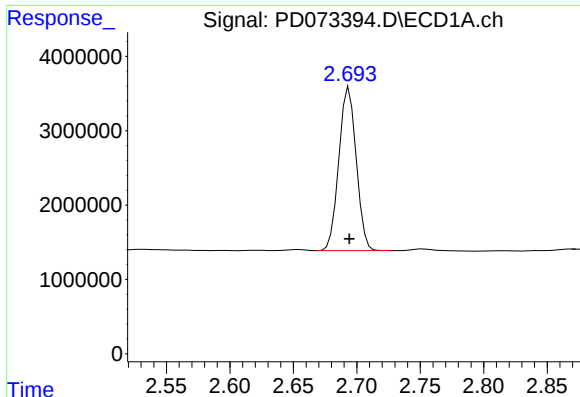

#1 Tetrachloro-m-xylene


R.T.: 2.694 min
Delta R.T.: 0.000 min
Response: 20915716
Conc: 10.57 ng/ml

Instrument :
ECD_D
ClientSampleId :

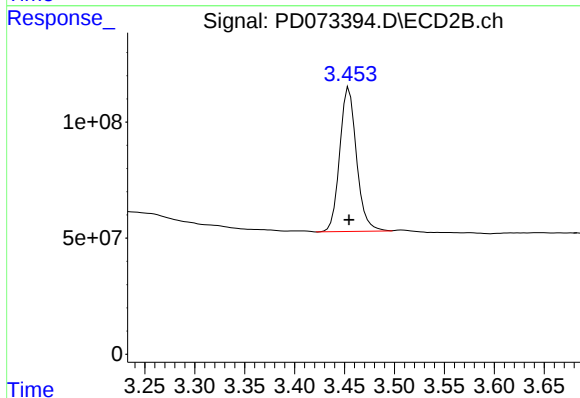


#1 Tetrachloro-m-xylene

R.T.: 3.455 min
Delta R.T.: 0.000 min
Response: 726994219
Conc: 11.44 ng/ml

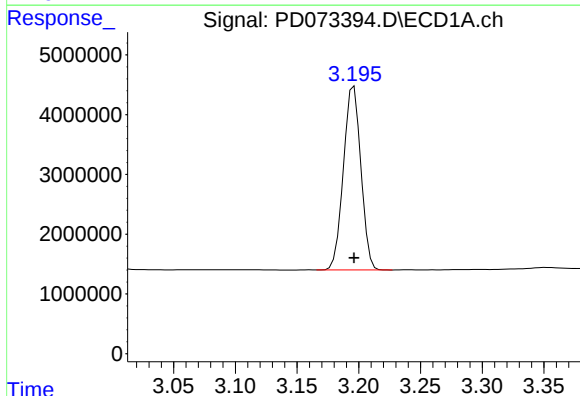


#2 alpha-BHC

R.T.: 3.196 min
Delta R.T.: 0.000 min
Response: 30210711
Conc: 9.83 ng/ml

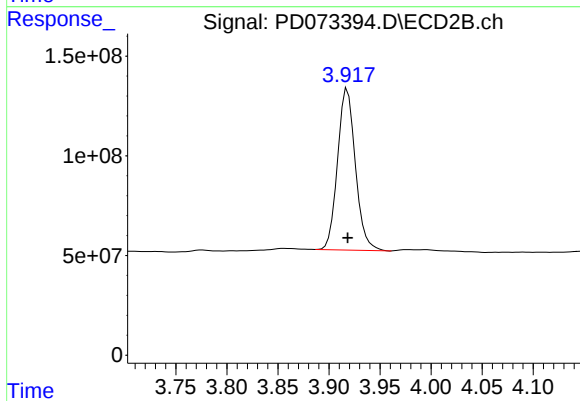

#2 alpha-BHC


R.T.: 3.918 min
Delta R.T.: 0.000 min
Response: 987787493
Conc: 11.85 ng/ml

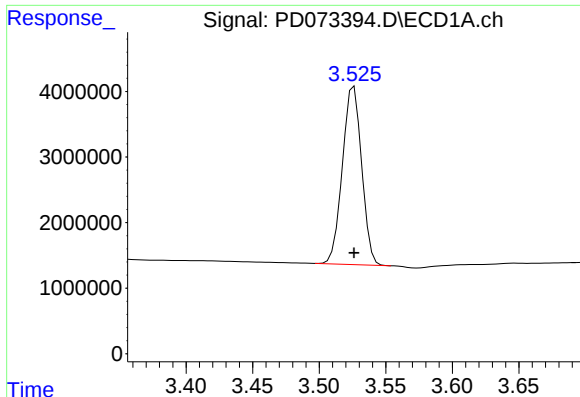

#3 gamma-BHC (Lindane)


R.T.: 3.526 min
Delta R.T.: 0.000 min
Response: 27315233
Conc: 9.82 ng/ml

Instrument :
ECD_D
ClientSampleId :

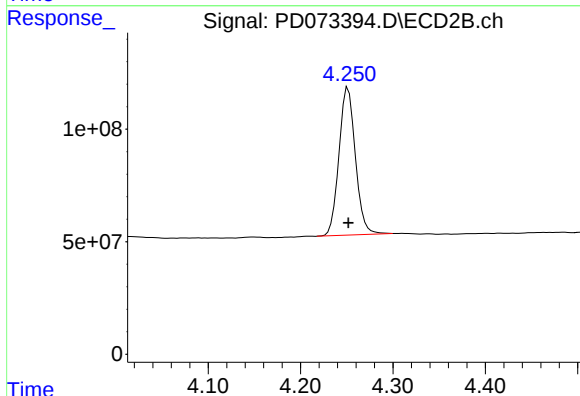


#3 gamma-BHC (Lindane)

R.T.: 4.251 min
Delta R.T.: 0.000 min
Response: 812478384
Conc: 11.73 ng/ml

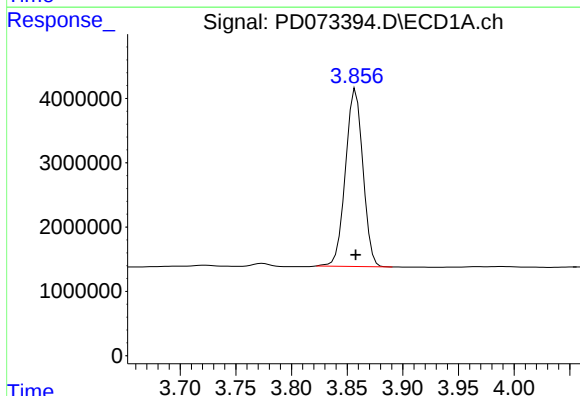


#4 Heptachlor

R.T.: 3.858 min
Delta R.T.: 0.000 min
Response: 30072987
Conc: 10.12 ng/ml

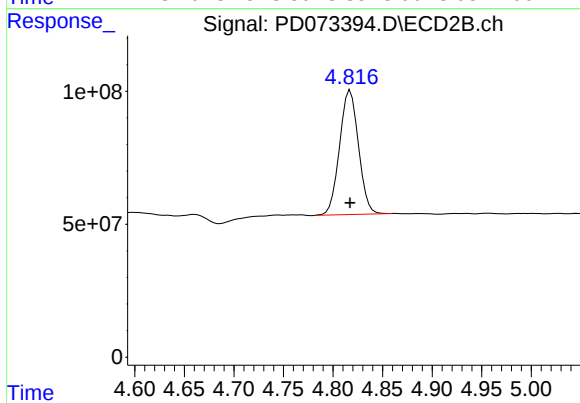

#4 Heptachlor


R.T.: 4.817 min
Delta R.T.: 0.000 min
Response: 620909595
Conc: 11.12 ng/ml

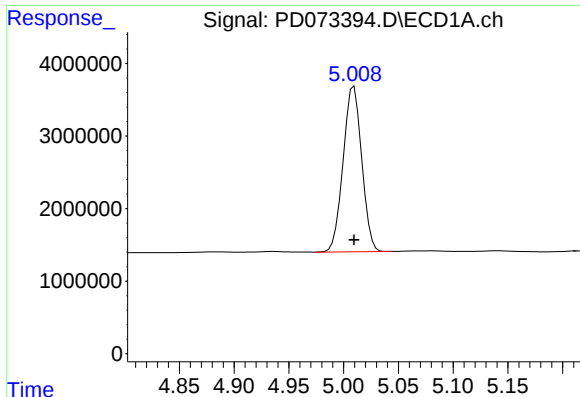

#9 Endosulfan I


R.T.: 5.009 min
Delta R.T.: 0.000 min
Response: 26934207
Conc: 10.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

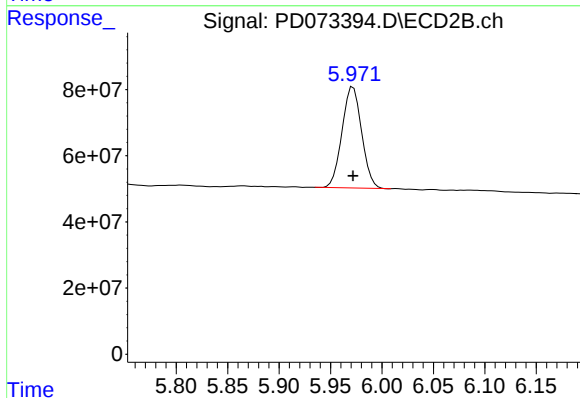


#9 Endosulfan I

R.T.: 5.972 min
Delta R.T.: 0.000 min
Response: 406001496
Conc: 10.69 ng/ml

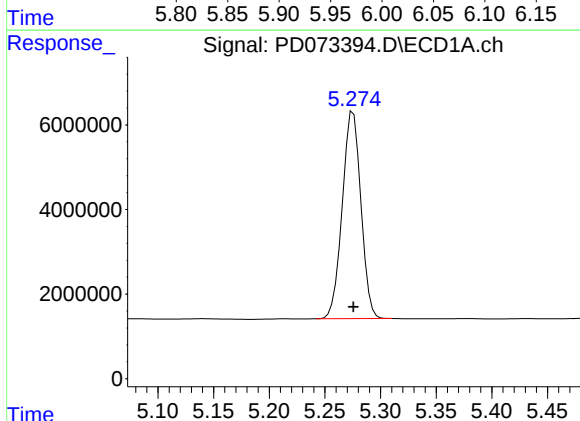


#13 Dieldrin

R.T.: 5.275 min
Delta R.T.: 0.000 min
Response: 57130934
Conc: 19.50 ng/ml

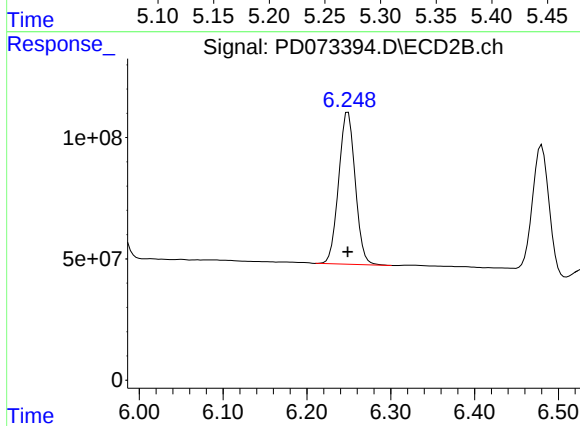

#13 Dieldrin


R.T.: 6.249 min
Delta R.T.: 0.000 min
Response: 858618584
Conc: 21.38 ng/ml

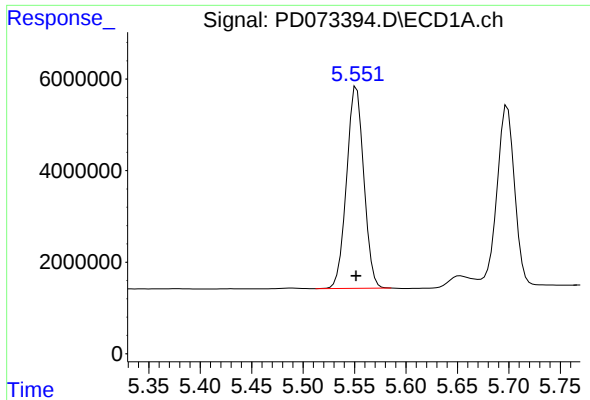

#14 Endrin


R.T.: 5.552 min
Delta R.T.: 0.000 min
Response: 51306459
Conc: 19.84 ng/ml

Instrument :
ECD_D
ClientSampleId :

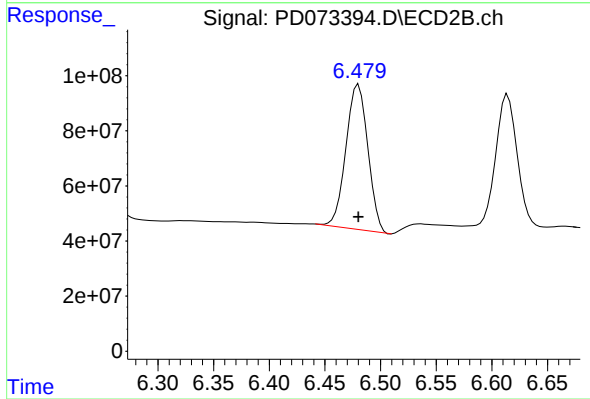


#14 Endrin

R.T.: 6.480 min
Delta R.T.: 0.000 min
Response: 723599134
Conc: 21.83 ng/ml

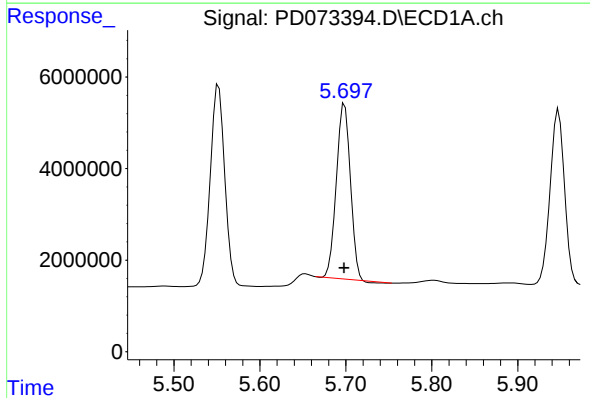


#16 4,4'-DDD

R.T.: 5.699 min
Delta R.T.: 0.000 min
Response: 43160796
Conc: 18.76 ng/ml

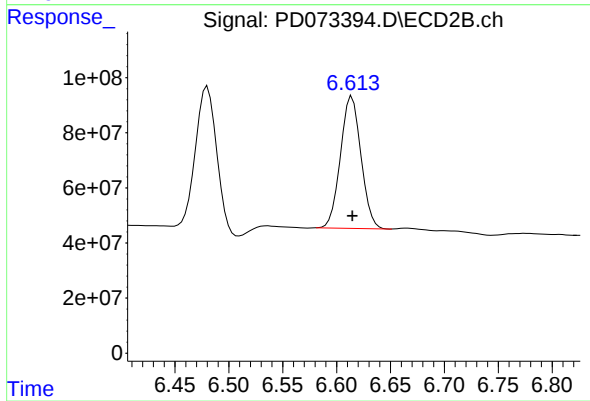

#16 4,4'-DDD


R.T.: 6.614 min
Delta R.T.: 0.000 min
Response: 635665971
Conc: 21.26 ng/ml

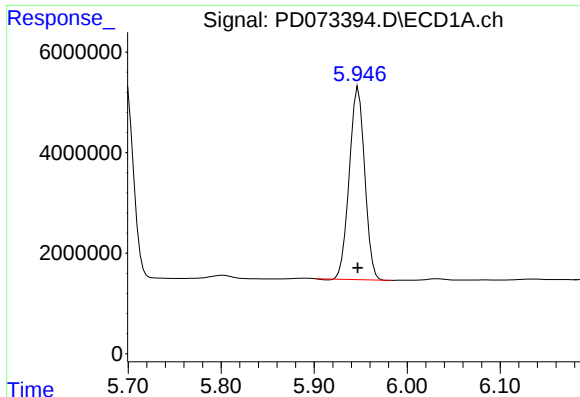

#17 4,4'-DDT


R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 44025301
Conc: 19.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

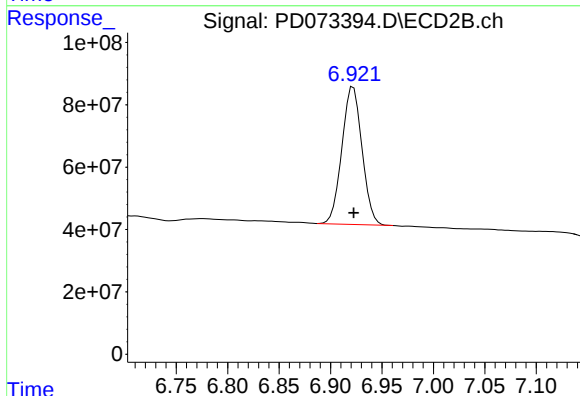


#17 4,4'-DDT

R.T.: 6.922 min
Delta R.T.: 0.000 min
Response: 600952224
Conc: 20.96 ng/ml

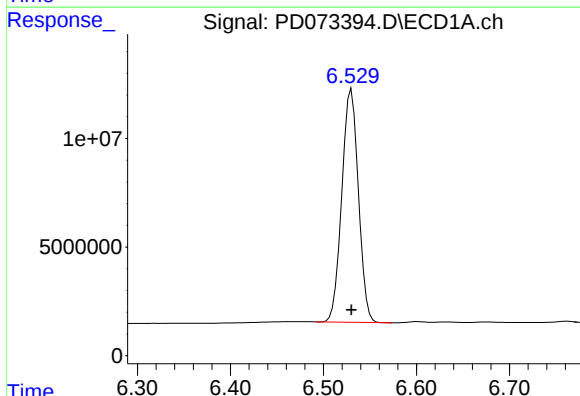


#20 Methoxychlor

R.T.: 6.530 min
Delta R.T.: 0.000 min
Response: 132723393
Conc: 102.54 ng/ml

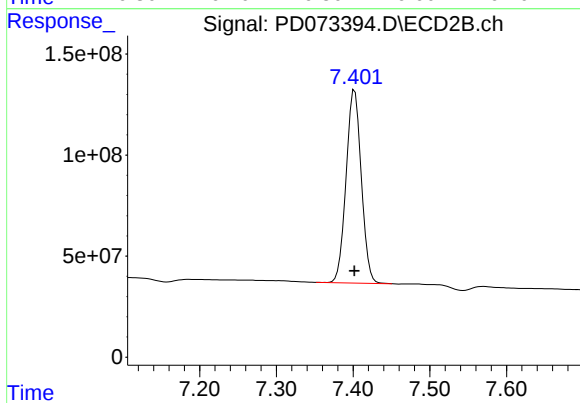

#20 Methoxychlor


R.T.: 7.402 min
Delta R.T.: 0.000 min
Response: 1322771491
Conc: 107.75 ng/ml

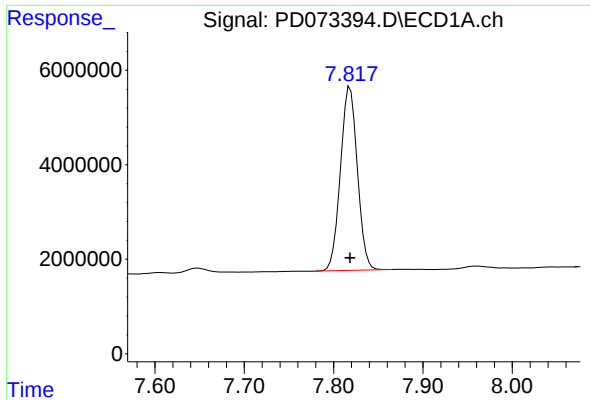

#27 Decachlorobiphenyl

R.T.: 7.818 min
Delta R.T.: 0.000 min
Response: 51109729
Conc: 21.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

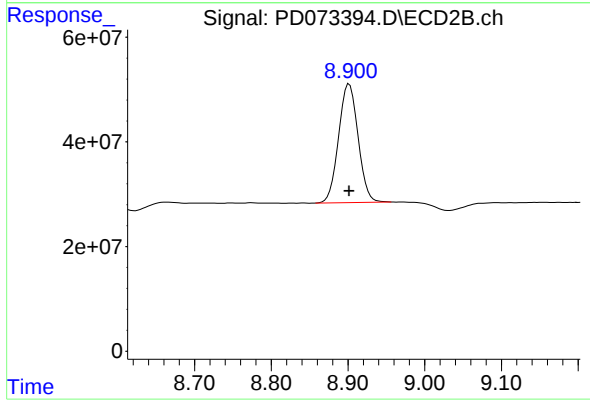

#27 Decachlorobiphenyl

R.T.: 8.902 min
Delta R.T.: 0.000 min
Response: 401717614
Conc: 21.21 ng/ml