

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122122\
 Data File : PD073396.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2022 14:13
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 03:49:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122122CLP.M
 Quant Title : GC Extractables
 QLast Update : Sun Dec 25 03:42:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.694	3.455	39590338	1270.7E6	20.000	20.000
27)	SA Decachlor...	7.819	8.901	96125799	757.6E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.196	3.918	61436817	1667.5E6	20.000	20.000
3)	MA gamma-BHC...	3.526	4.252	55640989	1385.6E6	20.000	20.000
4)	MA Heptachlor	3.858	4.817	59413431	1117.2E6	20.000	20.000
9)	A Endosulfan I	5.009	5.972	53034458	759.5E6	20.000	20.000
13)	MA Dieldrin	5.276	6.249	117.2E6	1606.4E6	40.000	40.000
14)	MA Endrin	5.551	6.480	103.5E6	1325.8E6	40.000	40.000
16)	A 4,4'-DDD	5.698	6.615	92023816	1195.8E6	40.000	40.000
17)	MA 4,4'-DDT	5.947	6.923	92023968	1146.8E6	40.000	40.000
20)	A Methoxychlor	6.530	7.402	258.9E6	2455.2E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122122\
Data File : PD073396.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2022 14:13
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 03:49:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122122CLP.M
Quant Title : GC Extractables
QLast Update : Sun Dec 25 03:42:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

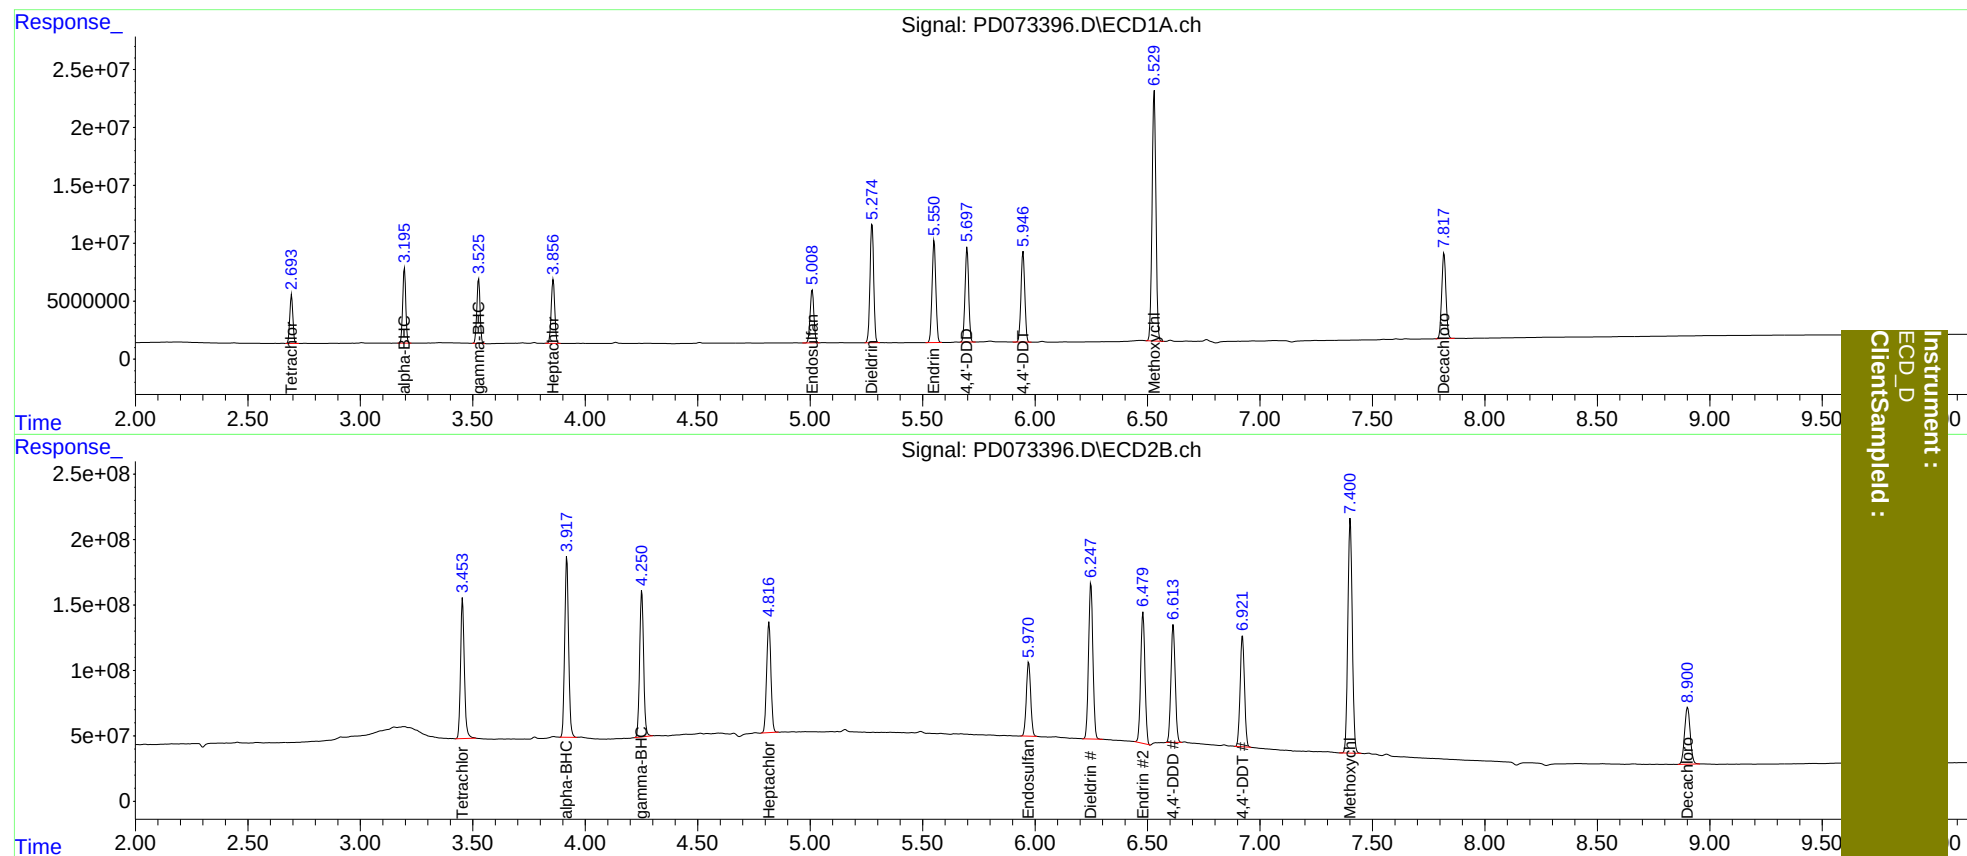


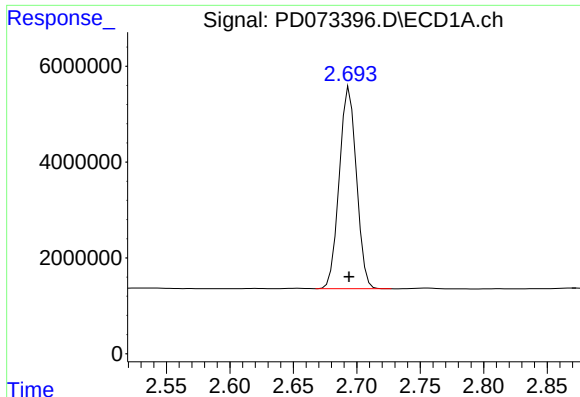

#1 Tetrachloro-m-xylene


R.T.: 2.694 min
Delta R.T.: 0.000 min
Response: 39590338
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

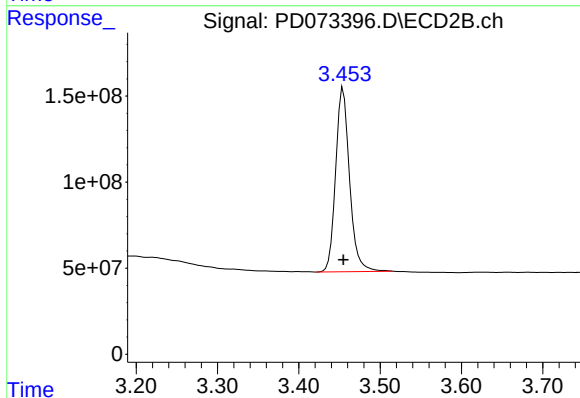


#1 Tetrachloro-m-xylene

R.T.: 3.455 min
Delta R.T.: 0.000 min
Response: 1270735666
Conc: 20.00 ng/ml

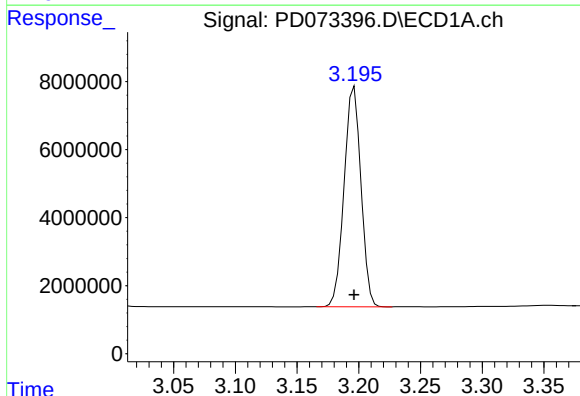


#2 alpha-BHC

R.T.: 3.196 min
Delta R.T.: 0.000 min
Response: 61436817
Conc: 20.00 ng/ml

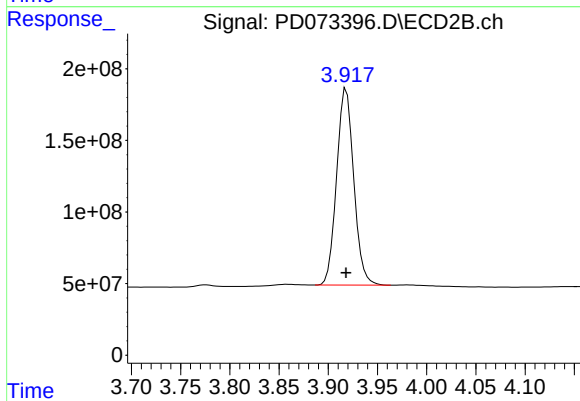

#2 alpha-BHC


R.T.: 3.918 min
Delta R.T.: 0.000 min
Response: 1667452712
Conc: 20.00 ng/ml

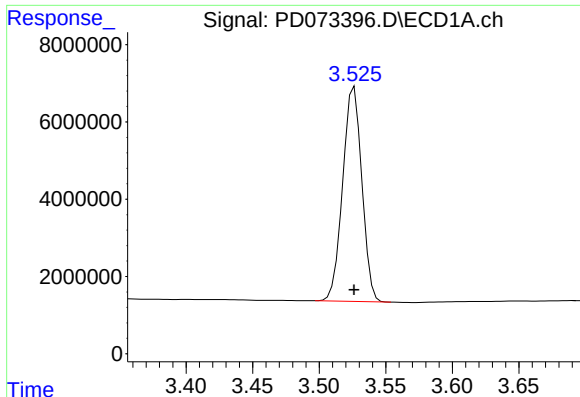

#3 gamma-BHC (Lindane)


R.T.: 3.526 min
Delta R.T.: 0.000 min
Response: 55640989
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

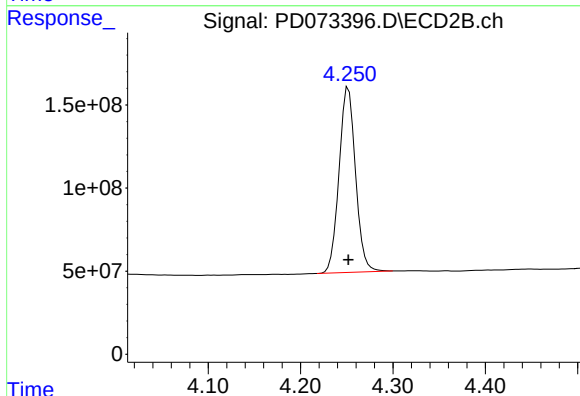


#3 gamma-BHC (Lindane)

R.T.: 4.252 min
Delta R.T.: 0.000 min
Response: 1385604518
Conc: 20.00 ng/ml

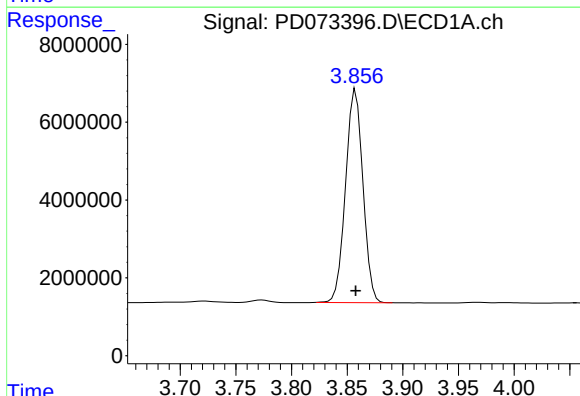


#4 Heptachlor

R.T.: 3.858 min
Delta R.T.: 0.000 min
Response: 59413431
Conc: 20.00 ng/ml

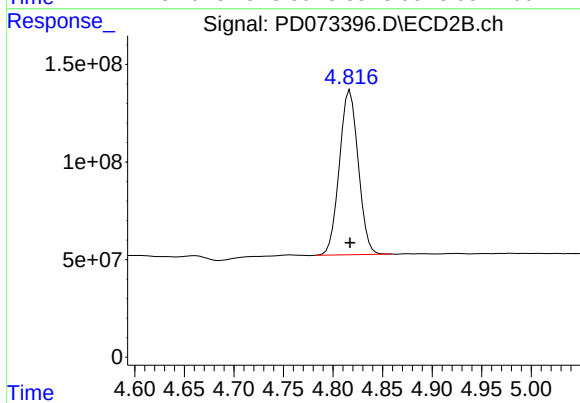

#4 Heptachlor


R.T.: 4.817 min
Delta R.T.: 0.000 min
Response: 1117223112
Conc: 20.00 ng/ml

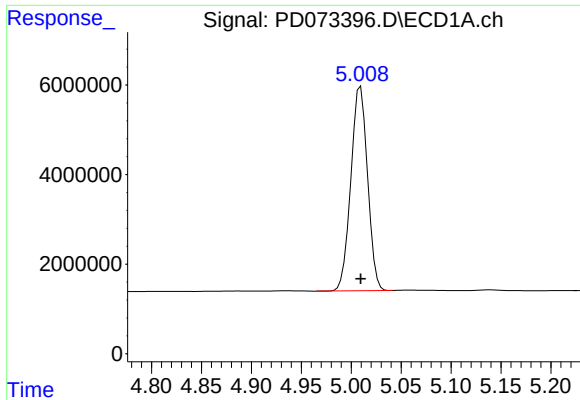

#9 Endosulfan I


R.T.: 5.009 min
Delta R.T.: 0.000 min
Response: 53034458
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

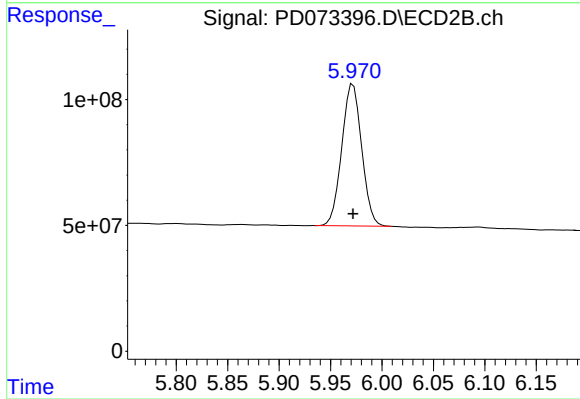


#9 Endosulfan I

R.T.: 5.972 min
Delta R.T.: 0.000 min
Response: 759537527
Conc: 20.00 ng/ml

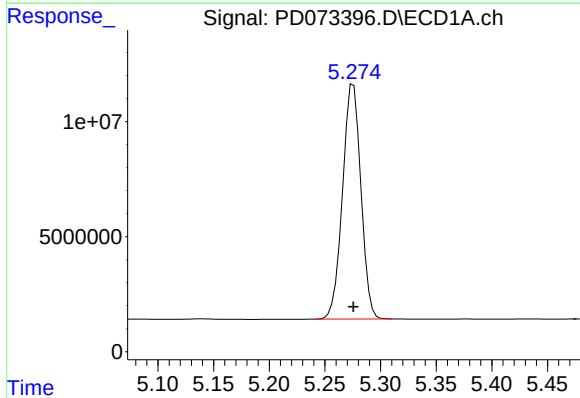


#13 Dieldrin

R.T.: 5.276 min
Delta R.T.: 0.000 min
Response: 117170695
Conc: 40.00 ng/ml

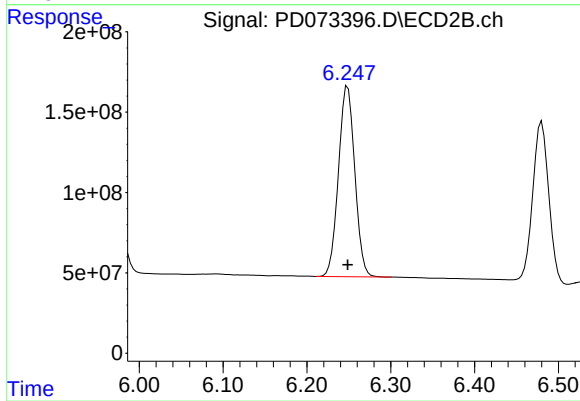

#13 Dieldrin


R.T.: 6.249 min
Delta R.T.: 0.000 min
Response: 1606443866
Conc: 40.00 ng/ml

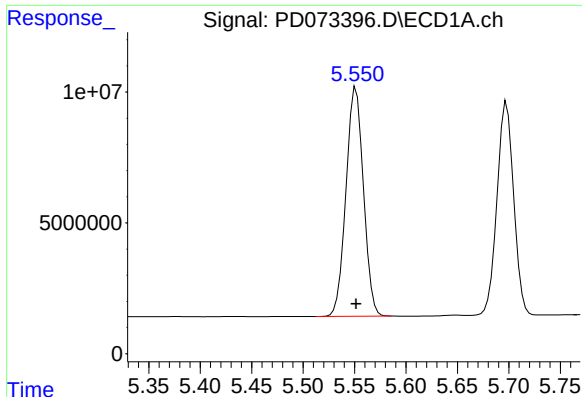

#14 Endrin


R.T.: 5.551 min
Delta R.T.: 0.000 min
Response: 103463140
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

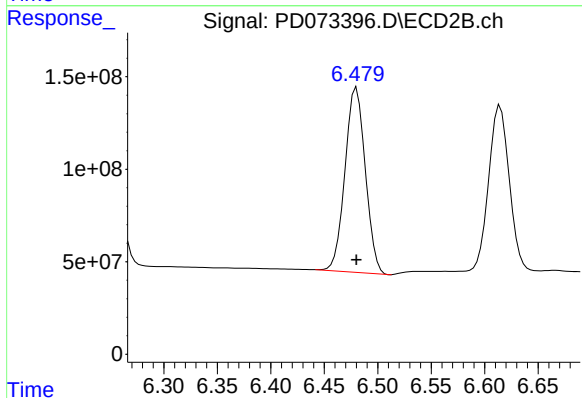


#14 Endrin

R.T.: 6.480 min
Delta R.T.: 0.000 min
Response: 1325824940
Conc: 40.00 ng/ml

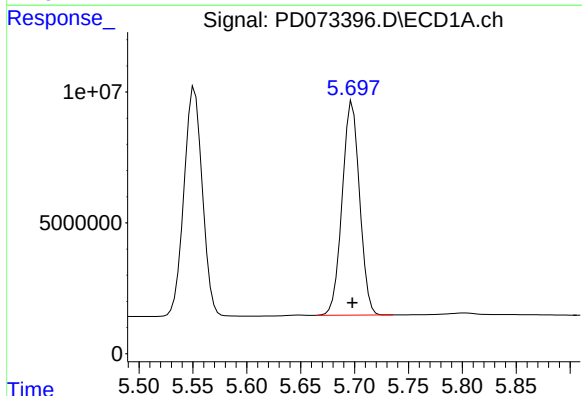


#16 4,4'-DDD

R.T.: 5.698 min
Delta R.T.: 0.000 min
Response: 92023816
Conc: 40.00 ng/ml

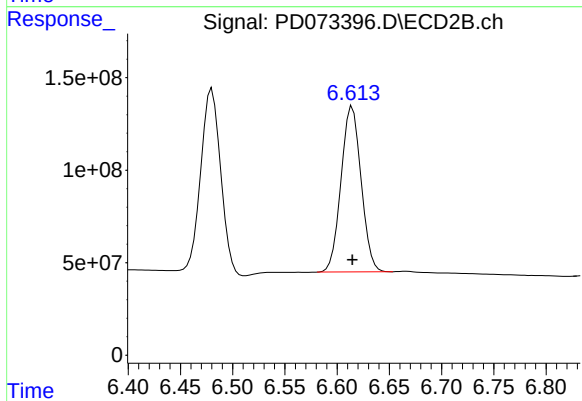

#16 4,4'-DDD


R.T.: 6.615 min
Delta R.T.: 0.000 min
Response: 1195829855
Conc: 40.00 ng/ml

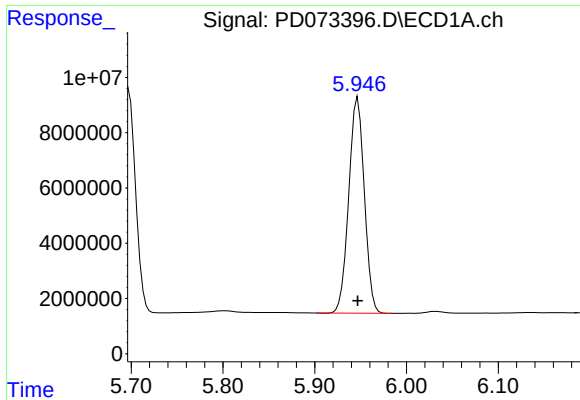

#17 4,4'-DDT


R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 92023968
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

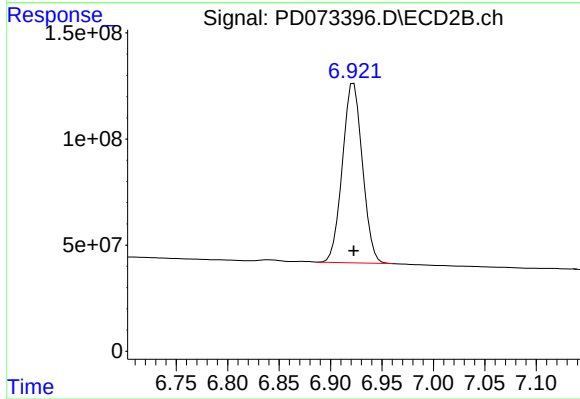


#17 4,4'-DDT

R.T.: 6.923 min
Delta R.T.: 0.000 min
Response: 1146805478
Conc: 40.00 ng/ml

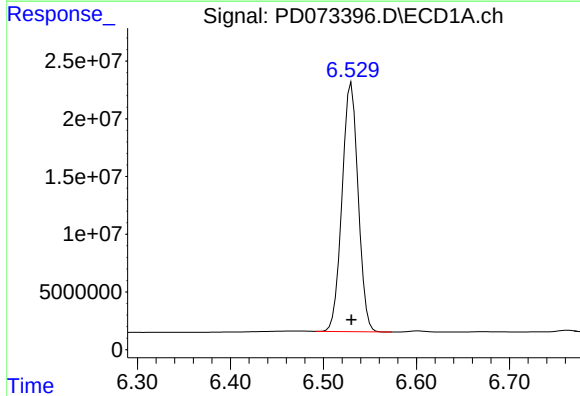


#20 Methoxychlor

R.T.: 6.530 min
Delta R.T.: 0.000 min
Response: 258863237
Conc: 200.00 ng/ml

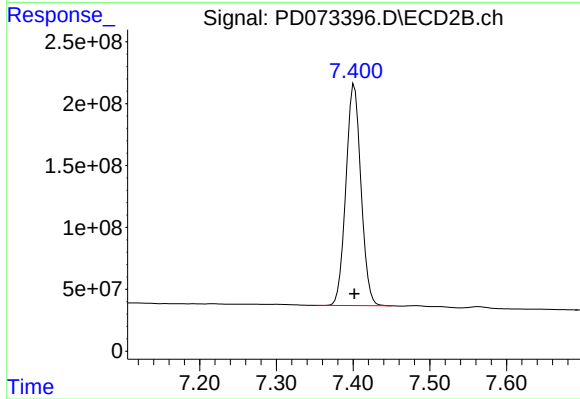

#20 Methoxychlor


R.T.: 7.402 min
Delta R.T.: 0.000 min
Response: 2455192843
Conc: 200.00 ng/ml

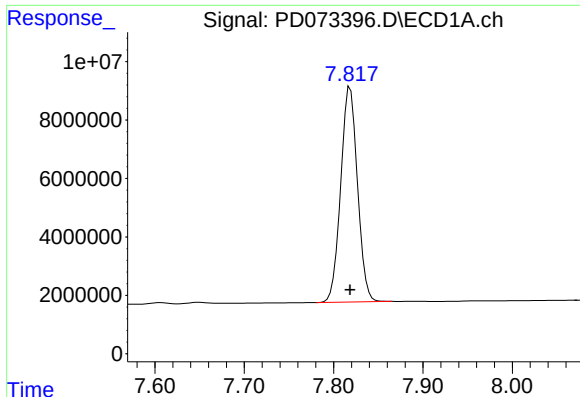

#27 Decachlorobiphenyl

R.T.: 7.819 min
Delta R.T.: 0.000 min
Response: 96125799
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

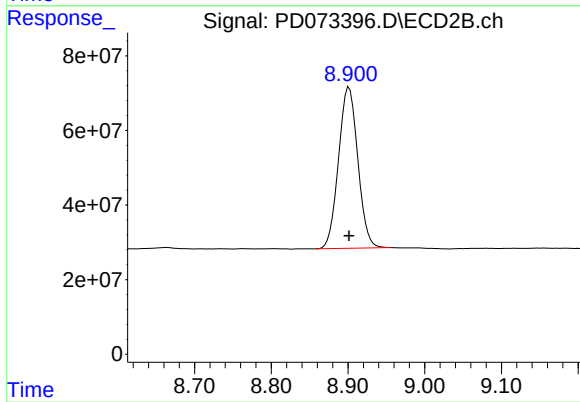

#27 Decachlorobiphenyl

R.T.: 8.901 min
Delta R.T.: 0.000 min
Response: 757625934
Conc: 40.00 ng/ml