

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122122\
 Data File : PD073398.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2022 14:50
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 03:49:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122122CLP.M
 Quant Title : GC Extractables
 QLast Update : Sun Dec 25 03:42:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.701	3.454	80778975	3335.4E6	40.807	52.496 #
27)	SA Decachlor...	7.825	8.903	185.6E6	1488.9E6	77.221	78.609
Target Compounds							
2)	A alpha-BHC	3.204	3.917	131.8E6	4317.8E6	42.916	51.789
3)	MA gamma-BHC...	3.534	4.251	122.8E6	3245.1E6	44.152	46.840
4)	MA Heptachlor	3.866	4.817	129.5E6	2261.0E6	43.592	40.475
9)	A Endosulfan I	5.017	5.971	106.6E6	1518.1E6	40.182	39.974
13)	MA Dieldrin	5.283	6.248	241.2E6	3270.5E6	82.328	81.435
14)	MA Endrin	5.559	6.480	210.5E6	2345.2E6	81.395	70.753
16)	A 4,4'-DDD	5.706	6.614	187.7E6	2389.0E6	81.570	79.910
17)	MA 4,4'-DDT	5.954	6.923	193.6E6	2361.2E6	84.142	82.359
20)	A Methoxychlor	6.537	7.402	511.4E6	4808.9E6	395.090	391.735

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122122\
Data File : PD073398.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2022 14:50
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 03:49:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122122CLP.M
Quant Title : GC Extractables
QLast Update : Sun Dec 25 03:42:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

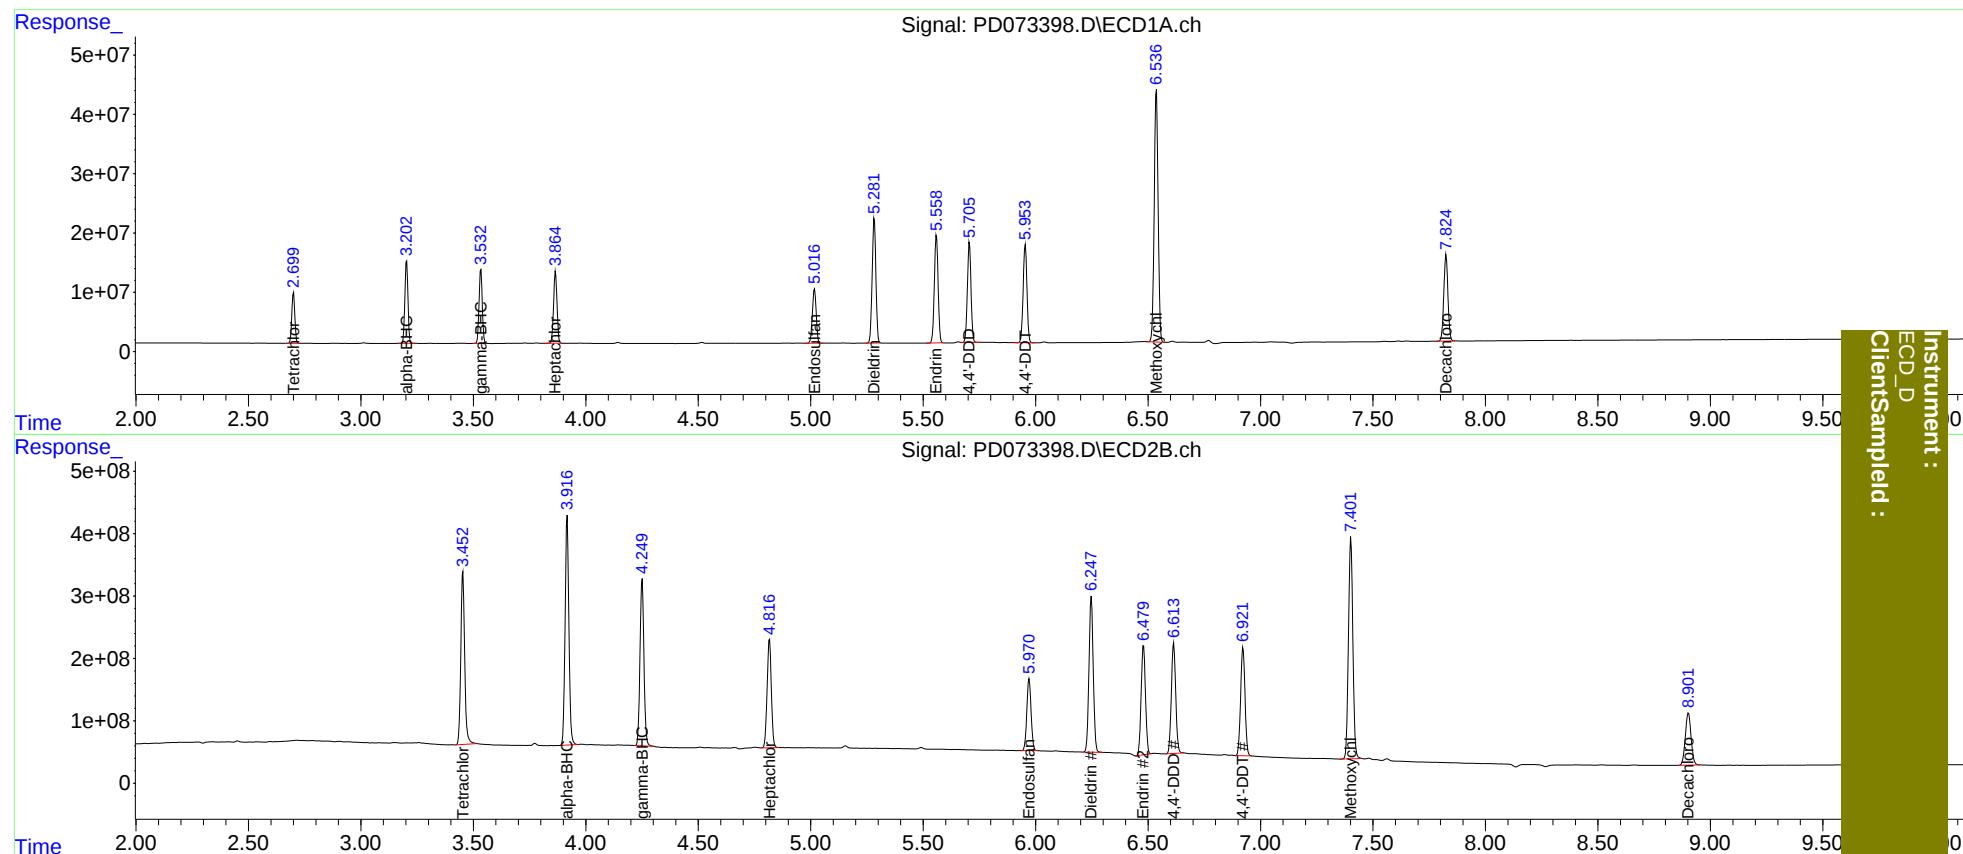


Instrument :
ECD_D
ClientSampled :
0

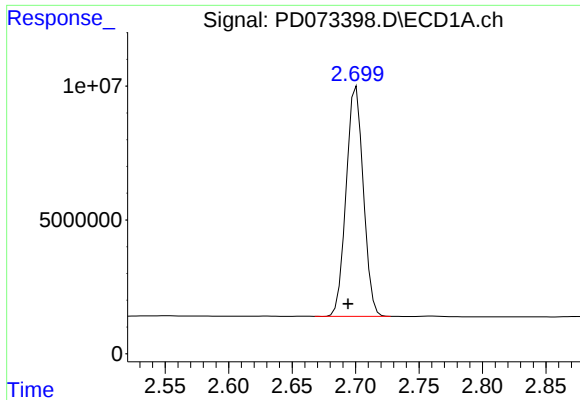

#1 Tetrachloro-m-xylene


R.T.: 2.701 min
Delta R.T.: 0.007 min
Response: 80778975
Conc: 40.81 ng/ml

Instrument :
ECD_D
ClientSampleId :

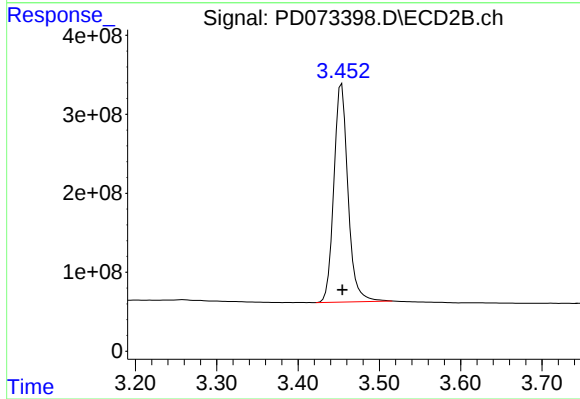


#1 Tetrachloro-m-xylene

R.T.: 3.454 min
Delta R.T.: 0.000 min
Response: 3335435307
Conc: 52.50 ng/ml

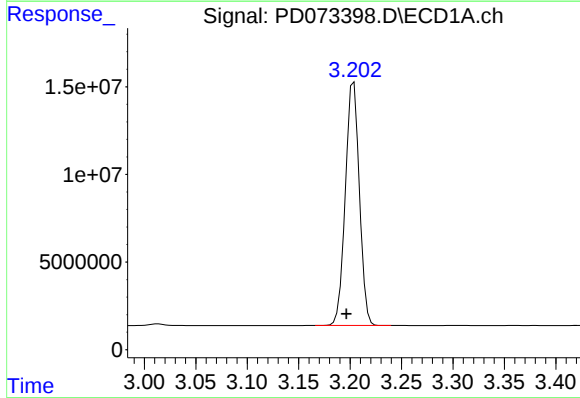


#2 alpha-BHC

R.T.: 3.204 min
Delta R.T.: 0.007 min
Response: 131830721
Conc: 42.92 ng/ml

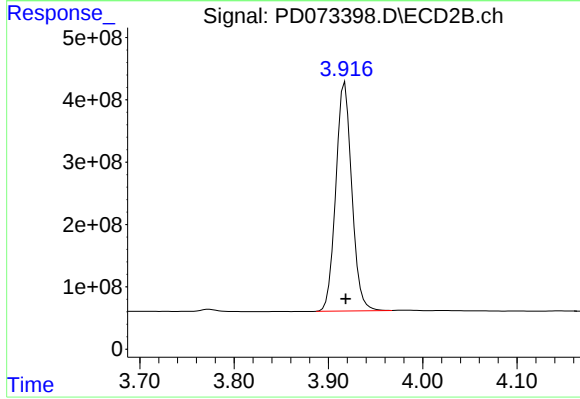

#2 alpha-BHC


R.T.: 3.917 min
Delta R.T.: 0.000 min
Response: 4317818673
Conc: 51.79 ng/ml

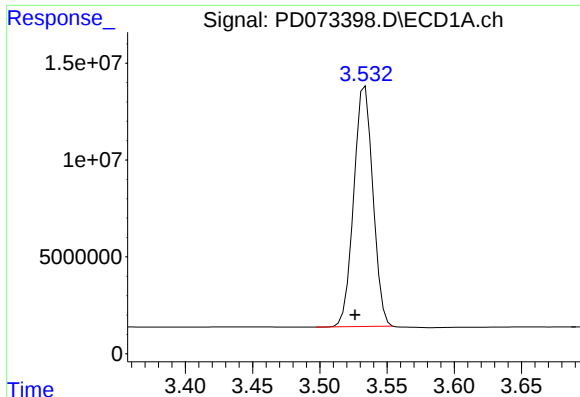

#3 gamma-BHC (Lindane)


R.T.: 3.534 min
Delta R.T.: 0.007 min
Response: 122832050
Conc: 44.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

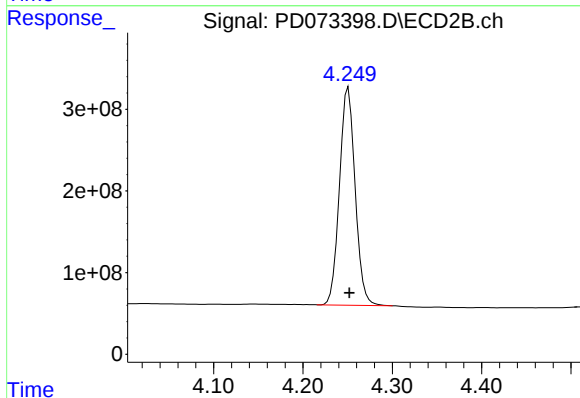


#3 gamma-BHC (Lindane)

R.T.: 4.251 min
Delta R.T.: 0.000 min
Response: 3245068745
Conc: 46.84 ng/ml

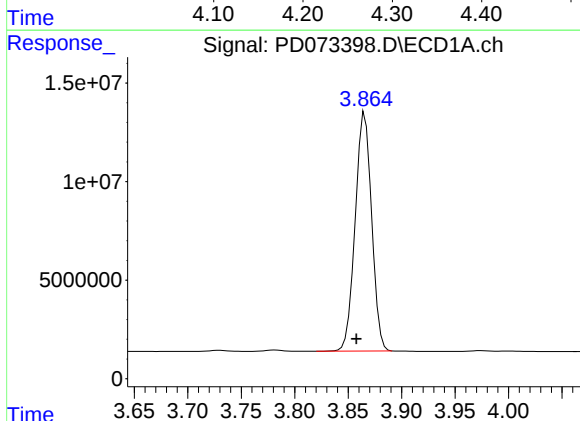


#4 Heptachlor

R.T.: 3.866 min
Delta R.T.: 0.008 min
Response: 129497888
Conc: 43.59 ng/ml

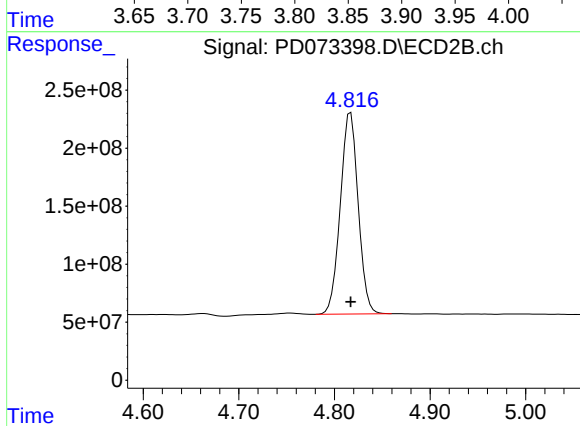

#4 Heptachlor


R.T.: 4.817 min
Delta R.T.: 0.000 min
Response: 2260995980
Conc: 40.48 ng/ml

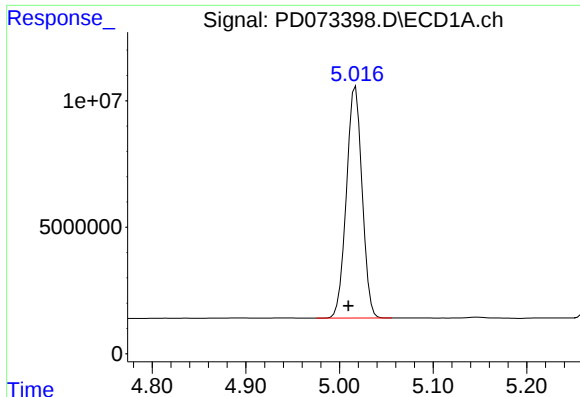

#9 Endosulfan I


R.T.: 5.017 min
Delta R.T.: 0.008 min
Response: 106550879
Conc: 40.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

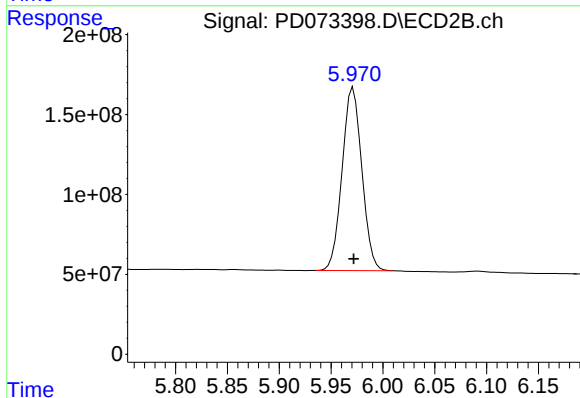


#9 Endosulfan I

R.T.: 5.971 min
Delta R.T.: 0.000 min
Response: 1518094111
Conc: 39.97 ng/ml

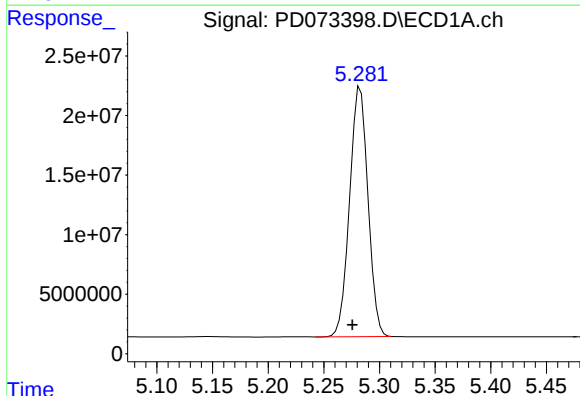


#13 Dieldrin

R.T.: 5.283 min
Delta R.T.: 0.007 min
Response: 241160174
Conc: 82.33 ng/ml

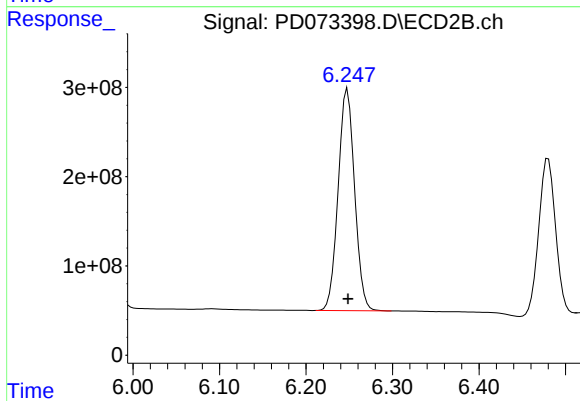

#13 Dieldrin


R.T.: 6.248 min
Delta R.T.: 0.000 min
Response: 3270535286
Conc: 81.44 ng/ml

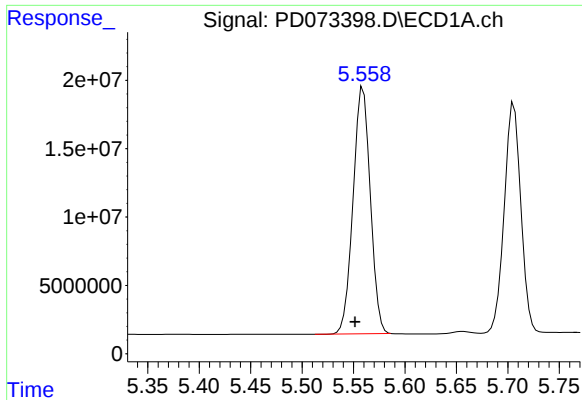

#14 Endrin


R.T.: 5.559 min
Delta R.T.: 0.008 min
Response: 210533709
Conc: 81.39 ng/ml

Instrument :
ECD_D
ClientSampleId :

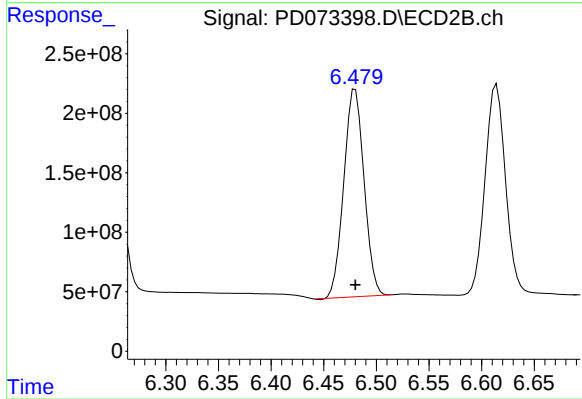


#14 Endrin

R.T.: 6.480 min
Delta R.T.: 0.000 min
Response: 2345168491
Conc: 70.75 ng/ml

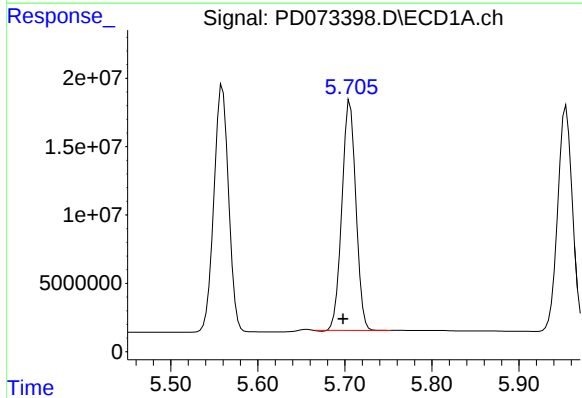


#16 4,4'-DDD

R.T.: 5.706 min
Delta R.T.: 0.008 min
Response: 187659743
Conc: 81.57 ng/ml

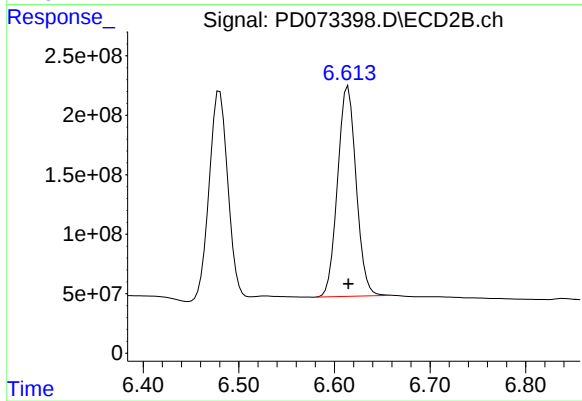

#16 4,4'-DDD


R.T.: 6.614 min
Delta R.T.: 0.000 min
Response: 2388968593
Conc: 79.91 ng/ml

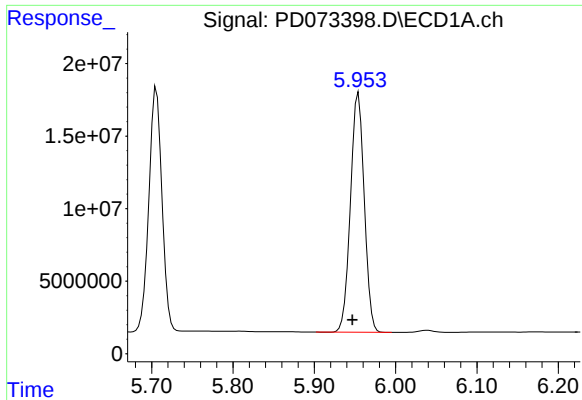

#17 4,4'-DDT


R.T.: 5.954 min
Delta R.T.: 0.007 min
Response: 193576948
Conc: 84.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

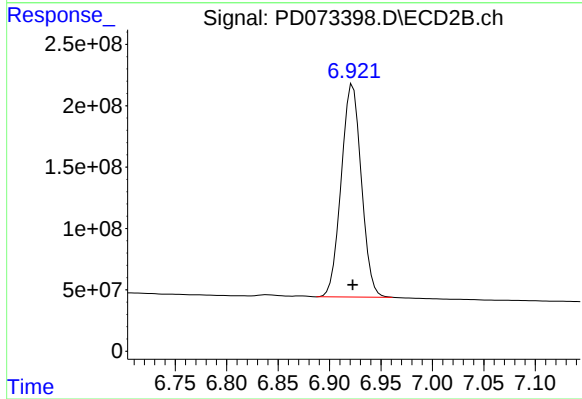


#17 4,4'-DDT

R.T.: 6.923 min
Delta R.T.: 0.000 min
Response: 2361236580
Conc: 82.36 ng/ml

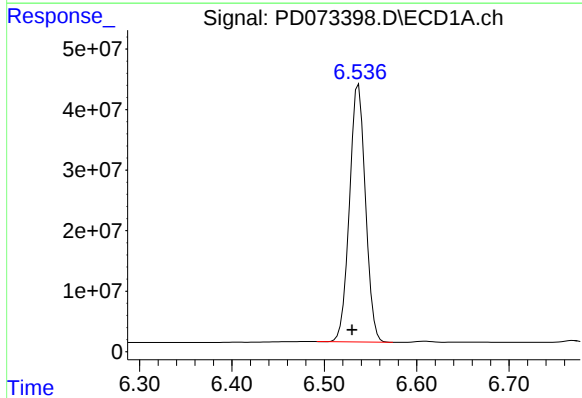


#20 Methoxychlor

R.T.: 6.537 min
Delta R.T.: 0.007 min
Response: 511371350
Conc: 395.09 ng/ml

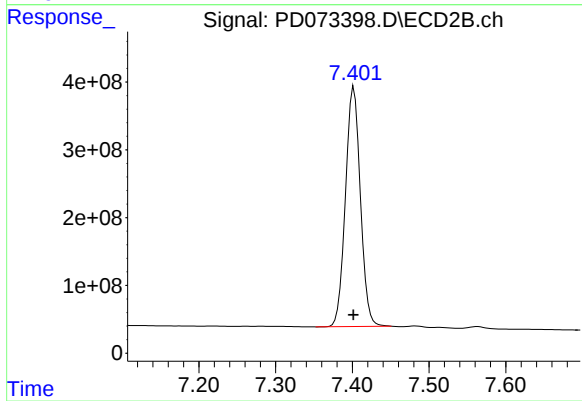

#20 Methoxychlor


R.T.: 7.402 min
Delta R.T.: 0.000 min
Response: 4808926340
Conc: 391.74 ng/ml

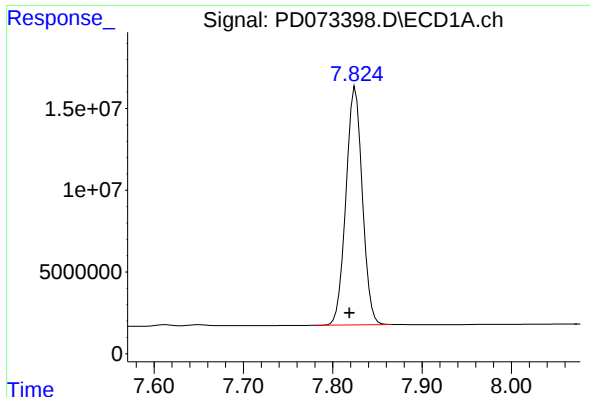

#27 Decachlorobiphenyl

R.T.: 7.825 min
Delta R.T.: 0.007 min
Response: 185574175
Conc: 77.22 ng/ml

Instrument :
ECD_D
ClientSampleId :

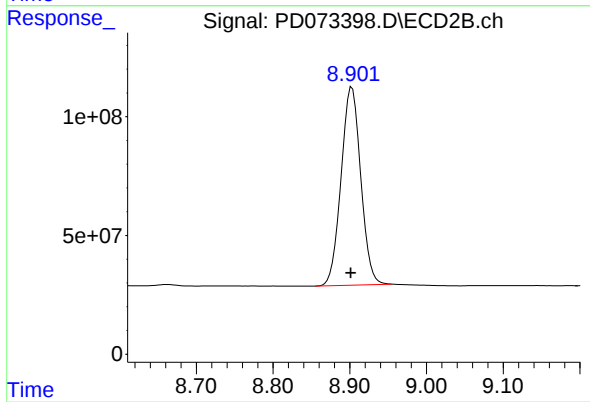

#27 Decachlorobiphenyl

R.T.: 8.903 min
Delta R.T.: 0.001 min
Response: 1488914194
Conc: 78.61 ng/ml