

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122122\
 Data File : PD073400.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2022 15:17
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 25 03:49:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122122CLP.M
 Quant Title : GC Extractables
 QLast Update : Sun Dec 25 03:42:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.694	3.455	162.4E6	5319.5E6	82.033	83.724
27)	SA Decachlor...	7.819	8.900	369.8E6	2900.2E6	153.882	153.122
Target Compounds							
2)	A alpha-BHC	3.196	3.919	283.7E6	8003.2E6	92.366	95.993
3)	MA gamma-BHC...	3.526	4.252	253.3E6	6391.5E6	91.040	92.256
4)	MA Heptachlor	3.858	4.817	266.2E6	4244.5E6	89.620	75.984
9)	A Endosulfan I	5.010	5.971	222.4E6	2877.4E6	83.873	75.766
13)	MA Dieldrin	5.276	6.248	508.5E6	6447.8E6	173.605	160.547
14)	MA Endrin	5.552	6.480	445.6E6	5120.7E6	172.293	154.490
16)	A 4,4'-DDD	5.699	6.614	397.4E6	4718.3E6	172.736	157.824
17)	MA 4,4'-DDT	5.947	6.921	410.2E6	4671.8E6	178.320	162.948
20)	A Methoxychlor	6.531	7.401	1007.6E6	8939.5E6	778.493	728.208

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122122\
Data File : PD073400.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2022 15:17
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 25 03:49:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122122CLP.M
Quant Title : GC Extractables
QLast Update : Sun Dec 25 03:42:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

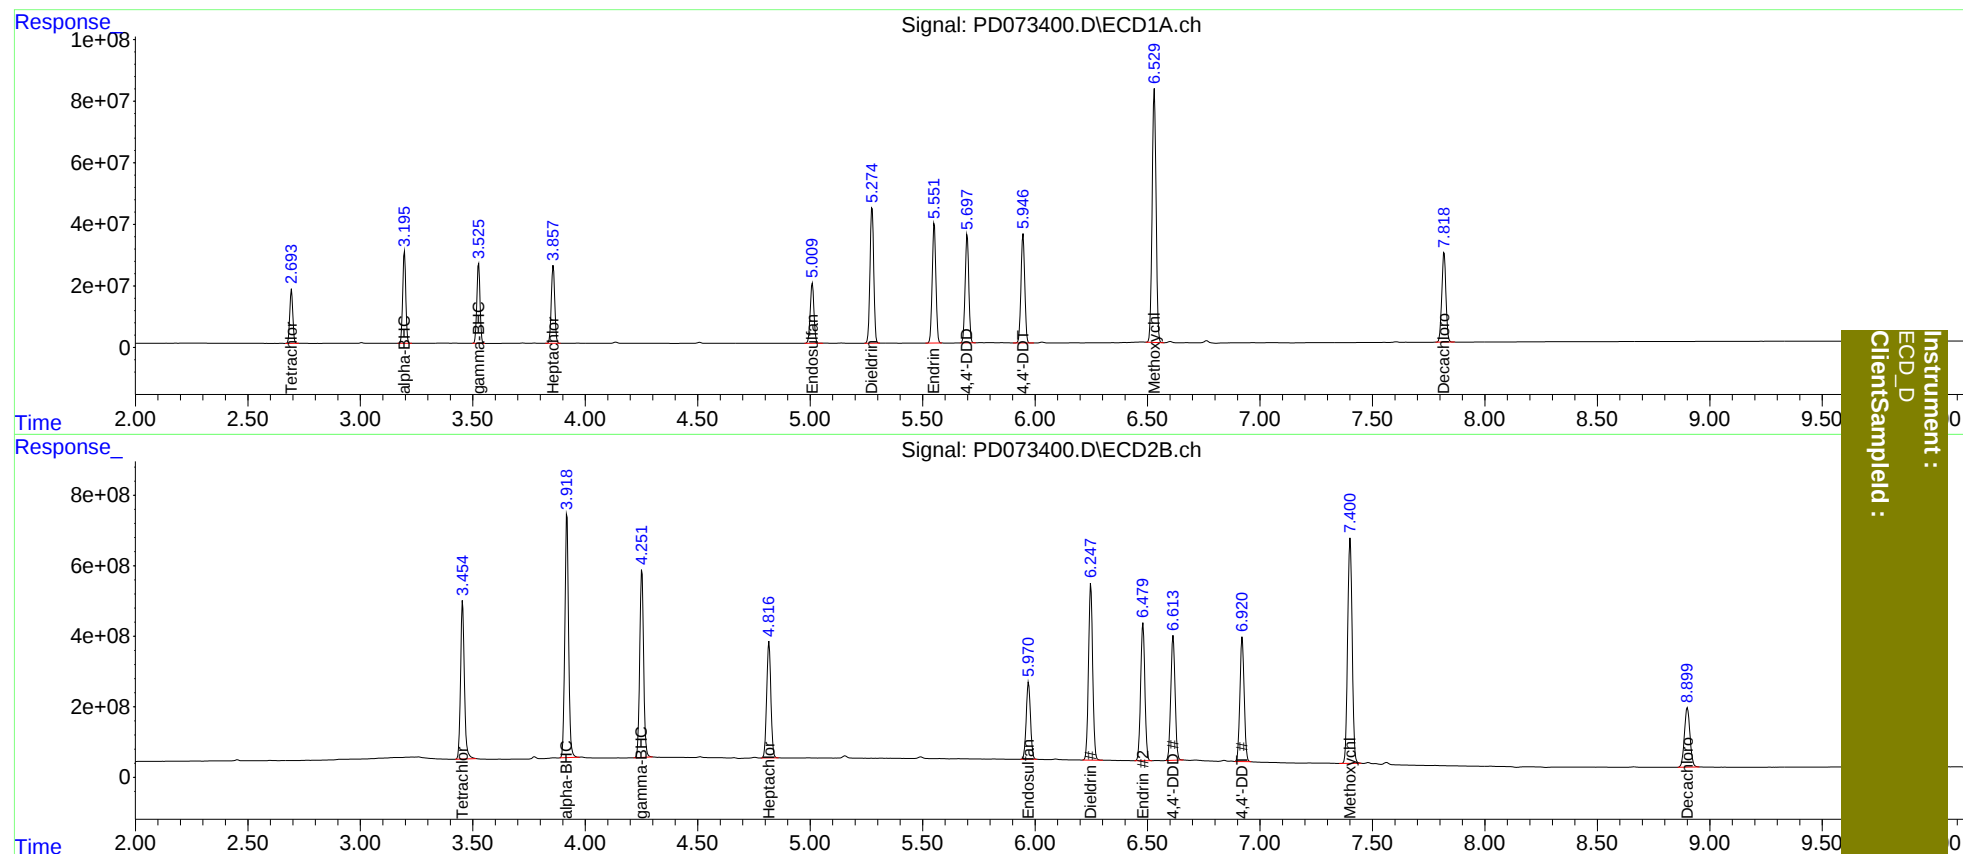


Instrument :
ECD_D
ClientSampled :
0

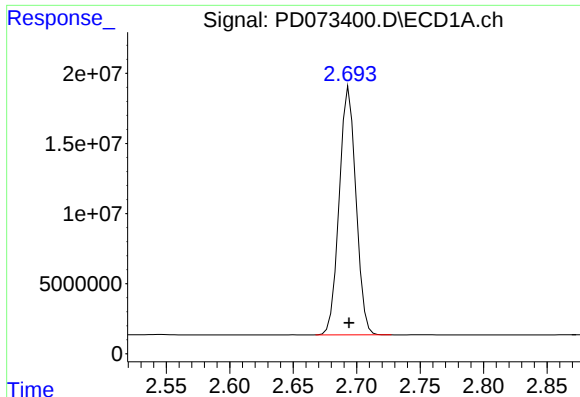

#1 Tetrachloro-m-xylene


R.T.: 2.694 min
Delta R.T.: 0.000 min
Response: 162385577
Conc: 82.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

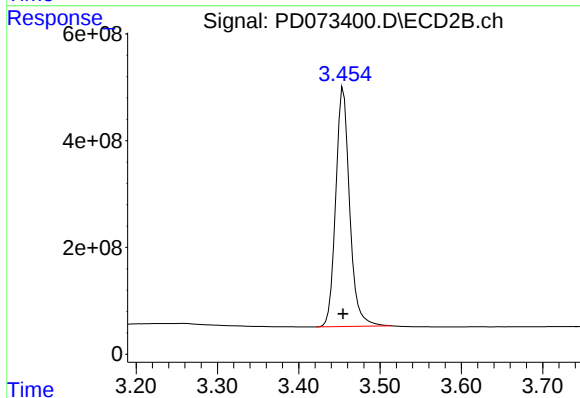


#1 Tetrachloro-m-xylene

R.T.: 3.455 min
Delta R.T.: 0.000 min
Response: 5319543779
Conc: 83.72 ng/ml

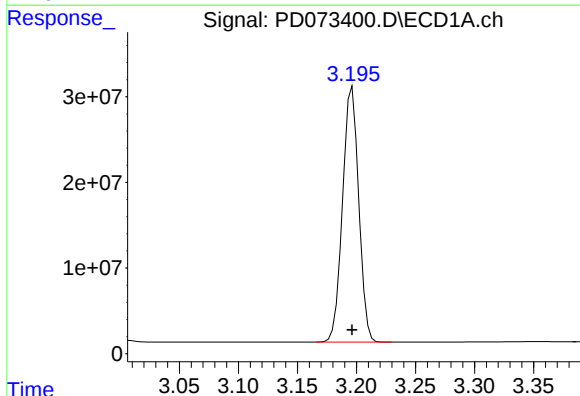


#2 alpha-BHC

R.T.: 3.196 min
Delta R.T.: 0.000 min
Response: 283732325
Conc: 92.37 ng/ml

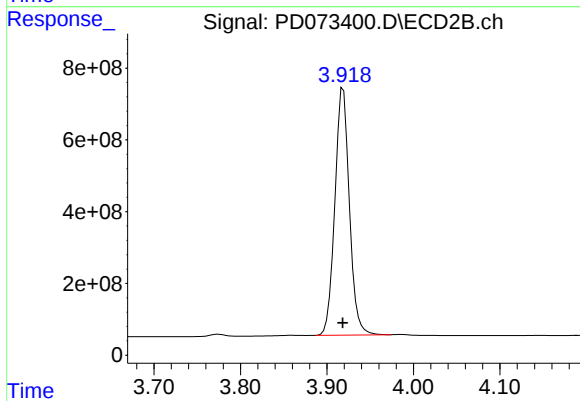

#2 alpha-BHC


R.T.: 3.919 min
Delta R.T.: 0.000 min
Response: 8003207852
Conc: 95.99 ng/ml

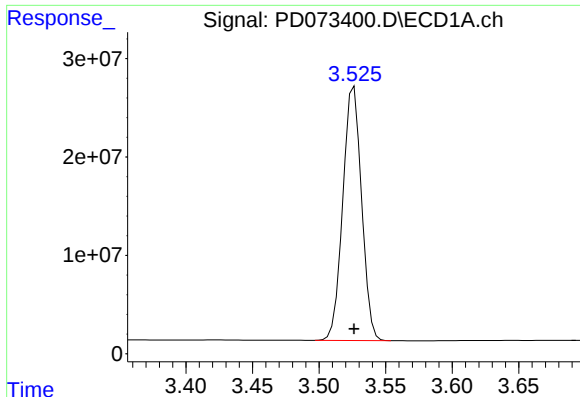

#3 gamma-BHC (Lindane)


R.T.: 3.526 min
Delta R.T.: 0.000 min
Response: 253278282
Conc: 91.04 ng/ml

Instrument :
ECD_D
ClientSampleId :

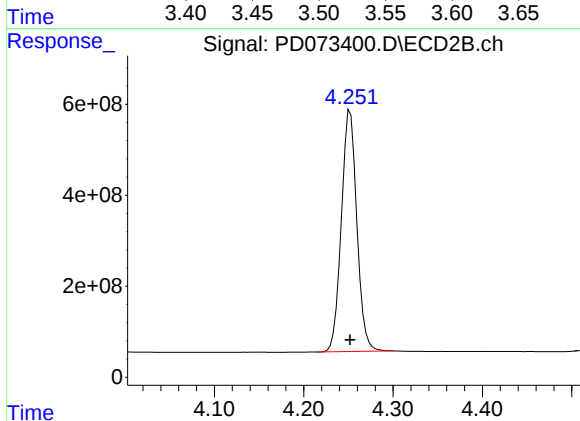


#3 gamma-BHC (Lindane)

R.T.: 4.252 min
Delta R.T.: 0.000 min
Response: 6391543984
Conc: 92.26 ng/ml

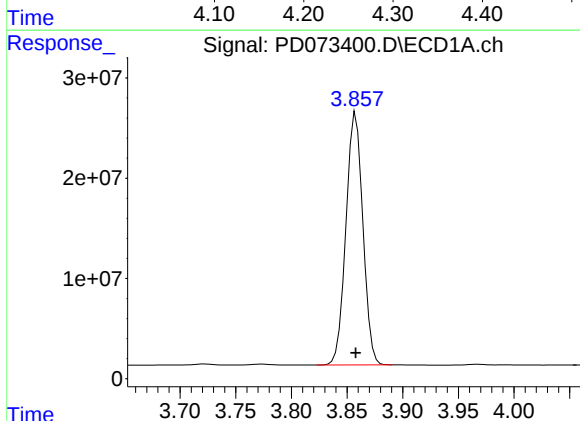


#4 Heptachlor

R.T.: 3.858 min
Delta R.T.: 0.000 min
Response: 266230416
Conc: 89.62 ng/ml

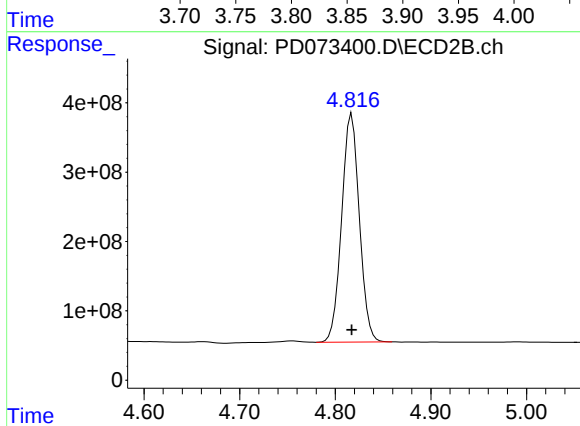

#4 Heptachlor


R.T.: 4.817 min
Delta R.T.: 0.000 min
Response: 4244548656
Conc: 75.98 ng/ml

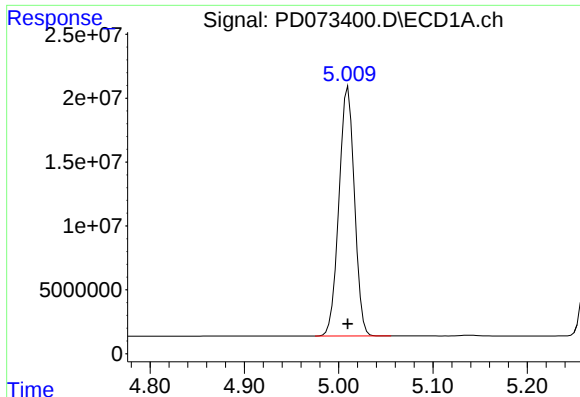

#9 Endosulfan I


R.T.: 5.010 min
Delta R.T.: 0.000 min
Response: 222408195
Conc: 83.87 ng/ml

Instrument :
ECD_D
ClientSampleId :

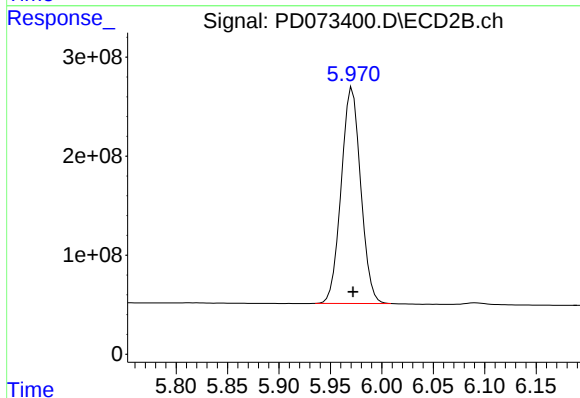


#9 Endosulfan I

R.T.: 5.971 min
Delta R.T.: 0.000 min
Response: 2877352845
Conc: 75.77 ng/ml

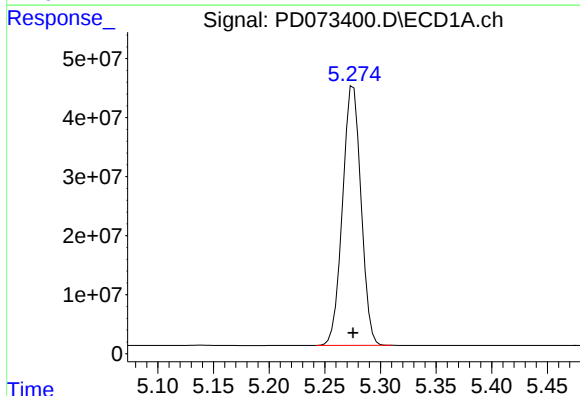


#13 Dieldrin

R.T.: 5.276 min
Delta R.T.: 0.000 min
Response: 508535272
Conc: 173.60 ng/ml

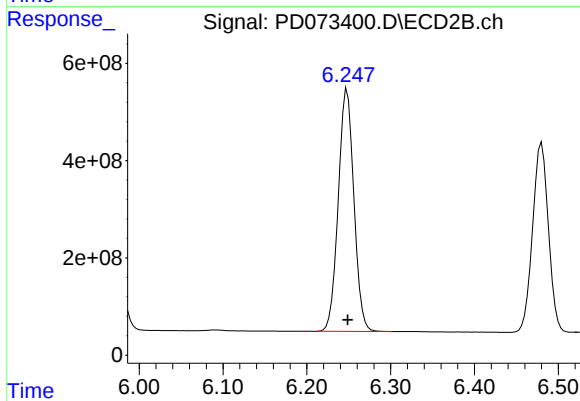

#13 Dieldrin


R.T.: 6.248 min
Delta R.T.: 0.000 min
Response: 6447760120
Conc: 160.55 ng/ml

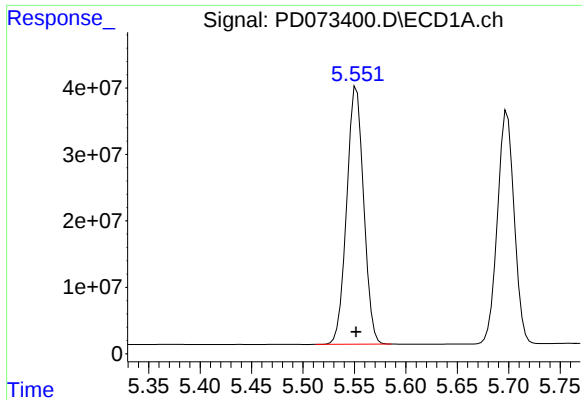

#14 Endrin


R.T.: 5.552 min
Delta R.T.: 0.000 min
Response: 445649292
Conc: 172.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

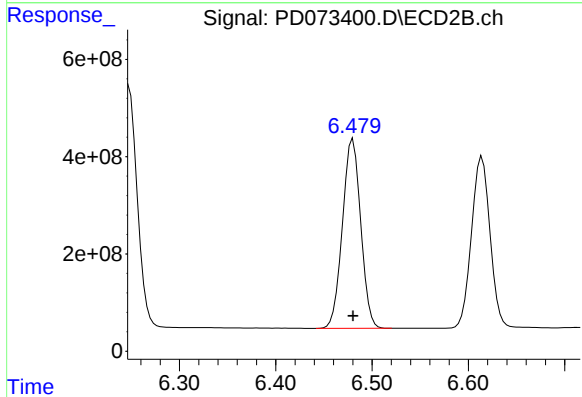


#14 Endrin

R.T.: 6.480 min
Delta R.T.: 0.000 min
Response: 5120683741
Conc: 154.49 ng/ml

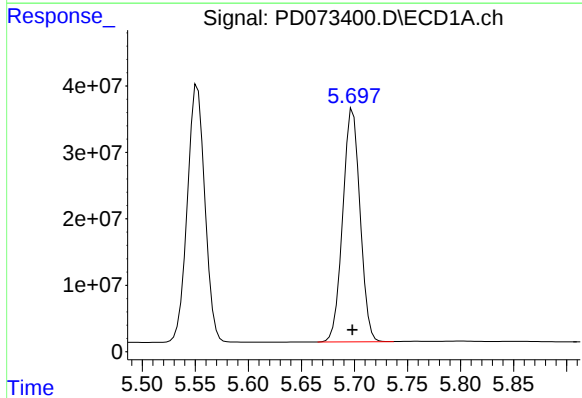


#16 4,4'-DDD

R.T.: 5.699 min
Delta R.T.: 0.000 min
Response: 397395780
Conc: 172.74 ng/ml

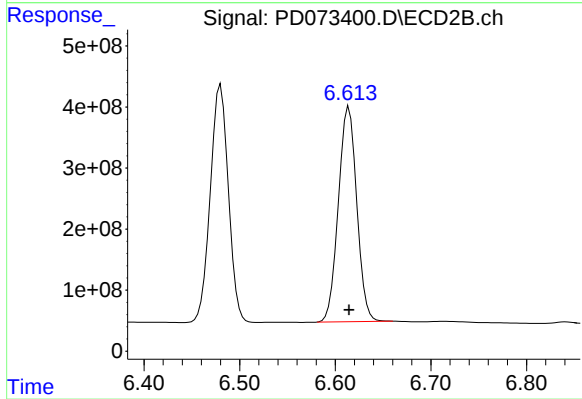

#16 4,4'-DDD


R.T.: 6.614 min
Delta R.T.: 0.000 min
Response: 4718269663
Conc: 157.82 ng/ml

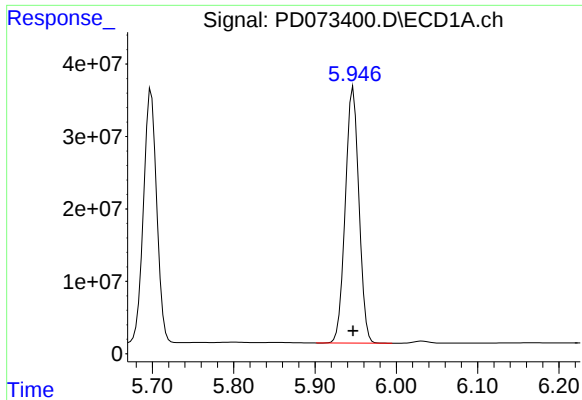

#17 4,4'-DDT


R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 410242226
Conc: 178.32 ng/ml

Instrument :
ECD_D
ClientSampleId :

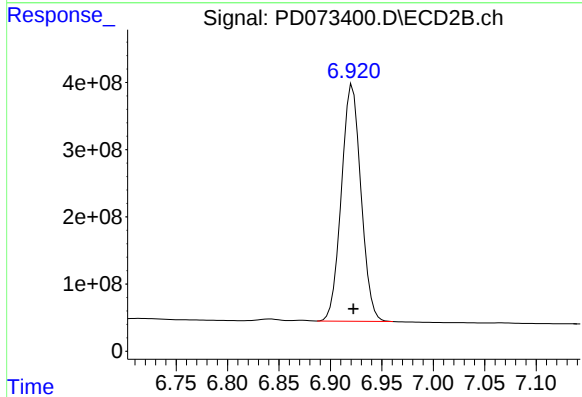


#17 4,4'-DDT

R.T.: 6.921 min
Delta R.T.: -0.001 min
Response: 4671753211
Conc: 162.95 ng/ml

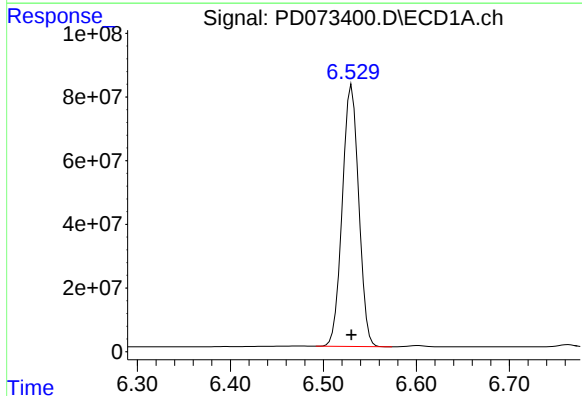


#20 Methoxychlor

R.T.: 6.531 min
Delta R.T.: 0.000 min
Response: 1007616361
Conc: 778.49 ng/ml

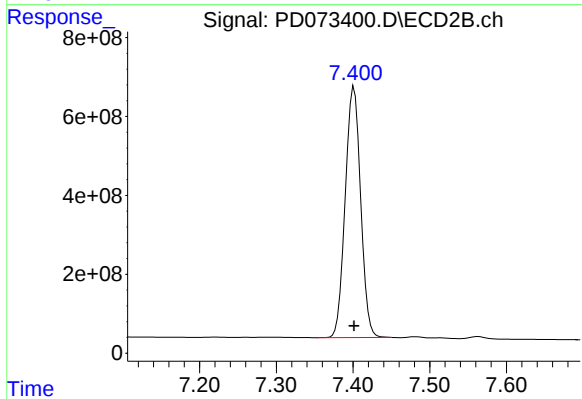

#20 Methoxychlor


R.T.: 7.401 min
Delta R.T.: 0.000 min
Response: 8939460238
Conc: 728.21 ng/ml

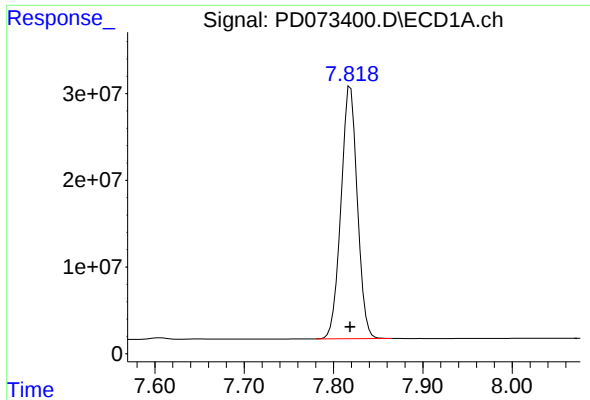

#27 Decachlorobiphenyl

R.T.: 7.819 min
Delta R.T.: 0.000 min
Response: 369800193
Conc: 153.88 ng/ml

Instrument :
ECD_D
ClientSampleId :

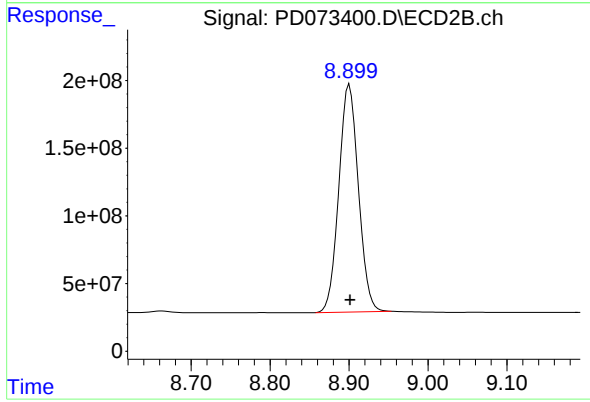

#27 Decachlorobiphenyl

R.T.: 8.900 min
Delta R.T.: 0.000 min
Response: 2900232175
Conc: 153.12 ng/ml