

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122123\
 Data File : PD080230.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2023 17:09
 Operator : AR\AJ
 Sample : INDA344
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3226

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 01:09:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 18 00:44:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.568	2.800	27880210	50105931	21.836	22.534
27)	SA Decachlor...	9.114	7.942	71948380	98678399	44.751	41.112
Target Compounds							
2)	A alpha-BHC	4.024	3.302	45878572	80046600	22.255	23.478
3)	MA gamma-BHC...	4.357	3.631	44512453	75174887	22.416	23.354
4)	MA Heptachlor	4.951	3.973	45268457	73839866	21.677	23.058
9)	A Endosulfan I	6.108	5.126	37122754	61873778	20.839	22.570
13)	MA Dieldrin	6.383	5.390	80432631	139.3E6	43.218	46.493
14)	MA Endrin	6.614	5.666	62754639	117.9E6	40.066	44.802
16)	A 4,4'-DDD	6.745	5.812	58616077	107.9E6	42.259	46.918
17)	MA 4,4'-DDT	7.060	6.064	57199238	104.5E6	38.707	43.333
20)	A Methoxychlor	7.534	6.639	157.8E6	274.9E6	199.350	218.375

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122123\
Data File : PD080230.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2023 17:09
Operator : AR\AJ
Sample : INDA344
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 01:09:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Mon Dec 18 00:44:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

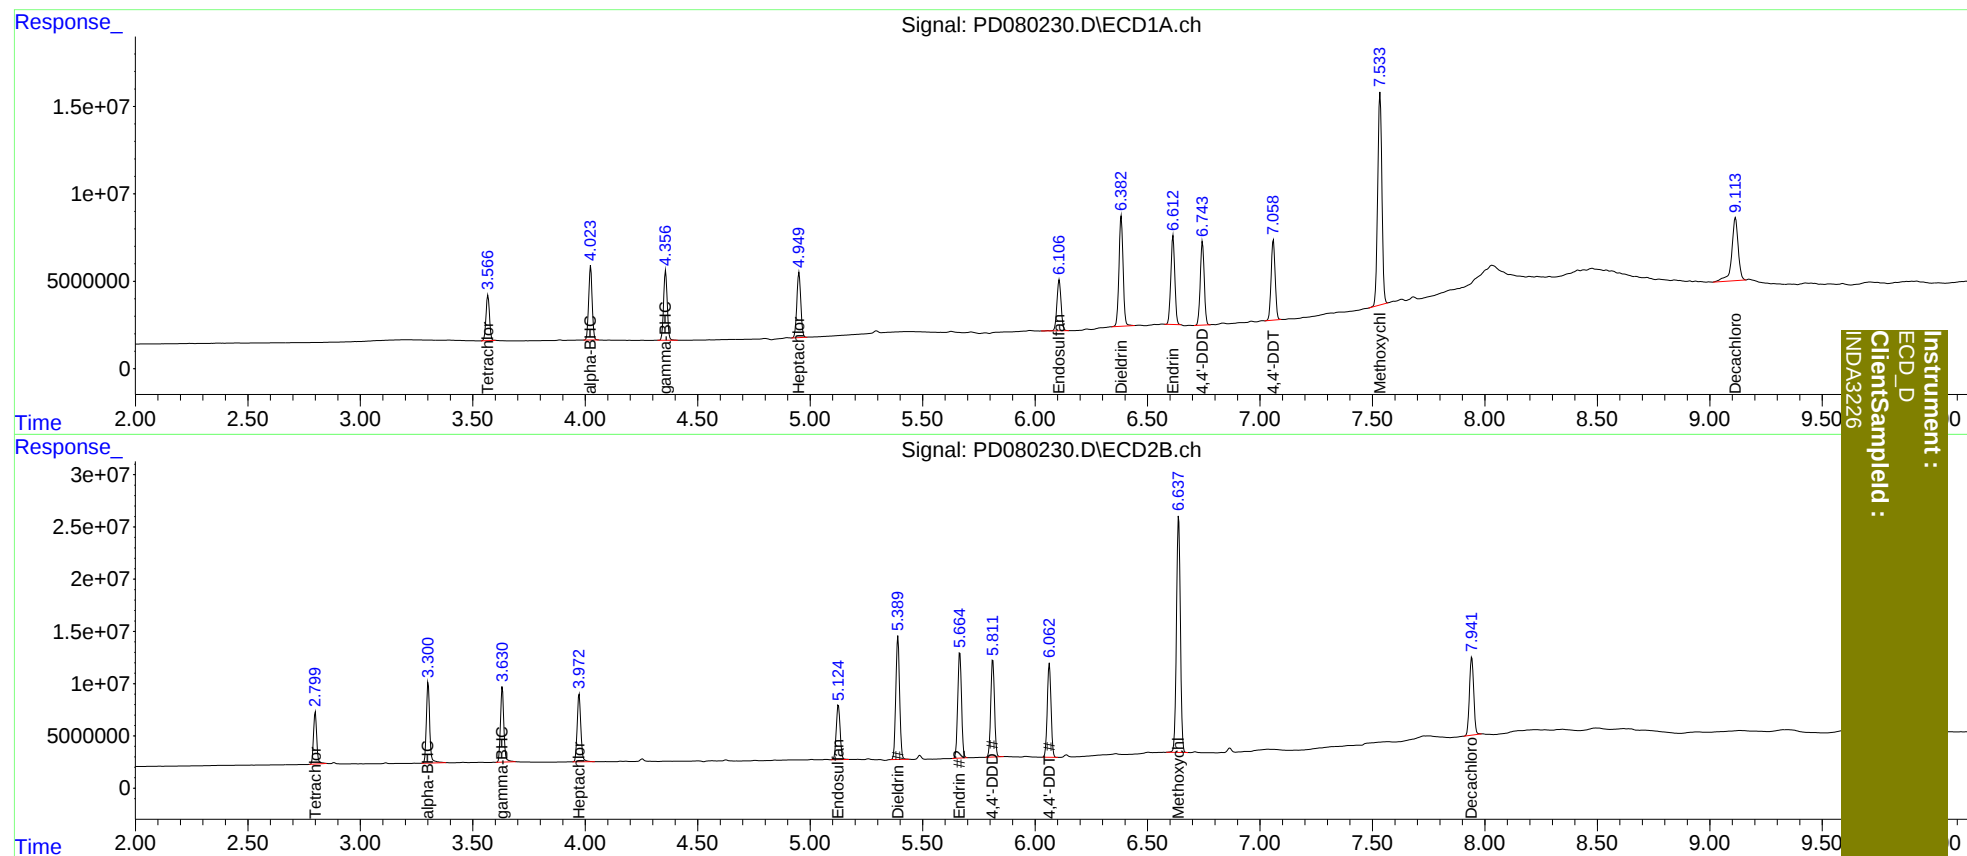

Instrument :
ECD_D
ClientSampled :
INDA3226