

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122123\
 Data File : PD080240.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2023 00:12
 Operator : AR\AJ
 Sample : 05818-03MS
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGRG7MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/20/2023
 Supervised By :Ankita Jodhani 12/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 01:13:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 18 00:44:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.801	13806079	32074010	10.813m	14.425 #
27)	SA Decachlor...	9.097	7.937	285.9E6	103.1E6	177.808	42.934 #
Target Compounds							
2)	A alpha-BHC	4.024	3.303	92954499	153.6E6	45.091m	45.061
3)	MA gamma-BHC...	4.357	3.634	76272774	284.6E6	38.410m	88.423m#
4)	MA Heptachlor	4.950	3.972	77658714	163.2E6	37.188m	50.959m#
5)	MB Aldrin	5.292	4.255	78713586	125.6E6	35.191m	35.546
6)	B beta-BHC	4.551	3.928	18984985	55636450	18.290m	32.403 #
7)	B delta-BHC	4.801	4.157	74708605	142.6E6	32.527m	36.671
8)	B Heptachlo...	5.720	4.756	61194924	102.5E6	28.487	30.246
9)	A Endosulfan I	6.105	5.127	63729597	41844769	35.775m	15.264m#
10)	B trans-Chl...	5.973	5.010	45164117	162.2E6	22.008m	49.272 #
11)	B cis-Chlor...	6.055	5.071	105.3E6	96824180	50.177	28.799 #
12)	B 4,4'-DDE	6.227	5.260	305.7E6	466.3E6	158.258	148.470
13)	MA Dieldrin	6.399	5.395	365.2E6	548.8E6	196.230	183.113m
14)	MA Endrin	6.617	5.665	211.7E6	294.0E6	135.167m	111.754
15)	B Endosulfa...	6.828	5.959	145.4E6	298.5E6	77.562	102.951m#
16)	A 4,4'-DDD	6.735	5.812	342.5E6	259.0E6	246.940	112.665 #
17)	MA 4,4'-DDT	7.060	6.064	289.1E6	330.7E6	195.663	137.167 #
18)	B Endrin al...	6.961	6.140	198.0E6	99430194	132.725	43.119 #
19)	B Endosulfa...	7.196	6.361	188.8E6	180.9E6	102.944	64.486 #
20)	A Methoxychlor	7.532	6.638	320.7E6	373.0E6	405.026m	296.335m#
21)	B Endrin ke...	7.683	6.866	105.3E6	128.1E6	54.124m	40.023 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122123\
Data File : PD080240.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2023 00:12
Operator : AR\AJ
Sample : 05818-03MS
Misc :
ALS Vial : 35 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 01:13:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Mon Dec 18 00:44:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

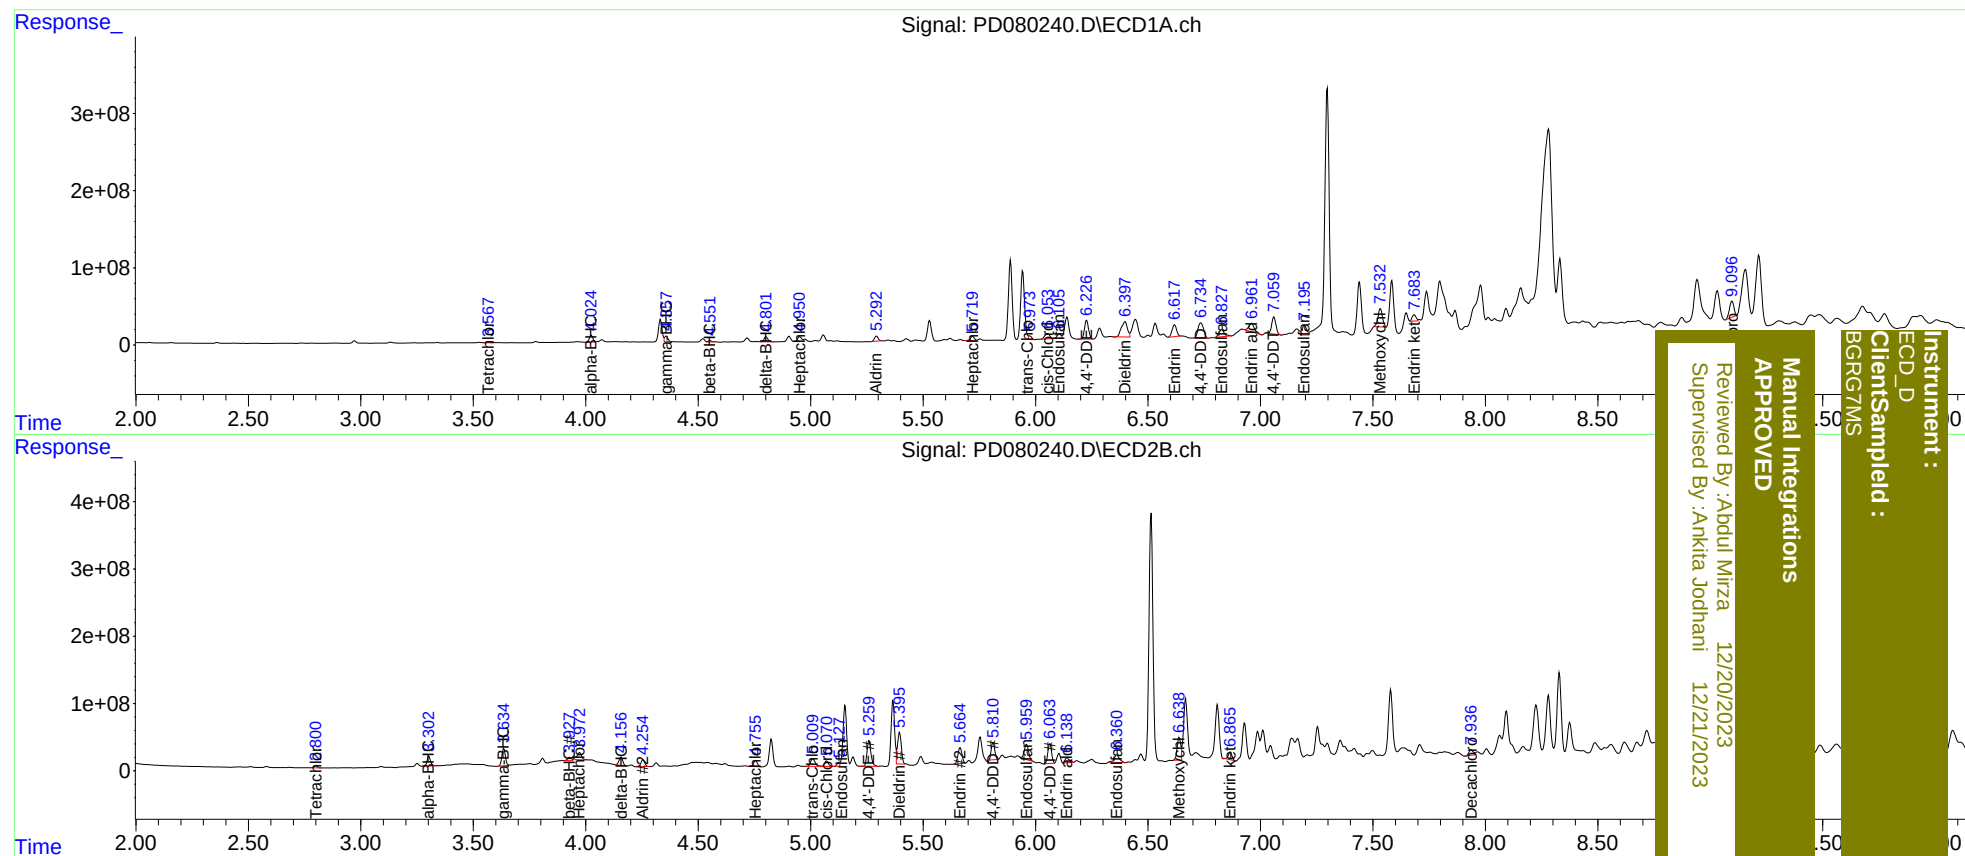

Instrument :
ECD_D
Client Sampled :
BGRGZMS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 12/20/2023
Supervised By: Ankita Jodhani 12/21/2023