

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122123\
 Data File : PD080215.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2023 13:45
 Operator : AR\AJ
 Sample : 05794-11DL 2X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH3Q6DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/20/2023
 Supervised By : Ankita Jodhani 12/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 01:05:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 18 00:44:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.567	2.800	6881973	12735608	5.390	5.728
27) SA Decachlor...	9.100	7.941	8349635	15574433	5.193	6.489
Target Compounds						
12) B 4,4'-DDE	6.226	5.259	192.0E6	377.1E6	99.372	120.072
14) MA Endrin	6.646	5.675	31898273	54693389	20.365m	20.787m
16) A 4,4'-DDD	6.744	5.812	18906351	22069196	13.630	9.598 #
17) MA 4,4'-DDT	7.059	6.064	151.0E6	257.9E6	102.152	106.972

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122123\
Data File : PD080215.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2023 13:45
Operator : AR\AJ
Sample : 05794-11DL 2X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 01:05:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Mon Dec 18 00:44:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

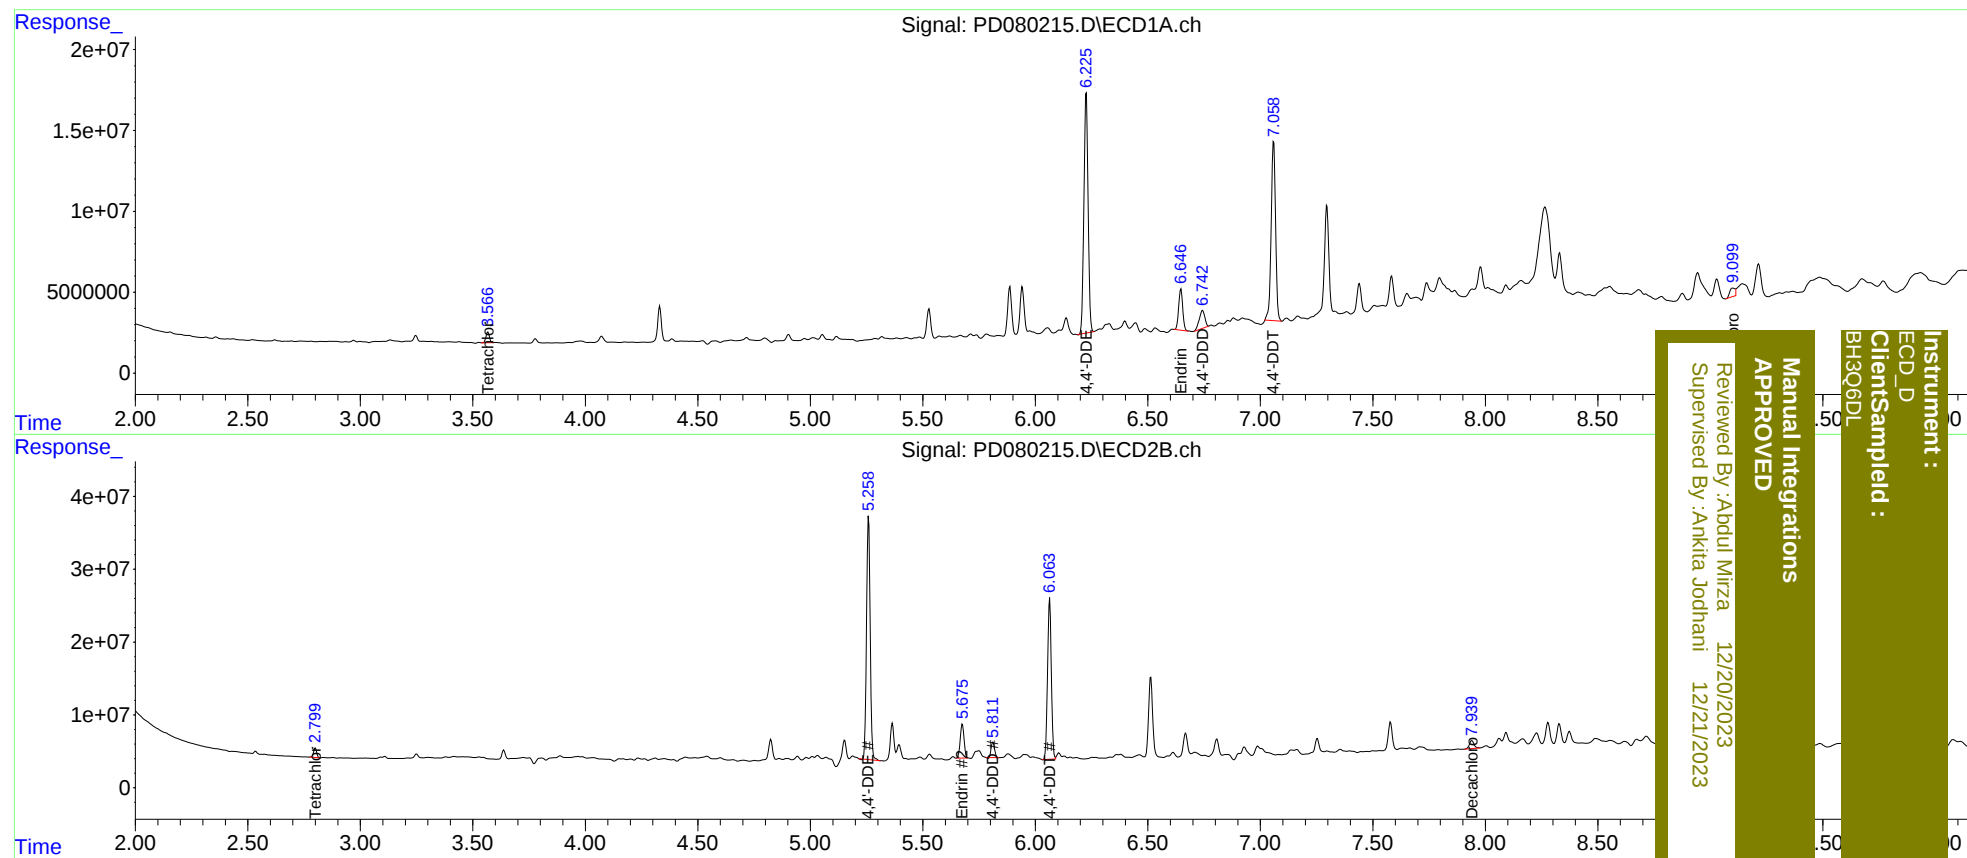

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 12/20/2023
Supervised By: Ankita Jodhani 12/21/2023

Instrument :
ECD_D
Client Sampled :
BH306DL