

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122123\
 Data File : PD080217.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2023 14:12
 Operator : AR\AJ
 Sample : 05794-12DL2 50X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH3Q7DL2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/20/2023
 Supervised By : Ankita Jodhani 12/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 01:06:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 18 00:44:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
10) B	trans-Chl...	5.944	5.011	4298563	4122517	2.095m 1.252m#
11) B	cis-Chlor...	6.052	5.098	1260997	2185962	0.601 0.650m
12) B	4,4'-DDE	6.228	5.260	117.5E6	192.5E6	60.829 61.281
16) A	4,4'-DDD	6.745	5.813	19479928	37967126	14.044 16.513
17) MA	4,4'-DDT	7.060	6.064	336.2E6	573.2E6	227.517 237.744

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122123\
Data File : PD080217.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2023 14:12
Operator : AR\AJ
Sample : 05794-12DL2 50X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 01:06:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Mon Dec 18 00:44:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

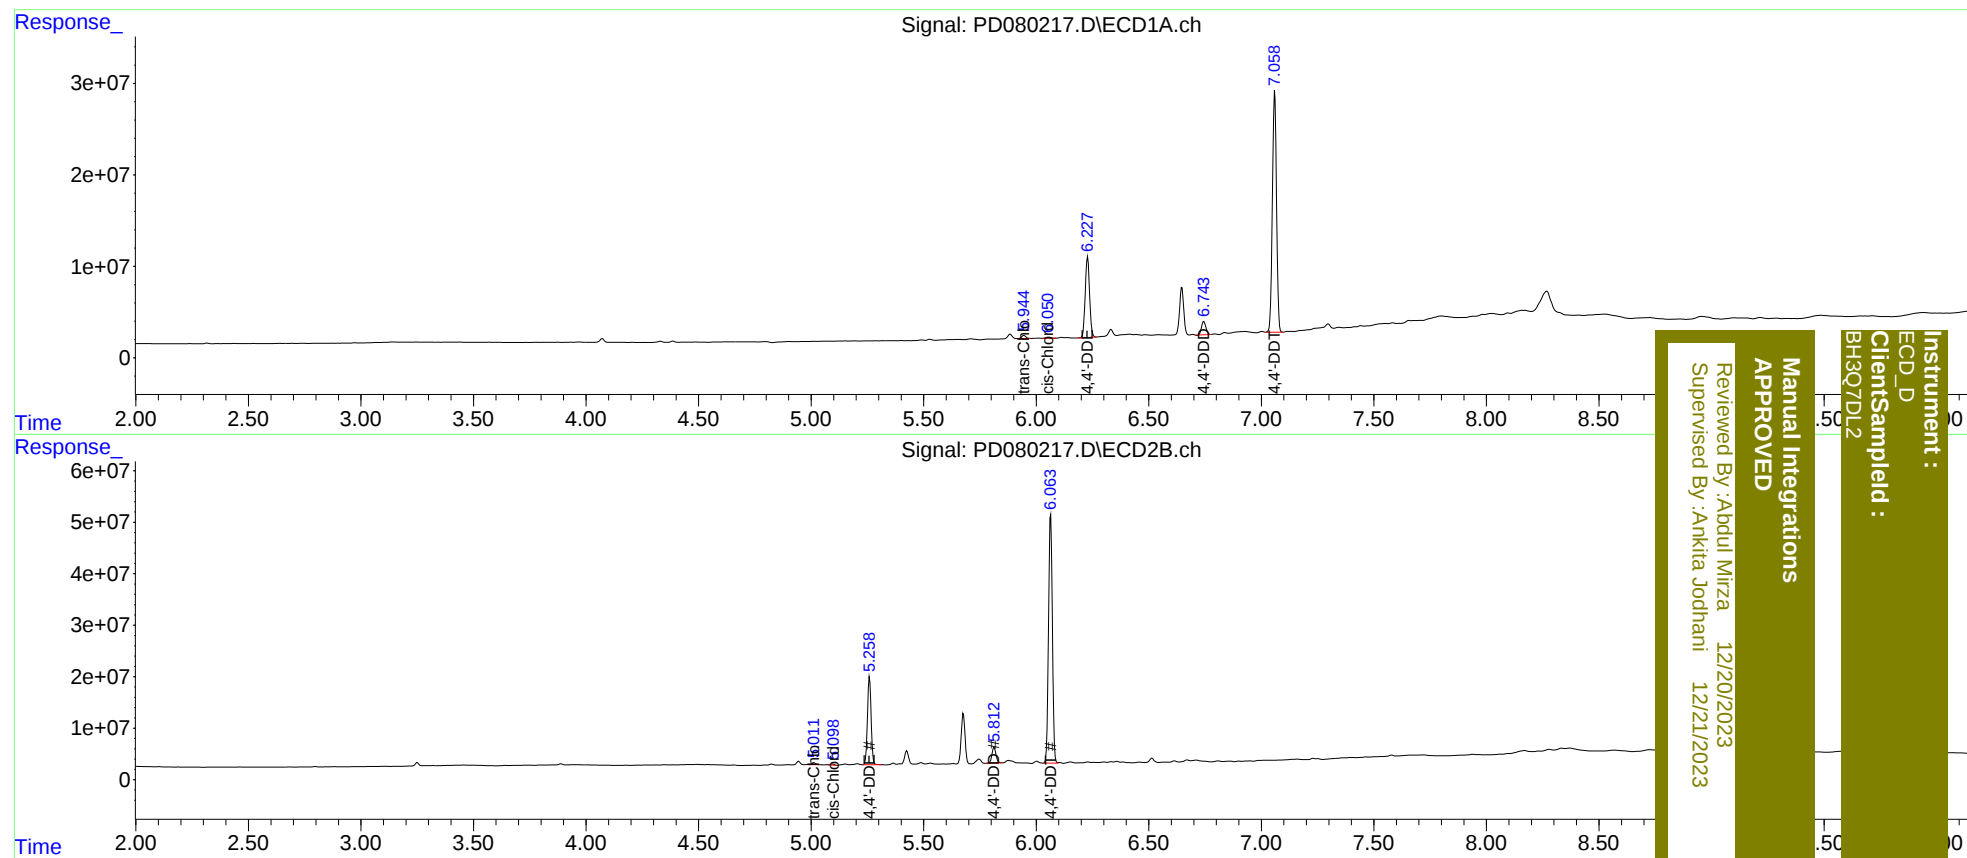

Instrument :
ECD_D
ClientSampled :
BH307DL2

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/20/2023
Supervised By :Ankita Jodhani 12/21/2023