Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122124\
Data File : PD087241.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2024 13:17
Operator : AR\AJ
Sample : P5235-10 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

**Instrument :**
ECD_D
**ClientSampleId :**
C0AW0

**Manual Integrations APPROVED**

Reviewed By :Yogesh Patel 12/25/2024
Supervised By :mohammad ahmed 12/25/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 23:40:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121924CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 05:53:12 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x0.25µm

| | Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|---|---|---|---|---|---|---|---|
| | System Monitoring Compounds | | | | | | |
| 1) | SA Tetrachlo... | 3.556 | 2.882 | 40103667 | 244.9E6 | 19.764 | 22.280m |
| 27) | SA Decachlor... | 9.085 | 8.086 | 59546689 | 262.3E6 | 20.102 | 21.228 |
| | Target Compounds | | | | | | |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122124\
Data File : PD087241.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2024 13:17
Operator : AR\AJ
Sample : P5235-10 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 23:40:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121924CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 05:53:12 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x0.25µm

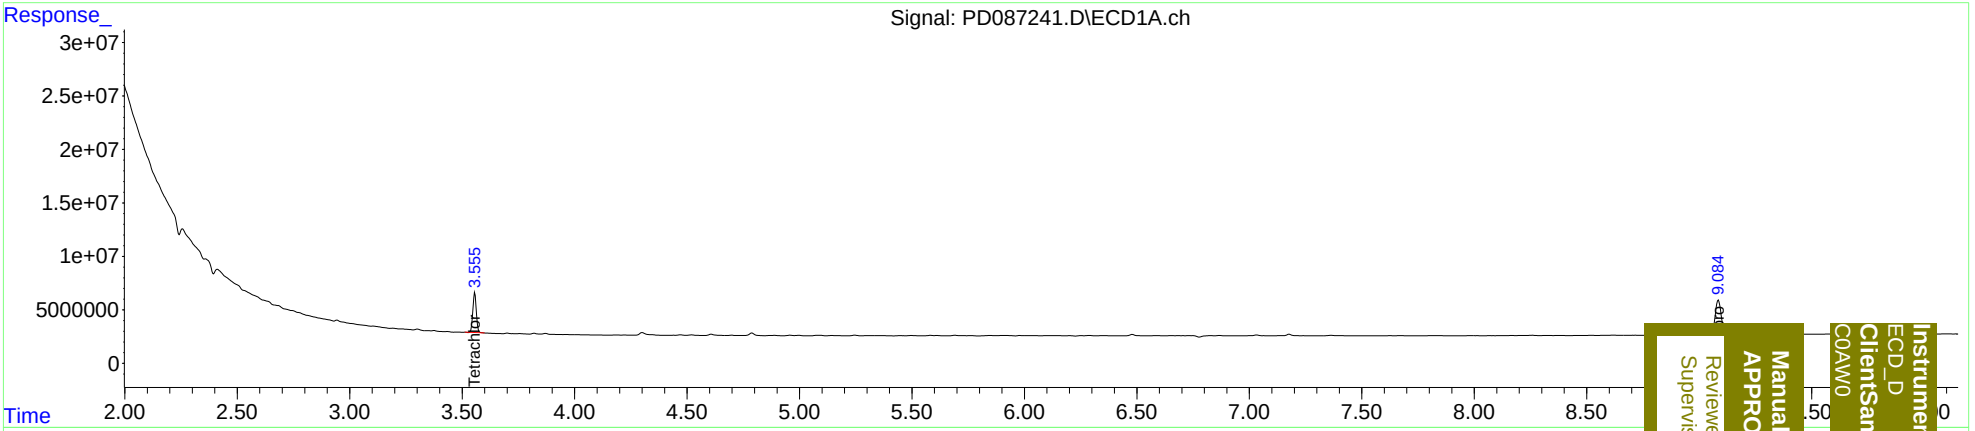


Manual Integrations APPROVED
Reviewed By :Yogesh Patel 12/25/2024
Supervised By :mohammad ahmed 12/25/2024

Instrument :
ECD_D
ClientSampleId :
C0AW0