

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122124\
 Data File : PD087249.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2024 15:10
 Operator : AR\AJ
 Sample : P5235-22MS 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AT9MS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/25/2024
 Supervised By :mohammad ahmed 12/25/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 23:42:51 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121924CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 20 05:53:12 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.882	40258055	239.9E6	19.840m	21.821m
27)	SA Decachlor...	9.085	8.086	59151643	262.4E6	19.969	21.237
Target Compounds							
2)	A alpha-BHC	4.006	3.397	225.5E6	932.2E6	54.740	53.587
3)	MA gamma-BHC...	4.338	3.734	224.3E6	873.2E6	56.427	54.120
4)	MA Heptachlor	4.938	4.089	215.9E6	856.7E6	54.135	52.292
5)	MB Aldrin	5.280	4.376	210.0E6	836.4E6	53.761	52.284
6)	B beta-BHC	4.521	4.028	82744964	373.3E6	48.214	50.068m
7)	B delta-BHC	4.770	4.267	143.8E6	597.5E6	35.541	35.858
8)	B Heptachlo...	5.699	4.880	193.4E6	777.0E6	54.229	52.199
9)	A Endosulfan I	6.082	5.255	179.0E6	730.1E6	54.047m	53.248
10)	B trans-Chl...	5.955	5.134	190.5E6	810.1E6	54.198	52.045
11)	B cis-Chlor...	6.035	5.198	194.5E6	794.4E6	54.973m	52.813
12)	B 4,4'-DDE	6.205	5.384	370.3E6	1507.0E6	110.003	105.457
13)	MA Dieldrin	6.356	5.522	404.9E6	1548.8E6	111.715	106.486
14)	MA Endrin	6.583	5.798	341.7E6	1404.2E6	113.161	105.195
15)	B Endosulfa...	6.794	6.089	329.1E6	1331.4E6	109.805	103.858
16)	A 4,4'-DDD	6.714	5.939	288.8E6	1241.2E6	111.084	107.480
17)	MA 4,4'-DDT	7.028	6.194	306.7E6	1301.5E6	113.070m	107.865
18)	B Endrin al...	6.923	6.268	237.3E6	980.4E6	101.412	98.400
19)	B Endosulfa...	7.157	6.491	295.8E6	1246.5E6	102.379	99.353
20)	A Methoxychlor	7.502	6.765	781.0E6	2706.7E6	531.979	500.062
21)	B Endrin ke...	7.639	7.001	336.3E6	1418.3E6	105.527	103.478

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122124\
Data File : PD087249.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2024 15:10
Operator : AR\AJ
Sample : P5235-22MS 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 23:42:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121924CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 05:53:12 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x0.25µm

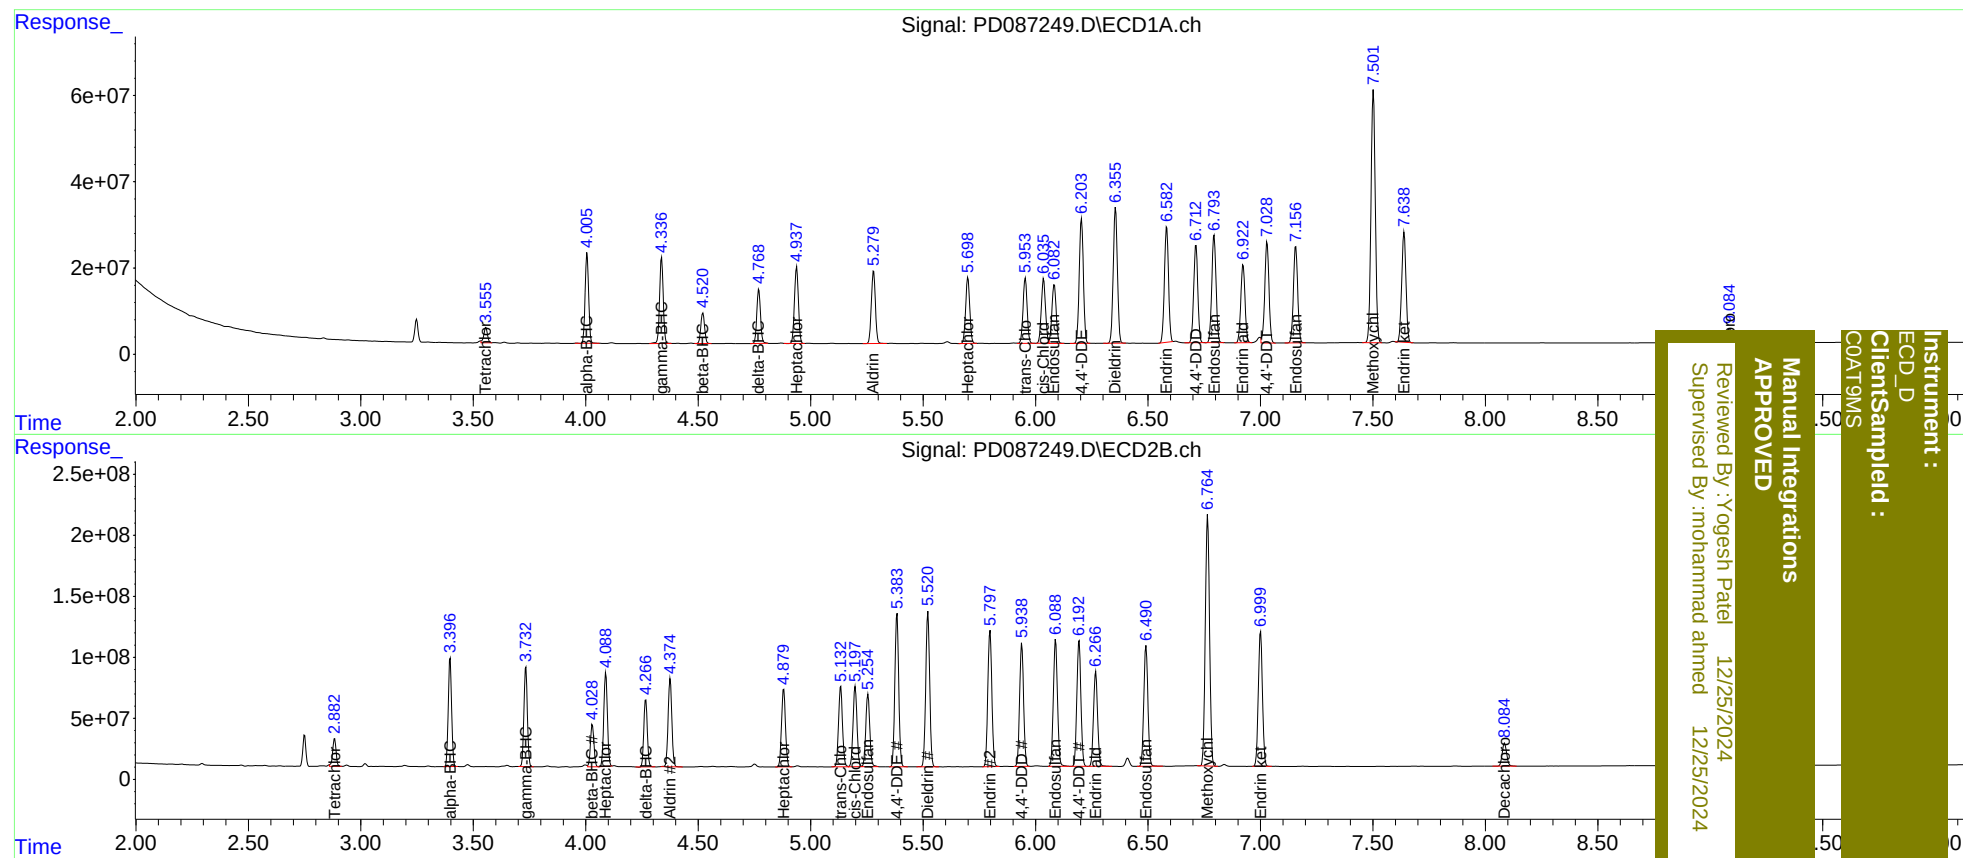

Instrument :
ECD_D
ClientSampled :
COAT9MS

Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 12/25/2024
Supervised By : mohammad ahmed 12/25/2024