

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122124\
 Data File : PD087250.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2024 15:24
 Operator : AR\AJ
 Sample : P5235-23MSD 10X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AT9MSD

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/25/2024
 Supervised By :mohammad ahmed 12/25/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 23:43:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121924CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 20 05:53:12 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.882	40814535	243.3E6	20.114m	22.133m
27)	SA Decachlor...	9.085	8.085	59216798	263.5E6	19.991	21.326
Target Compounds							
2)	A alpha-BHC	4.006	3.397	226.5E6	939.4E6	54.977	53.998
3)	MA gamma-BHC...	4.337	3.734	225.1E6	881.1E6	56.628	54.604
4)	MA Heptachlor	4.937	4.089	217.2E6	863.2E6	54.471	52.689
5)	MB Aldrin	5.279	4.375	211.0E6	846.0E6	54.011	52.883
6)	B beta-BHC	4.521	4.028	83220942	374.2E6	48.491	50.183m
7)	B delta-BHC	4.769	4.267	143.8E6	603.0E6	35.532	36.192
8)	B Heptachlo...	5.699	4.880	194.5E6	782.4E6	54.543	52.565
9)	A Endosulfan I	6.081	5.255	180.4E6	735.1E6	54.489m	53.614
10)	B trans-Chl...	5.954	5.133	191.3E6	816.3E6	54.427	52.445
11)	B cis-Chlor...	6.033	5.198	196.3E6	801.4E6	55.495m	53.280
12)	B 4,4'-DDE	6.203	5.384	372.8E6	1518.2E6	110.743	106.240
13)	MA Dieldrin	6.355	5.521	407.1E6	1558.6E6	112.319	107.161
14)	MA Endrin	6.582	5.797	343.7E6	1413.0E6	113.848	105.853
15)	B Endosulfa...	6.793	6.089	331.4E6	1336.4E6	110.595	104.248
16)	A 4,4'-DDD	6.712	5.938	290.1E6	1247.2E6	111.604	108.000
17)	MA 4,4'-DDT	7.027	6.192	306.7E6	1309.9E6	113.084m	108.562
18)	B Endrin al...	6.922	6.266	237.6E6	987.3E6	101.522	99.097
19)	B Endosulfa...	7.157	6.491	297.3E6	1254.0E6	102.876	99.951
20)	A Methoxychlor	7.501	6.765	782.5E6	2715.4E6	533.015	501.675
21)	B Endrin ke...	7.638	7.000	337.7E6	1429.4E6	105.963	104.287

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122124\
Data File : PD087250.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2024 15:24
Operator : AR\AJ
Sample : P5235-23MSD 10X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 23:43:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121924CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 05:53:12 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x0.25µm

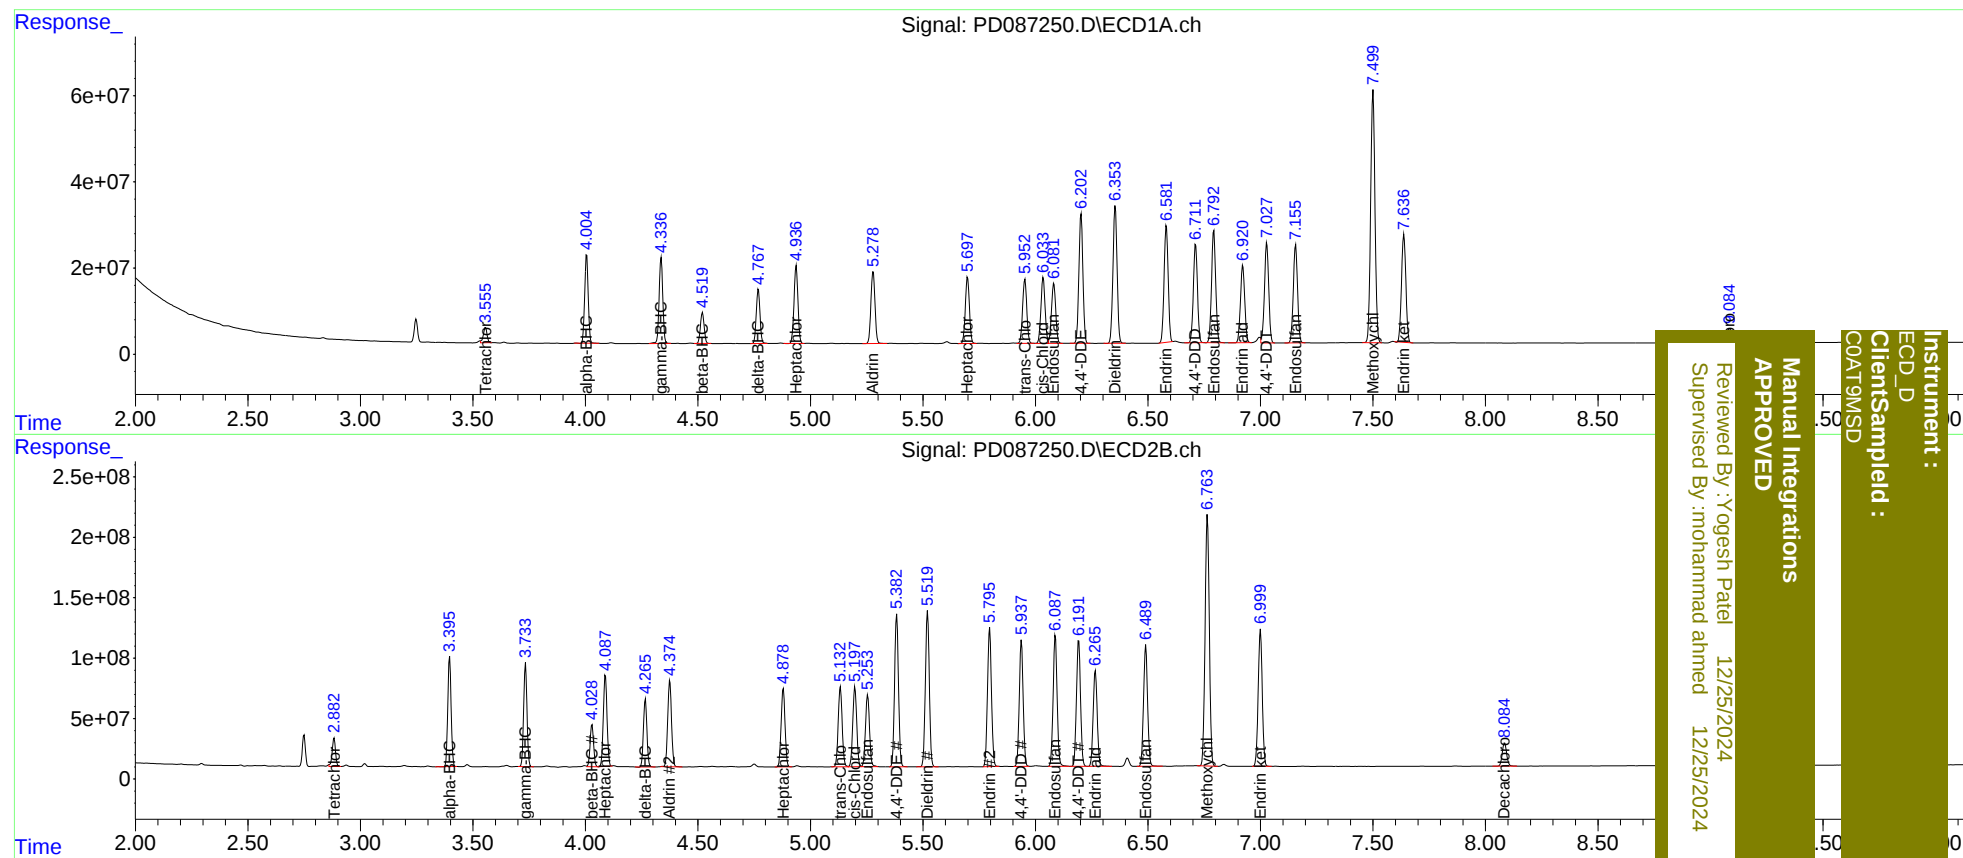

Instrument :
ECD_D
ClientSampled :
COAT9MSD

Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 12/25/2024
Supervised By : mohammad ahmed 12/25/2024