

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122222\
 Data File : PD073419.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2022 19:52
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 03:07:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122222CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 22 03:07:00 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.694	3.455	81498269	2533.3E6	38.917	34.744
27)	SA Decachlor...	7.818	8.900	195.6E6	1517.5E6	80.133	80.472
Target Compounds							
2)	A alpha-BHC	3.196	3.918	135.5E6	3839.4E6	38.193	32.510
3)	MA gamma-BHC...	3.526	4.252	126.4E6	3035.9E6	38.429	35.911
4)	MA Heptachlor	3.858	4.817	131.0E6	2138.7E6	39.080	39.171
9)	A Endosulfan I	5.010	5.972	108.9E6	1481.6E6	39.369	39.590
13)	MA Dieldrin	5.275	6.248	246.4E6	3222.3E6	79.015	82.941
14)	MA Endrin	5.552	6.480	214.5E6	2428.8E6	80.175	76.521
16)	A 4,4'-DDD	5.698	6.614	192.4E6	2411.9E6	78.390	78.863
17)	MA 4,4'-DDT	5.947	6.922	198.4E6	2347.4E6	78.703	79.397
20)	A Methoxychlor	6.530	7.401	536.2E6	4852.6E6	410.081	419.728

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122222\
Data File : PD073419.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2022 19:52
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 03:07:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122222CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 22 03:07:00 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

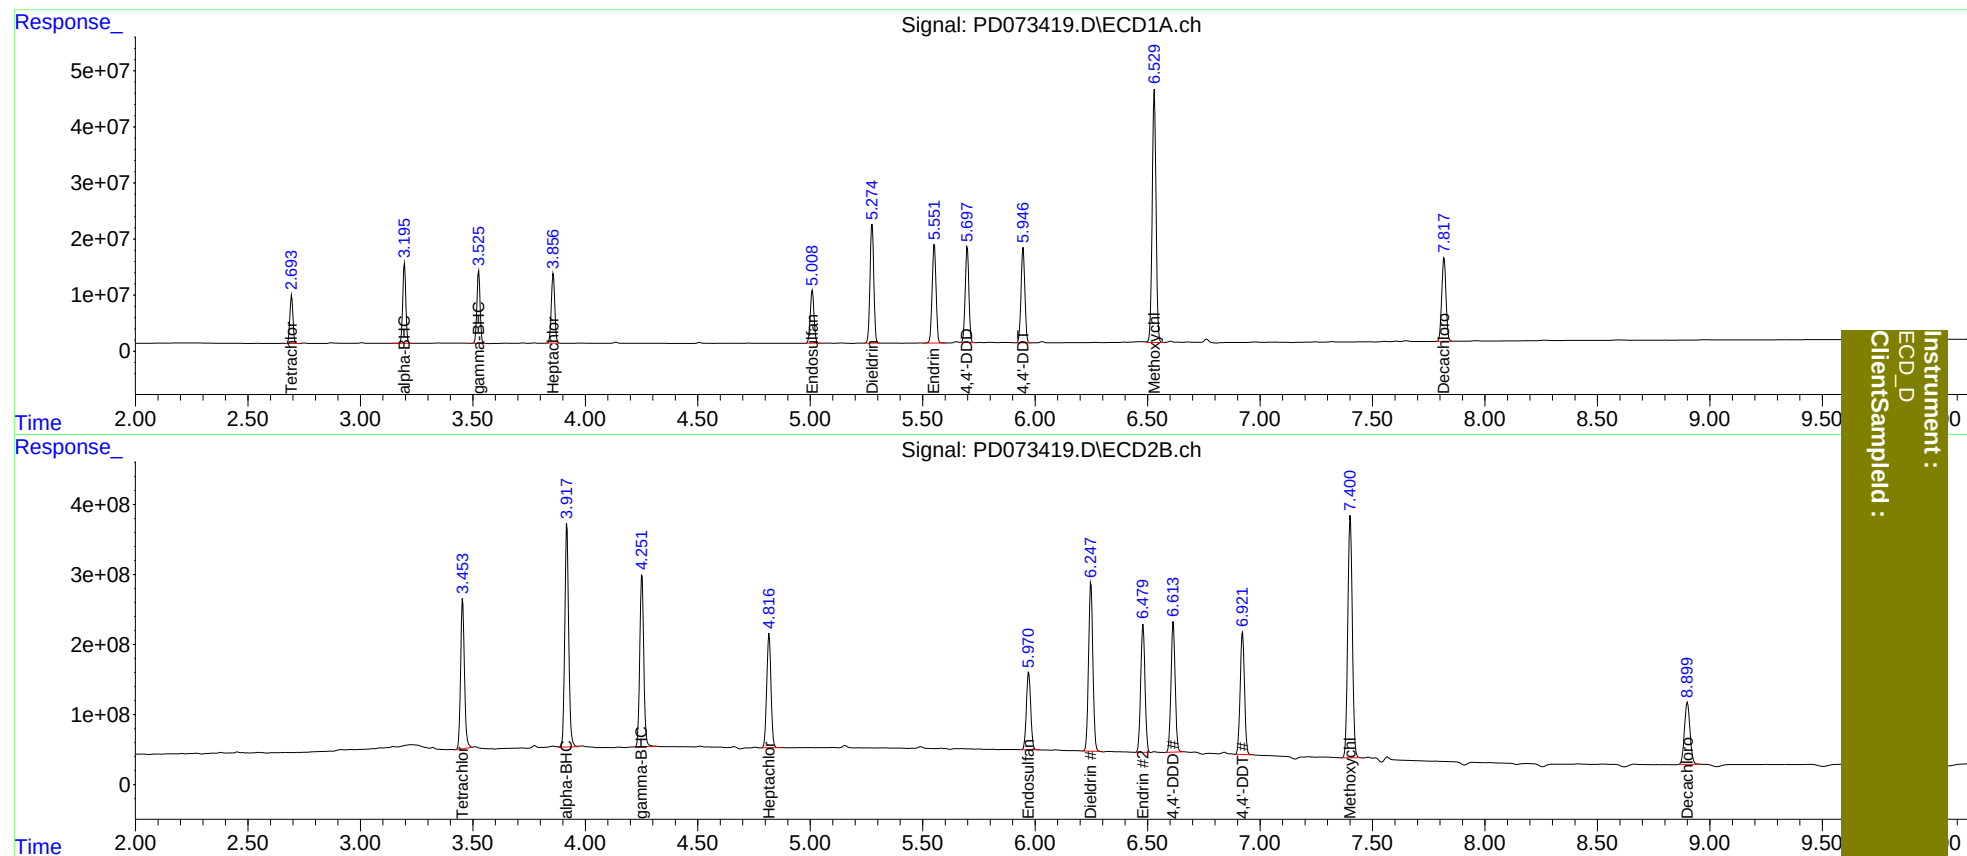

Instrument :
ECD_D
ClientSampled :
0