

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122222\
 Data File : PD073431.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2022 05:07
 Operator : AR\AJ
 Sample : N6130-03MSD 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EXGJ0MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/23/2022
 Supervised By :Ankita Jodhani 12/23/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 23 09:55:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122222CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 22 04:14:38 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.696	3.456	43331065	1615.6E6	20.358	21.595
27)	SA Decachlor...	7.820	8.901	62375356	497.3E6	24.466	25.326
Target Compounds							
2)	A alpha-BHC	3.198	3.919	177.9E6	5316.4E6	52.333	45.080
3)	MA gamma-BHC...	3.528	4.253	158.7E6	3930.9E6	49.896	44.225
4)	MA Heptachlor	3.858	4.818	161.9E6	2734.5E6	49.010m	46.427
5)	MB Aldrin	4.138	5.156	167.4E6	2547.5E6	51.681	50.023
6)	B beta-BHC	3.828	4.468	66794297	1364.0E6	45.179m	43.642
7)	B delta-BHC	4.059	4.712	155.8E6	2920.5E6	45.079	41.569
8)	B Heptachlo...	4.643	5.588	150.4E6	2208.0E6	50.635	49.340
9)	A Endosulfan I	5.011	5.972	140.0E6	2040.1E6	50.228	51.390
10)	B trans-Chl...	4.891	5.842	154.2E6	2174.4E6	52.151	51.307
11)	B cis-Chlor...	4.954	5.917	152.6E6	2160.0E6	50.840	50.639
12)	B 4,4'-DDE	5.143	6.091	308.5E6	4264.5E6	105.159	102.796
13)	MA Dieldrin	5.277	6.249	328.5E6	4489.5E6	107.368	109.191
14)	MA Endrin	5.554	6.481	286.7E6	3549.1E6	108.289	105.502
15)	B Endosulfa...	5.852	6.711	274.6E6	3367.1E6	103.428	102.498
16)	A 4,4'-DDD	5.700	6.615	252.6E6	3211.8E6	105.439	101.310
17)	MA 4,4'-DDT	5.949	6.923	269.5E6	3368.8E6	111.183	111.635
18)	B Endrin al...	6.033	6.842	186.3E6	2276.3E6	87.655	88.534
19)	B Endosulfa...	6.256	7.074	248.3E6	2810.9E6	99.363	101.497
20)	A Methoxychlor	6.531	7.402	694.1E6	6416.7E6	520.083	520.207
21)	B Endrin ke...	6.766	7.564	310.4E6	3024.1E6	103.854	101.956

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122222\
Data File : PD073431.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2022 05:07
Operator : AR\AJ
Sample : N6130-03MSD 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 23 09:55:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122222CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 22 04:14:38 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

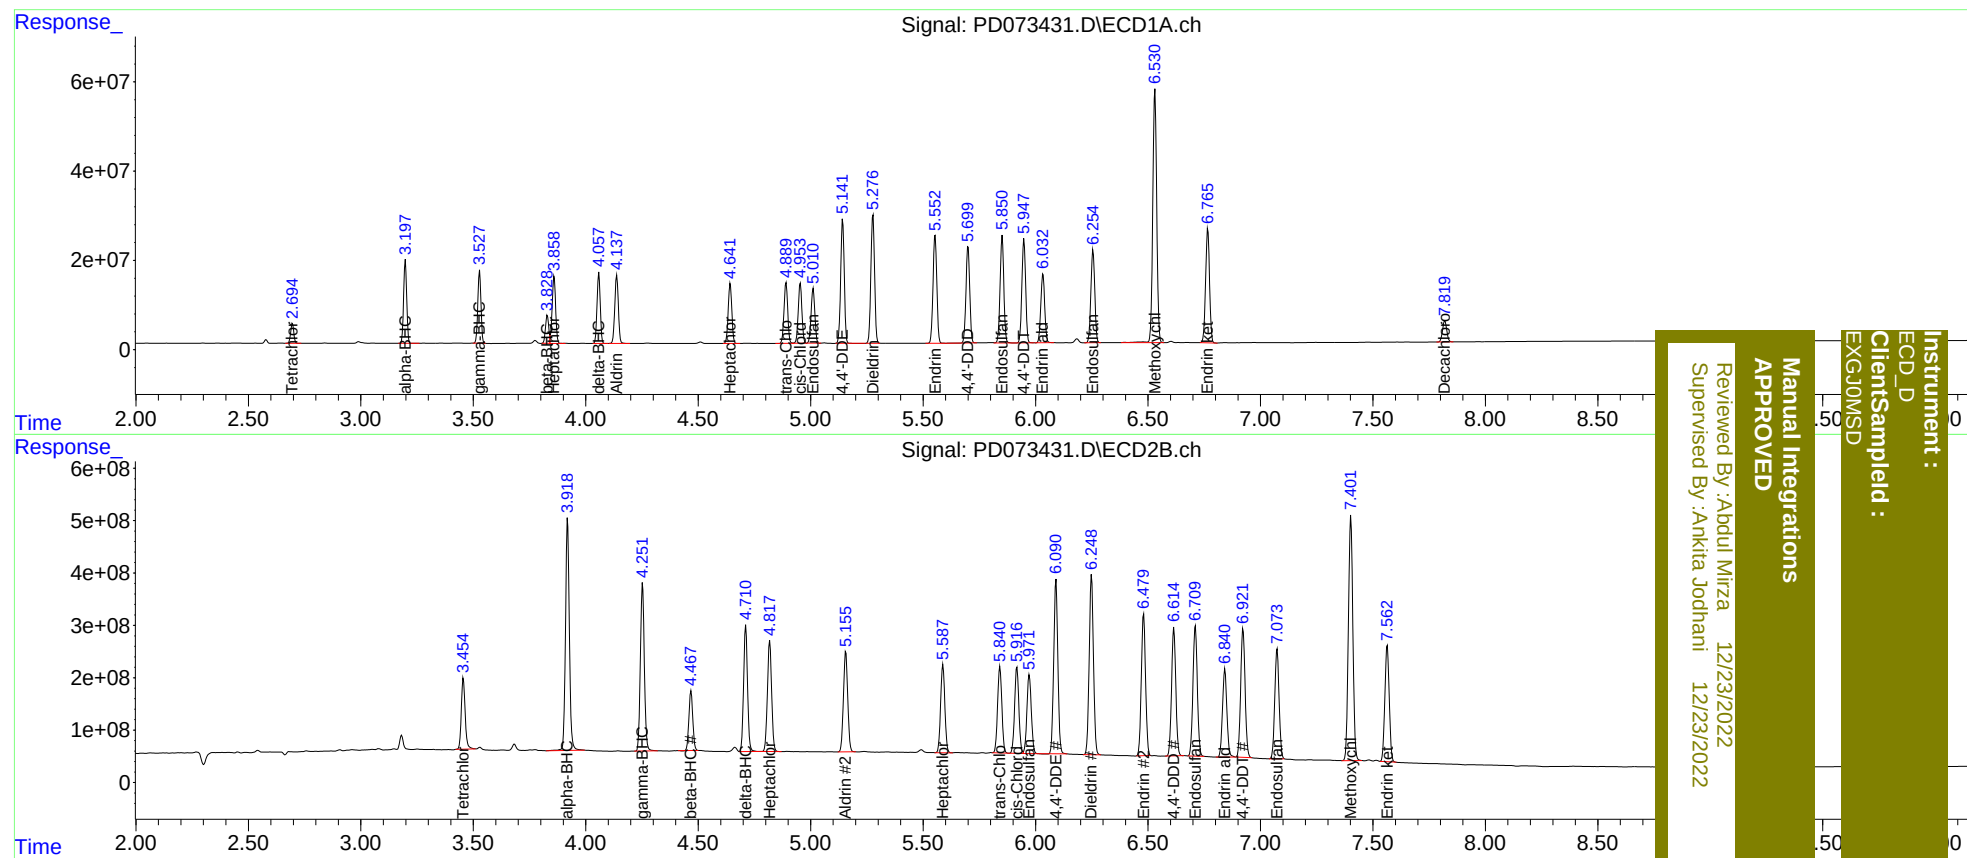

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 12/23/2022
Supervised By: Ankita Jodhani 12/23/2022

Instrument :
ECD_D
Client Sampled :
EXGJ0MSD