

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122222\
 Data File : PD073430.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2022 04:53
 Operator : AR\AJ
 Sample : N6130-02MS 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EXGJ0MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 23 09:55:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122222CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 22 04:14:38 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.701	3.455	41450829	1625.9E6	19.475	21.733
2)	SA Decachlor...	7.825	8.902	60529149	488.5E6	23.742	24.877
Target Compounds							
2)	A alpha-BHC	3.204	3.918	168.8E6	5226.6E6	49.644	44.319
3)	MA gamma-BHC...	3.534	4.252	150.9E6	3866.9E6	47.459	43.505
4)	MA Heptachlor	3.865	4.817	160.1E6	2770.4E6	48.471	47.038
5)	MB Aldrin	4.144	5.156	165.6E6	2575.2E6	51.119	50.568
6)	B beta-BHC	3.835	4.467	59538028	1330.0E6	40.271	42.553
7)	B delta-BHC	4.064	4.711	149.3E6	2877.5E6	43.219	40.957
8)	B Heptachlo...	4.648	5.588	146.7E6	2221.8E6	49.395	49.648
9)	A Endosulfan I	5.017	5.972	132.9E6	2018.2E6	47.677	50.836
10)	B trans-Chl...	4.896	5.841	150.5E6	2192.8E6	50.890	51.739
11)	B cis-Chlor...	4.959	5.917	145.8E6	2167.9E6	48.599	50.825
12)	B 4,4'-DDE	5.148	6.091	307.3E6	4237.1E6	104.735	102.135
13)	MA Dieldrin	5.283	6.249	323.2E6	4437.3E6	105.627	107.920
14)	MA Endrin	5.559	6.481	283.3E6	3243.7E6	107.000	96.424
15)	B Endosulfa...	5.857	6.710	269.8E6	3319.9E6	101.599	101.063
16)	A 4,4'-DDD	5.706	6.615	249.8E6	3177.7E6	104.287	100.233
17)	MA 4,4'-DDT	5.954	6.922	267.2E6	3348.2E6	110.253	110.952
18)	B Endrin al...	6.038	6.841	179.1E6	2216.0E6	84.259	86.190
19)	B Endosulfa...	6.261	7.074	241.0E6	2645.4E6	96.440	95.519
20)	A Methoxychlor	6.536	7.402	680.9E6	6314.7E6	510.205	511.939
21)	B Endrin ke...	6.771	7.564	303.6E6	2918.6E6	101.571	98.398

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122222\
Data File : PD073430.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2022 04:53
Operator : AR\AJ
Sample : N6130-02MS 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 23 09:55:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122222CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 22 04:14:38 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

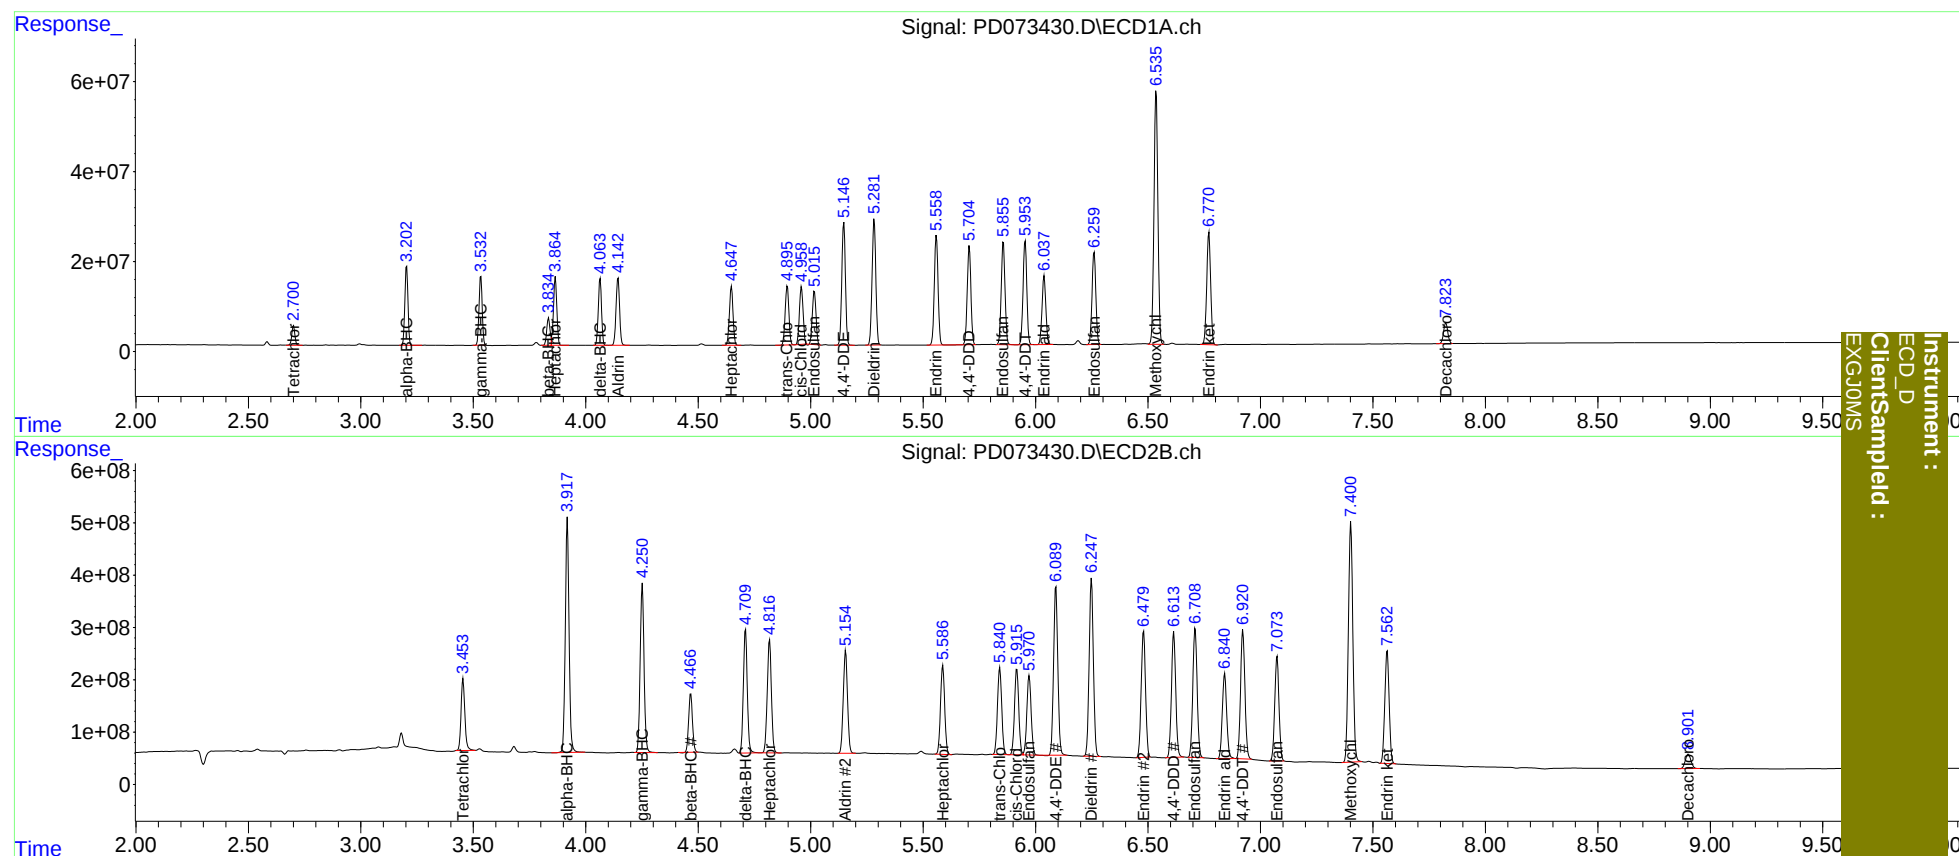

Instrument :
ECD_D
ClientSampled :
EXGJ0MS