

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122223\
 Data File : PD080260.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2023 12:51
 Operator : AR\AJ
 Sample : 05818-04MSD
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGRG7MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/22/2023
 Supervised By : Ankita Jodhani 12/22/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 20:34:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 18 00:44:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.801	13309914	32476317	10.425m	14.606 #
27)	SA Decachlor...	9.095	7.936	288.8E6	132.9E6	179.617	55.388 #
Target Compounds							
2)	A alpha-BHC	4.024	3.303	92744923	167.6E6	44.990	49.162
3)	MA gamma-BHC...	4.356	3.635	74522719	283.0E6	37.529m	87.906 #
4)	MA Heptachlor	4.948	3.971	71558899	104.3E6	34.267m	32.571m
5)	MB Aldrin	5.291	4.254	80738536	131.7E6	36.096	37.276
6)	B beta-BHC	4.551	3.925	14381660	34901557	13.855m	20.327m#
7)	B delta-BHC	4.801	4.157	71739498	171.2E6	31.234	44.033 #
8)	B Heptachlo...	5.719	4.755	65284272	103.4E6	30.390	30.522
9)	A Endosulfan I	6.137	5.151	302.3E6	924.8E6	169.708m	337.329m#
10)	B trans-Chl...	5.972	5.010	43870362	159.6E6	21.377m	48.481 #
11)	B cis-Chlor...	6.052	5.070	114.5E6	99198118	54.542	29.505 #
12)	B 4,4'-DDE	6.226	5.259	311.7E6	474.2E6	161.340	150.978
13)	MA Dieldrin	6.396	5.393	336.5E6	571.7E6	180.827m	190.773m
14)	MA Endrin	6.615	5.664	216.5E6	294.1E6	138.209m	111.769
15)	B Endosulfa...	6.827	5.959	90858710	284.3E6	48.464	98.062m#
16)	A 4,4'-DDD	6.733	5.811	343.2E6	271.3E6	247.397	118.004 #
17)	MA 4,4'-DDT	7.058	6.063	285.0E6	354.6E6	192.871	147.065
18)	B Endrin al...	6.959	6.139	109.8E6	111.9E6	73.620m	48.524 #
19)	B Endosulfa...	7.193	6.360	134.6E6	179.4E6	73.396m	63.971
20)	A Methoxychlor	7.530	6.637	418.4E6	358.4E6	528.440m	284.690m#
21)	B Endrin ke...	7.679	6.864	142.2E6	137.9E6	73.078m	43.103m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122223\
Data File : PD080260.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2023 12:51
Operator : AR\AJ
Sample : 05818-04MSD
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 20:34:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Mon Dec 18 00:44:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

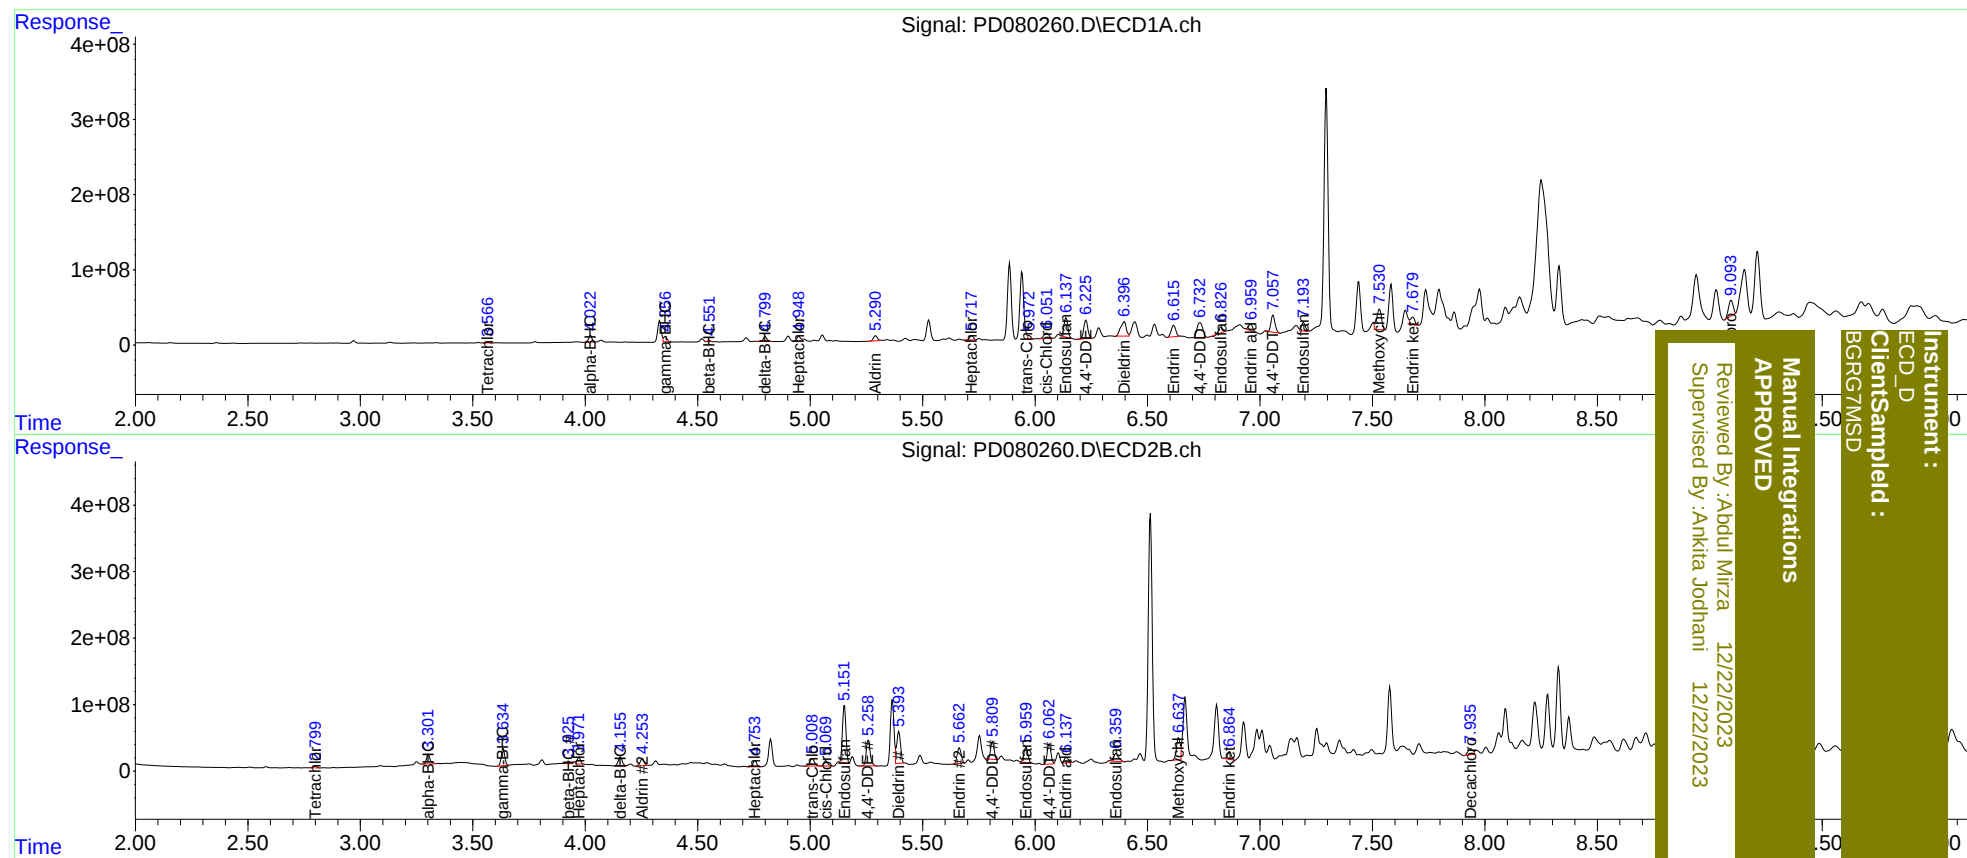

Reviewed By: Abdul Miza 12/22/2023
Supervised By: Ankita Jodhani 12/22/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
BGRGTMSD