

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122223\
 Data File : PD080275.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2023 17:35
 Operator : AR\AJ
 Sample : 05859-05
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGS96

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/21/2023
 Supervised By : Ankita Jodhani 12/22/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 20:45:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 18 00:44:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.800	31442242	57094936	24.626	25.677
27)	SA Decachlor...	9.109	7.940	35774726	54666940	22.251m	22.776
Target Compounds							
8)	B Heptachlo...	5.721	4.749	3440441	3332028	1.602	0.983m#
12)	B 4,4'-DDE	6.199	5.244	2876565	2642690	1.489m	0.841m#
13)	MA Dieldrin	6.382	5.388	10874742	15431610	5.843	5.149m
19)	B Endosulfa...	7.187	6.383	7910342	5585009	4.313m	1.991m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122223\
Data File : PD080275.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2023 17:35
Operator : AR\AJ
Sample : 05859-05
Misc :
ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 20:45:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Mon Dec 18 00:44:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

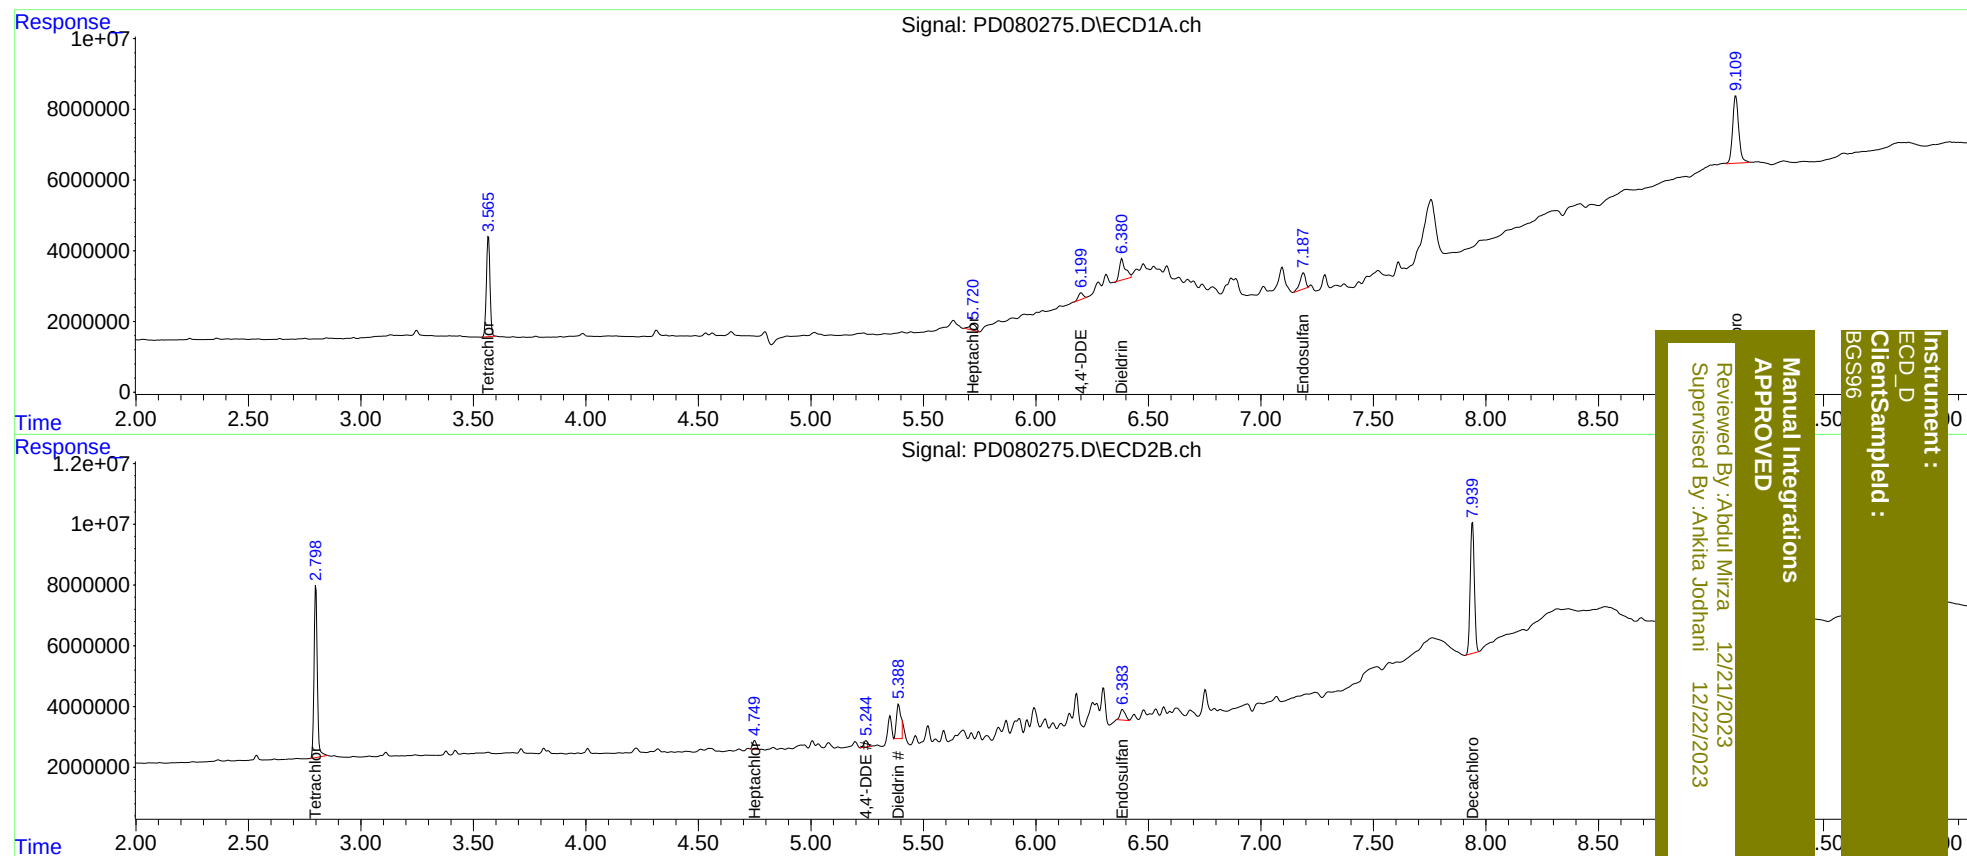

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 12/21/2023
Supervised By: Ankita Jodhani 12/22/2023

Instrument :
ECD_D
Client Sampled :
BGS96