

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122224\
 Data File : PD087271.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2024 21:32
 Operator : AR\AJ
 Sample : P5247-06MSD
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH7T5MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/23/2024
 Supervised By :mohammad ahmed 12/25/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 02:46:43 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122024CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 20 23:32:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.883	39420434	238.0E6	19.254m	20.449
27)	SA Decachlor...	9.087	8.086	59360950	264.4E6	19.436	20.072
Target Compounds							
2)	A alpha-BHC	4.006	3.397	229.1E6	952.7E6	56.774	52.267
3)	MA gamma-BHC...	4.337	3.734	223.7E6	886.2E6	57.282	52.381
4)	MA Heptachlor	4.937	4.089	211.2E6	843.0E6	53.222	48.753
5)	MB Aldrin	5.279	4.376	204.1E6	811.2E6	52.389	48.472
6)	B beta-BHC	4.521	4.030	86179767	375.2E6	49.283	47.936
7)	B delta-BHC	4.770	4.267	145.9E6	605.7E6	36.686	34.889
8)	B Heptachlo...	5.699	4.880	196.3E6	786.9E6	54.392	50.190
9)	A Endosulfan I	6.082	5.254	180.3E6	735.9E6	53.987m	50.769m
10)	B trans-Chl...	5.954	5.134	187.6E6	807.8E6	53.669	49.646
11)	B cis-Chlor...	6.035	5.197	195.6E6	807.0E6	55.073m	51.375m
12)	B 4,4'-DDE	6.205	5.384	375.3E6	1525.3E6	113.423	102.390
13)	MA Dieldrin	6.356	5.521	410.4E6	1559.2E6	113.489	101.845
14)	MA Endrin	6.583	5.798	343.8E6	1424.2E6	115.075	101.941
15)	B Endosulfa...	6.794	6.090	322.1E6	1353.1E6	107.744	99.655
16)	A 4,4'-DDD	6.713	5.939	294.4E6	1264.3E6	113.583	103.830
17)	MA 4,4'-DDT	7.029	6.194	308.0E6	1323.3E6	114.899m	104.958
18)	B Endrin al...	6.923	6.268	247.4E6	1025.1E6	105.421	98.111
19)	B Endosulfa...	7.157	6.492	299.2E6	1267.7E6	103.231	95.892
20)	A Methoxychlor	7.502	6.766	785.2E6	2730.6E6	527.754	468.375
21)	B Endrin ke...	7.639	7.001	348.4E6	1447.8E6	108.561	100.162

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122224\
Data File : PD087271.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2024 21:32
Operator : AR\AJ
Sample : P5247-06MSD
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 02:46:43 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122024CLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 23:32:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

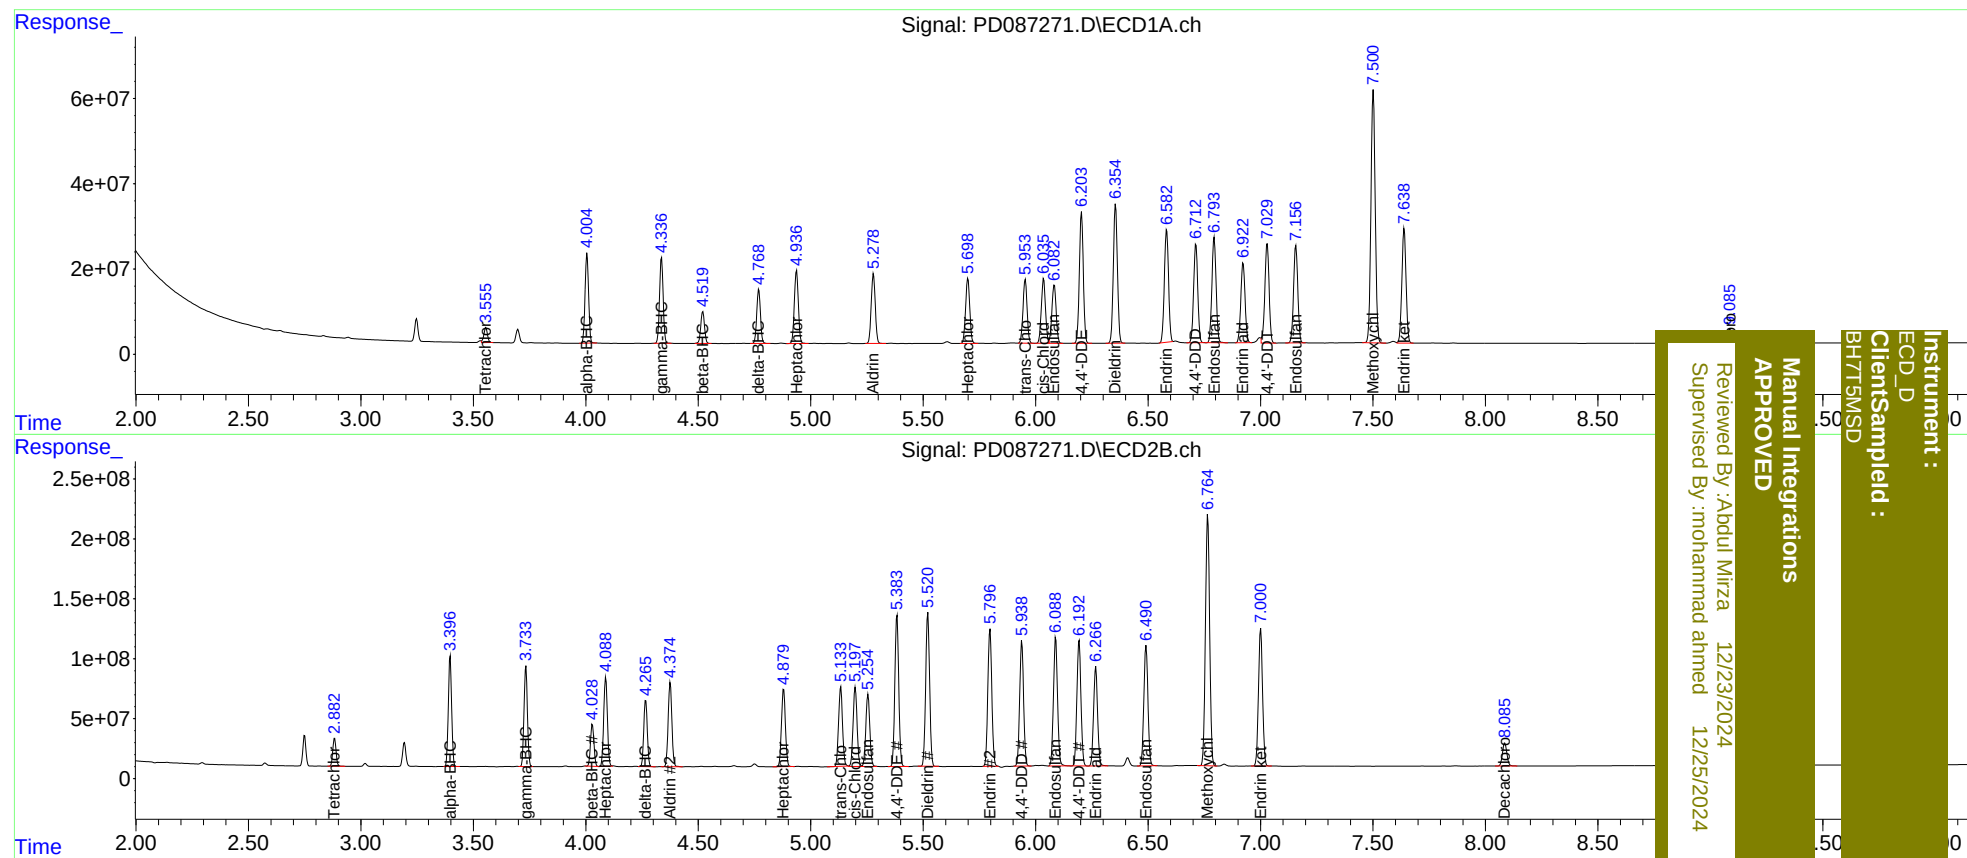

Instrument :
ECD_D
ClientSampled :
BHT/MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 12/23/2024
Supervised By: mohammad ahmed 12/25/2024