

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122319\
 Data File : PD056758.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2019 21:07
 Operator : SG\AJ
 Sample : K6279-09
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 00:43:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.286	3.961	9106350	16952766	10.995	14.101 #
27) SA Decachlor...	7.959	8.998	14935865	20970638	16.541	17.430
Target Compounds						
4) MA Heptachlor	0.000	5.091f	0	8925651	N.D.	5.477


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122319\
Data File : PD056758.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2019 21:07
Operator : SG\AJ
Sample : K6279-09
Misc :
ALS Vial : 43 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 00:43:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

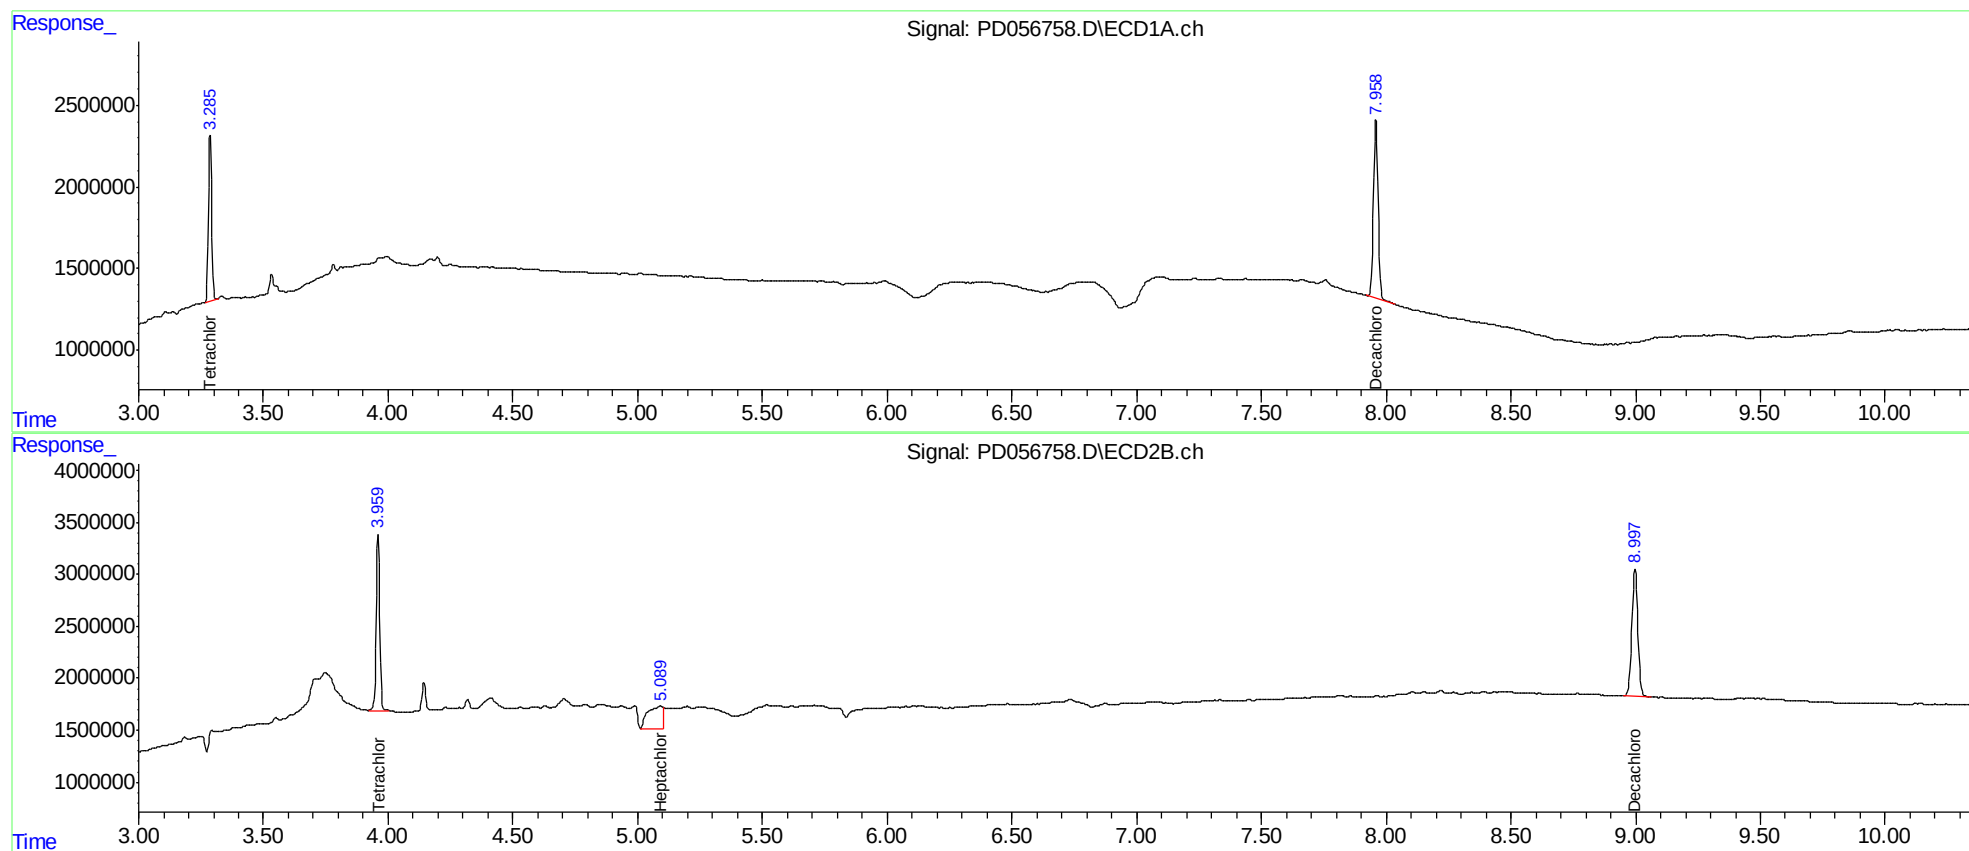

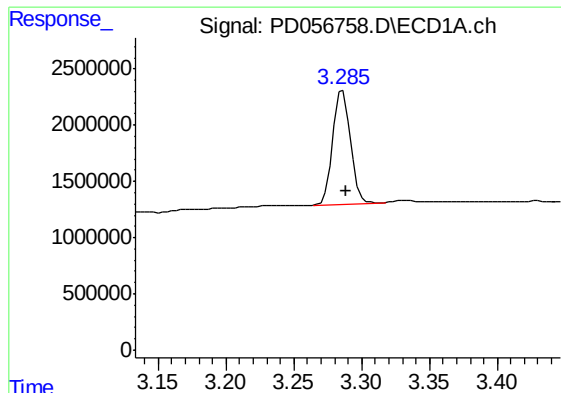


#1 Tetrachloro-m-xylene

R.T.: 3.286 min
Delta R.T.: -0.002 min
Response: 9106350
Conc: 11.00 ng/ml

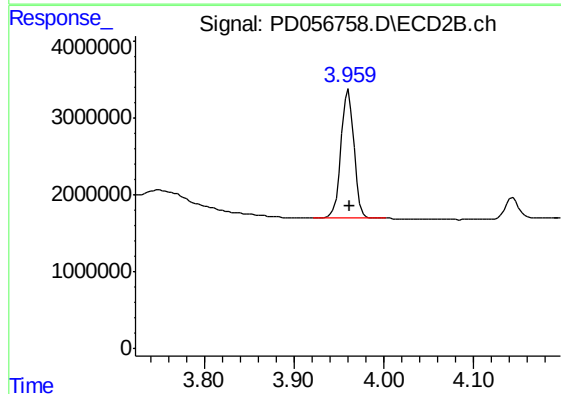


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: -0.002 min
Response: 16952766
Conc: 14.10 ng/ml

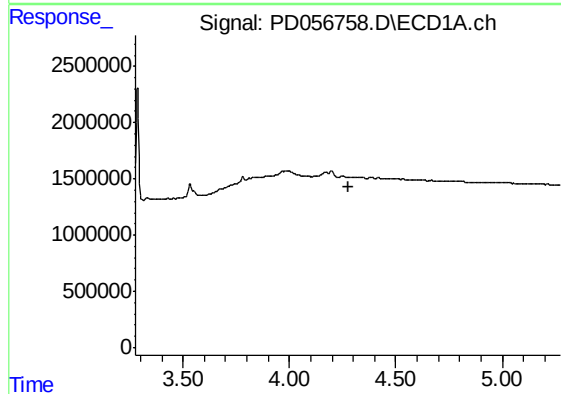


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 4.276 min
Response: 0
Conc: N.D.

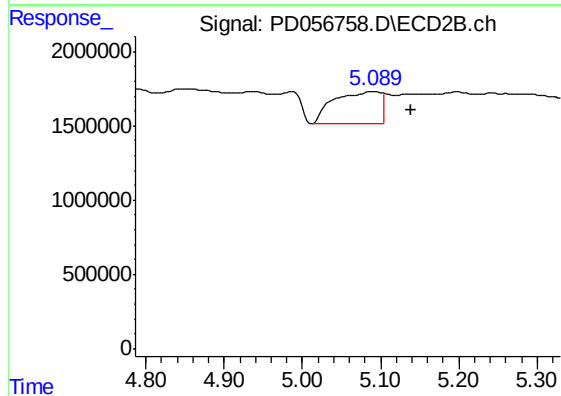


#4 Heptachlor

R.T.: 5.091 min
Delta R.T.: -0.048 min
Response: 8925651
Conc: 5.48 ng/ml

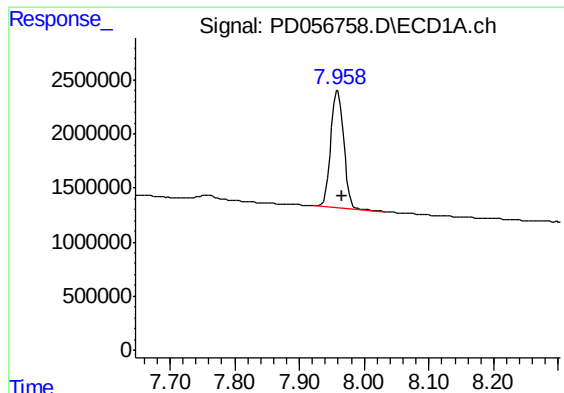

#27 Decachlorobiphenyl

R.T.: 7.959 min
Delta R.T.: -0.006 min
Response: 14935865
Conc: 16.54 ng/ml

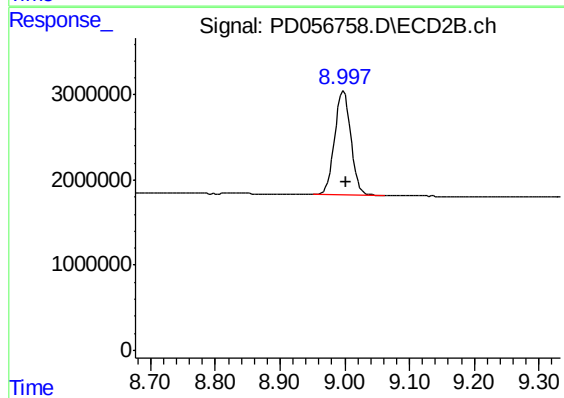

#27 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: -0.004 min
Response: 20970638
Conc: 17.43 ng/ml