

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122319\
 Data File : PD056752.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Dec 2019 19:43
 Operator : SG\AJ
 Sample : K6279-02MS
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFEX7MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 24 00:42:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.286	3.961	14856026	28475618	17.938	23.685 #
27) SA Decachlor...	7.959	8.997	26931354	37931858	29.825	31.527
Target Compounds						
3) MA gamma-BHC...	3.988	4.630	52299420	93616552	46.574	58.009
4) MA Heptachlor	4.274	5.136	50662221	92645840	50.264	56.845
5) MB Aldrin	4.512	5.440	49169228	90281142	45.276	54.943
13) MA Dieldrin	5.519	6.435	98417466	170.8E6	96.890	108.682
14) MA Endrin	5.772	6.652	81292414	136.2E6	97.275	107.650
17) MA 4,4'-DDT	6.142	7.072	68224765	120.4E6	96.959	101.849

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122319\
Data File : PD056752.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Dec 2019 19:43
Operator : SG\AJ
Sample : K6279-02MS
Misc :
ALS Vial : 37 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 24 00:42:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

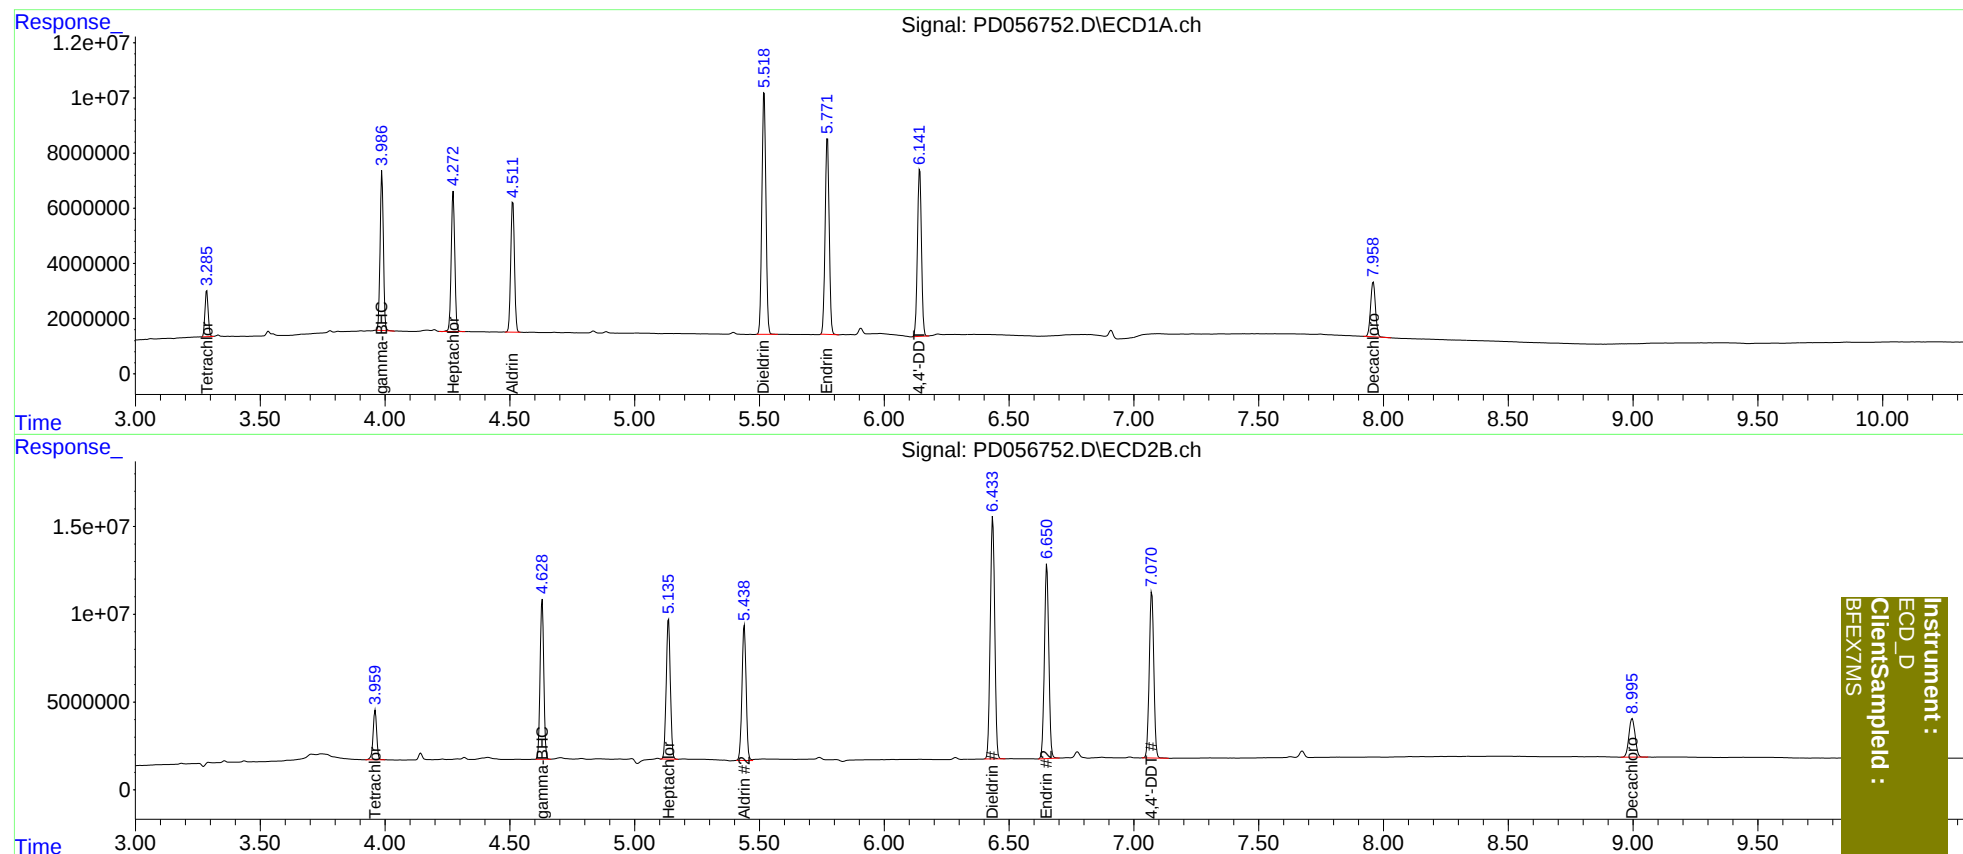

Instrument :
ECD_D
ClientSampled :
BFEEXTMS