

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122322\
 Data File : PD073443.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Dec 2022 15:25
 Operator : AR\AJ
 Sample : N6131-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 22 20:34:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122122CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 16 15:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
28)	SA Decachlor...	7.825	0.000	197528	0	0.082	N.D. #
Target Compounds							
2)	A alpha-BHC	3.200	3.921	133348	8646255	0.039	0.065 #
3)	MA gamma-BHC...	3.543	4.242	162133	7861897	0.059	0.080 #
5)	MB Aldrin	0.000	5.155	0	4697536	N.D.	0.085 #
7)	B delta-BHC	0.000	4.697f	0	1250160	N.D.	0.019 #
8)	B Heptachlo...	0.000	5.588	0	80256504	N.D.	1.800 #
13)	MA Dieldrin	0.000	6.262	0	9718364	N.D.	0.231 #
14)	MA Endrin	5.529f	0.000	333857	0	0.130	N.D. #
16)	A 4,4'-DDD	0.000	6.638f	0	45070600	N.D.	1.443 #
19)	B Endosulfa...	6.275	0.000	201241	0	0.085	N.D. #
20)	A Methoxychlor	6.549	0.000	148816	0	0.112	N.D. #
23)	Chlordane-1	0.000	4.608	0	2631830	N.D.	1.039 #
24)	Chlordane-2	4.238f	5.136	89542	1656439	0.898	0.991
27)	Chlordane-5	0.000	6.784	0	1775400	N.D.	1.496 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122322\
Data File : PD073443.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Dec 2022 15:25
Operator : AR\AJ
Sample : N6131-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 22 20:34:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122122CLP.M
Quant Title : GC Extractables
QLast Update : Fri Dec 16 15:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

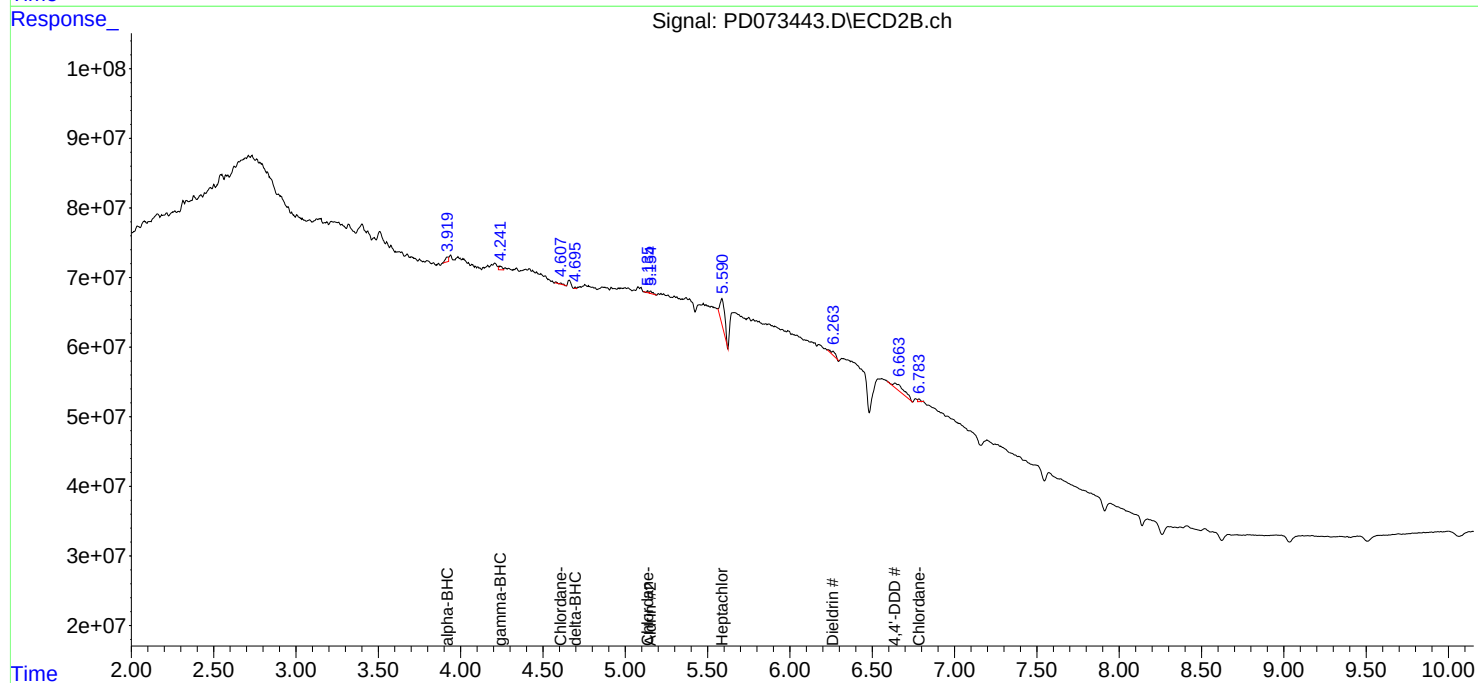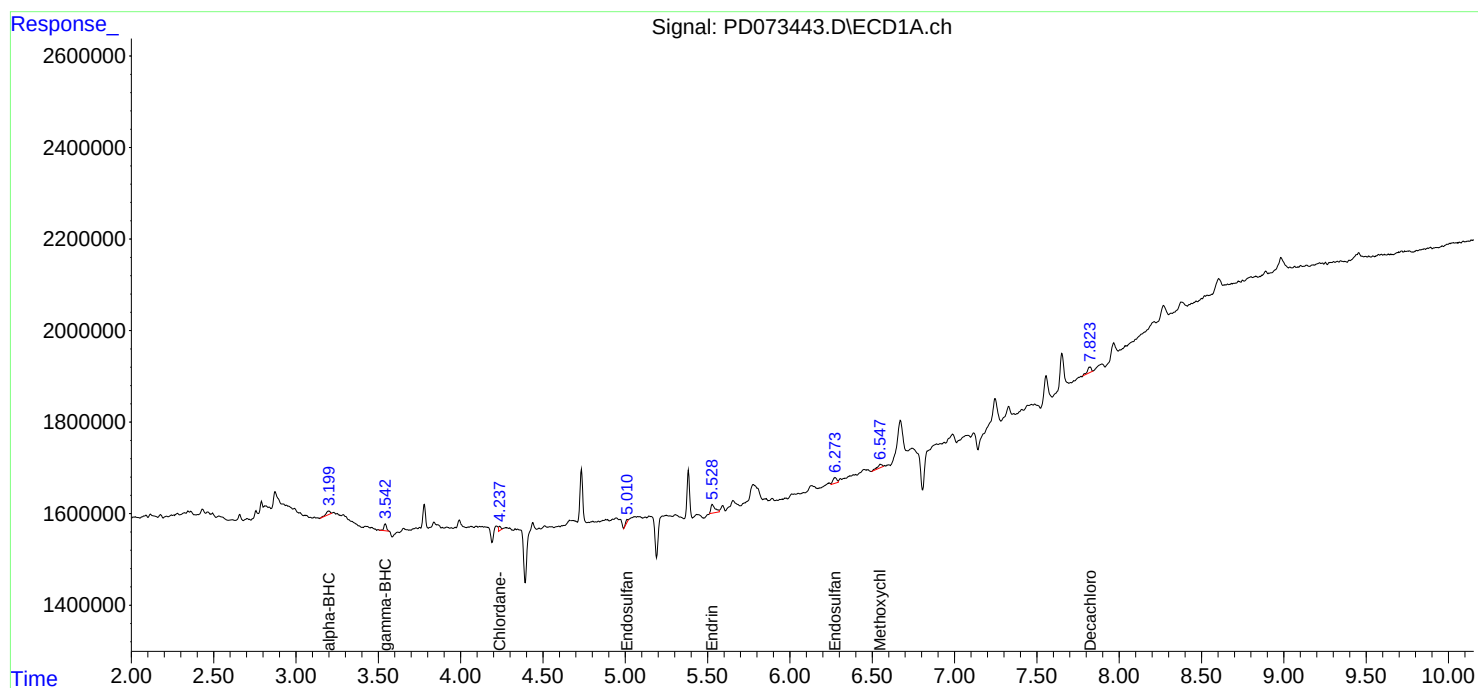

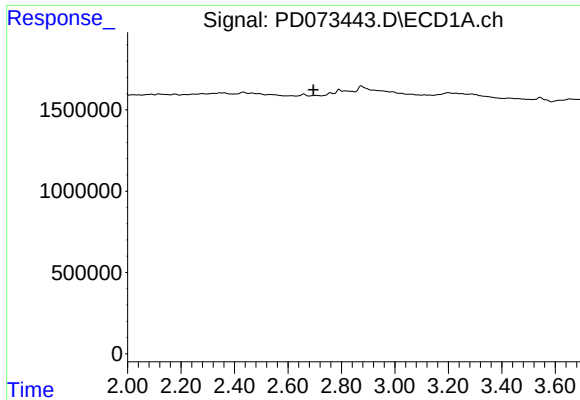


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.696 min
Response: 0
Conc: N.D.

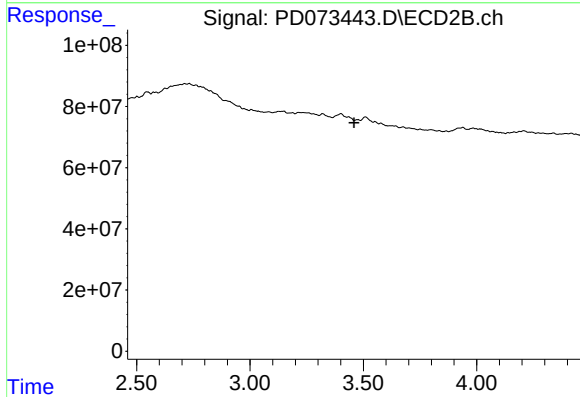


#1 Tetrachloro-m-xylene

R.T.: 3.477 min
Delta R.T.: 0.018 min
Response: -2866543
Conc: N.D.

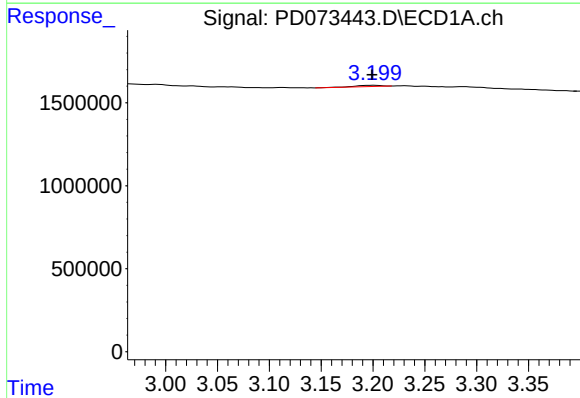


#2 alpha-BHC

R.T.: 3.200 min
Delta R.T.: 0.001 min
Response: 133348
Conc: 0.04 ng/ml

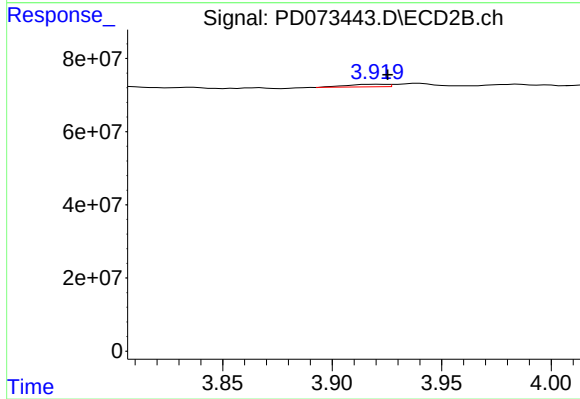

#2 alpha-BHC

R.T.: 3.921 min
Delta R.T.: -0.005 min
Response: 8646255
Conc: 0.06 ng/ml

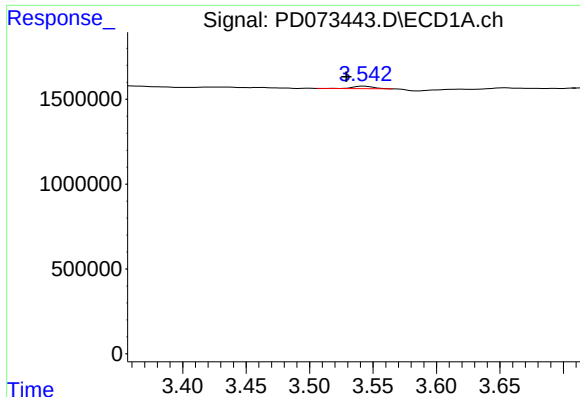


#3 gamma-BHC (Lindane)

R.T.: 3.543 min

Delta R.T.: 0.014 min

Response: 162133

Conc: 0.06 ng/ml

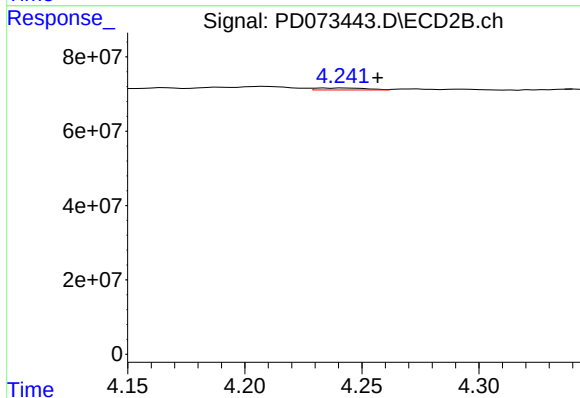


#3 gamma-BHC (Lindane)

R.T.: 4.242 min

Delta R.T.: -0.015 min

Response: 7861897

Conc: 0.08 ng/ml

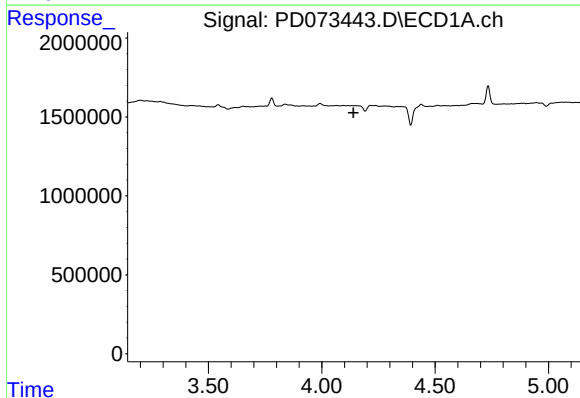


#5 Aldrin

R.T.: 0.000 min

Exp R.T. : 4.140 min

Response: 0

Conc: N.D.

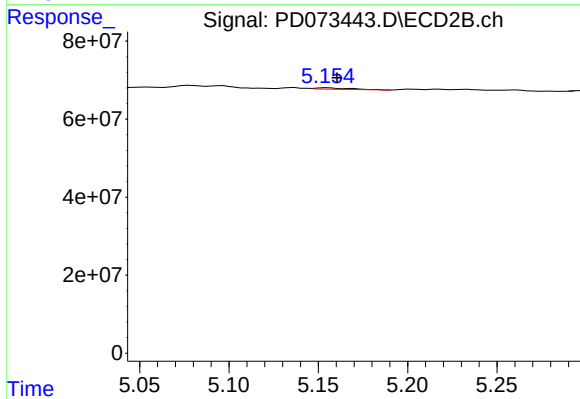


#5 Aldrin

R.T.: 5.155 min

Delta R.T.: -0.006 min


Response: 4697536

Conc: 0.09 ng/ml

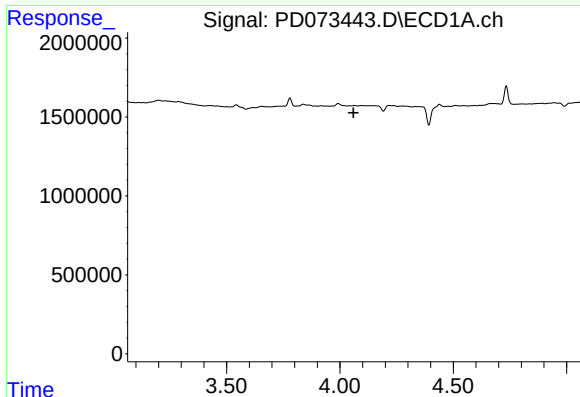


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.060 min
Response: 0
Conc: N.D.

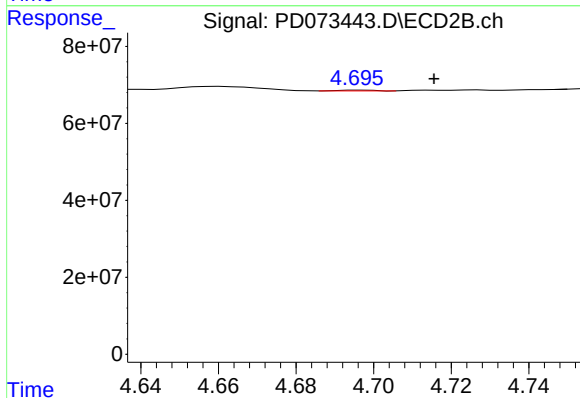


#7 delta-BHC

R.T.: 4.697 min
Delta R.T.: -0.019 min
Response: 1250160
Conc: 0.02 ng/ml

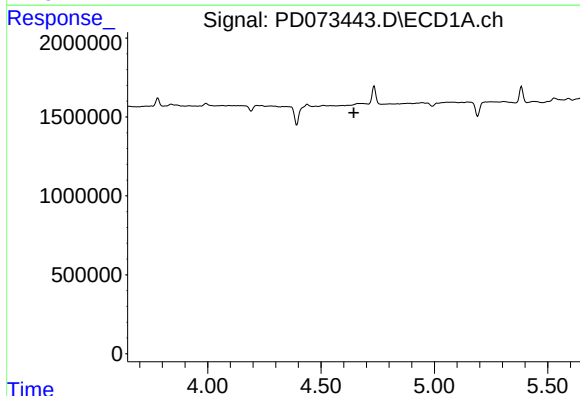


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.645 min
Response: 0
Conc: N.D.

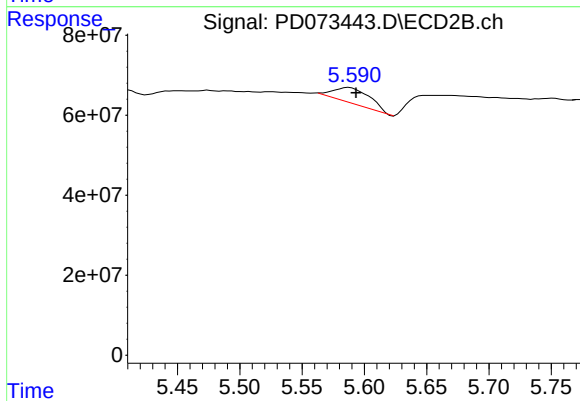


#8 Heptachlor epoxide

R.T.: 5.588 min
Delta R.T.: -0.006 min
Response: 80256504
Conc: 1.80 ng/ml

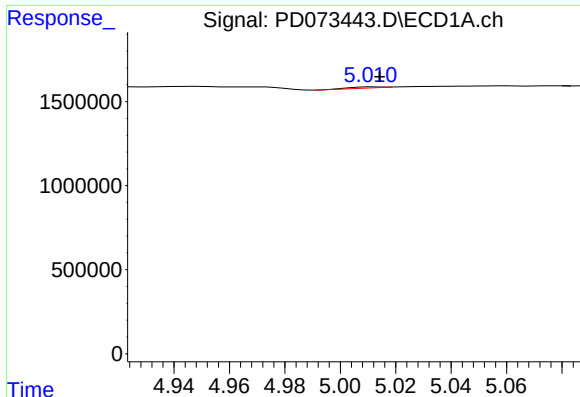


#9 Endosulfan I

R.T.: 5.012 min
Delta R.T.: -0.002 min
Response: 44925
Conc: 0.02 ng/ml

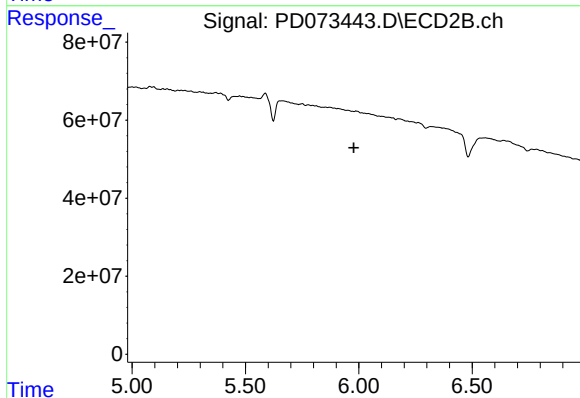


#9 Endosulfan I

R.T.: 5.989 min
Delta R.T.: 0.012 min
Response: -1385299
Conc: N.D.

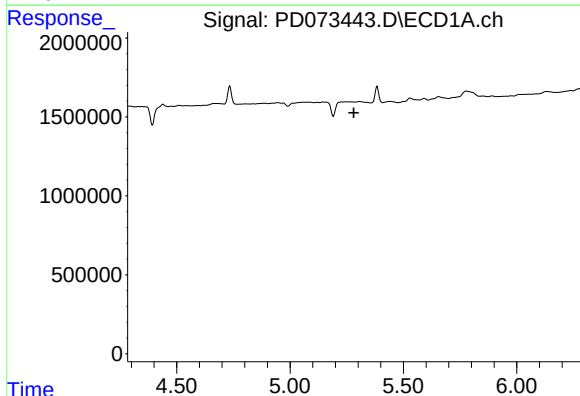


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 5.281 min
Response: 0
Conc: N.D.

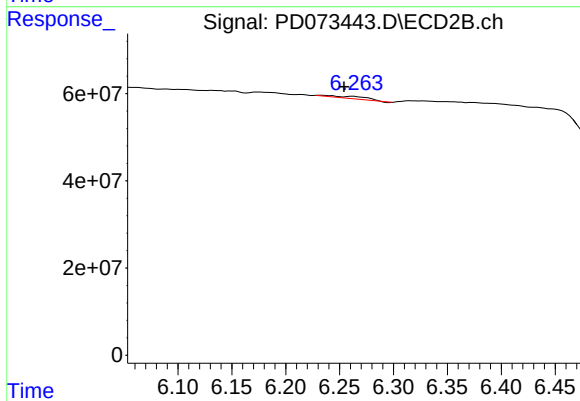


#13 Dieldrin

R.T.: 6.262 min
Delta R.T.: 0.008 min
Response: 9718364
Conc: 0.23 ng/ml

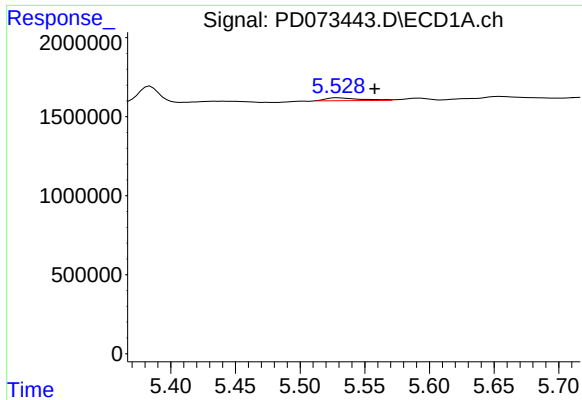


#14 Endrin

R.T.: 5.529 min
Delta R.T.: -0.029 min
Response: 333857
Conc: 0.13 ng/ml

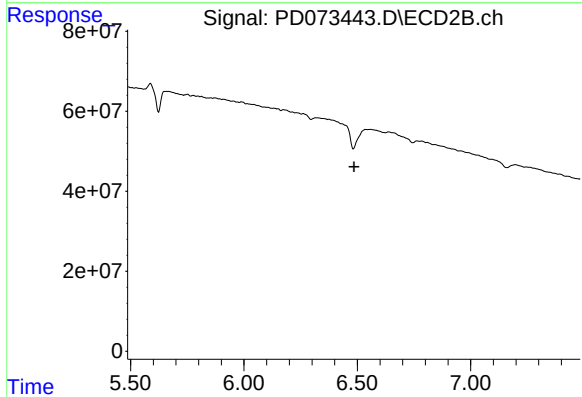


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.486 min
Response: 0
Conc: N.D.

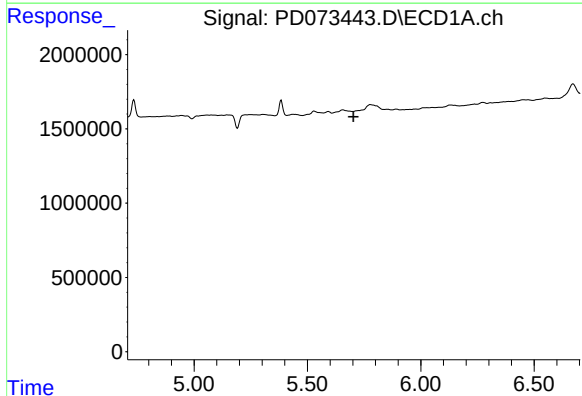


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.704 min
Response: 0
Conc: N.D.

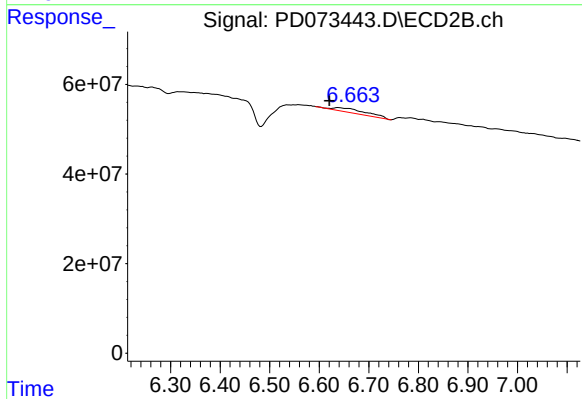


#16 4,4'-DDD

R.T.: 6.638 min
Delta R.T.: 0.018 min
Response: 45070600
Conc: 1.44 ng/ml

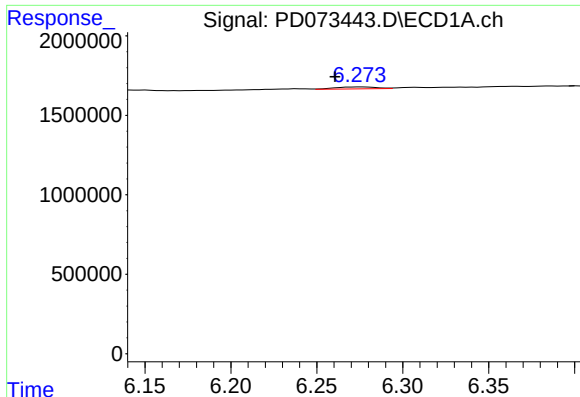


#19 Endosulfan Sulfate

R.T.: 6.275 min
Delta R.T.: 0.015 min
Response: 201241
Conc: 0.08 ng/ml

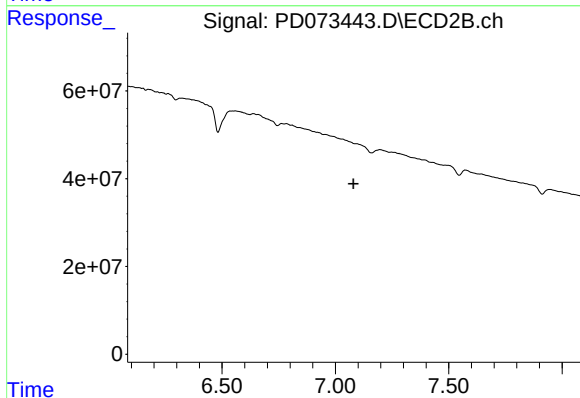


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 7.080 min
Response: 0
Conc: N.D.

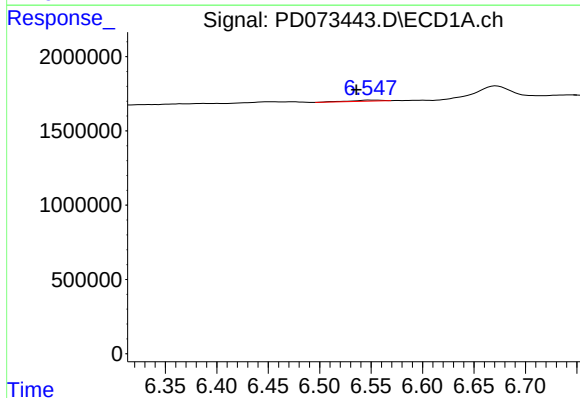


#20 Methoxychlor

R.T.: 6.549 min
Delta R.T.: 0.013 min
Response: 148816
Conc: 0.11 ng/ml

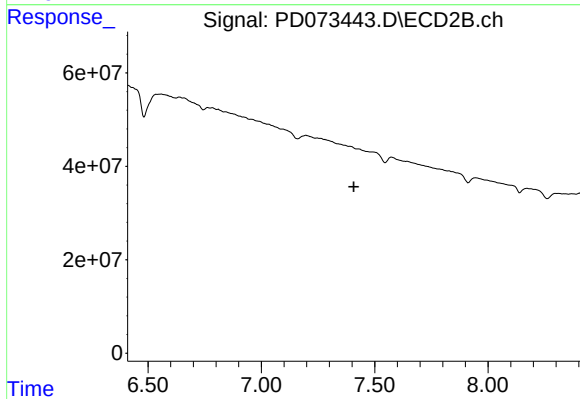


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.408 min
Response: 0
Conc: N.D.

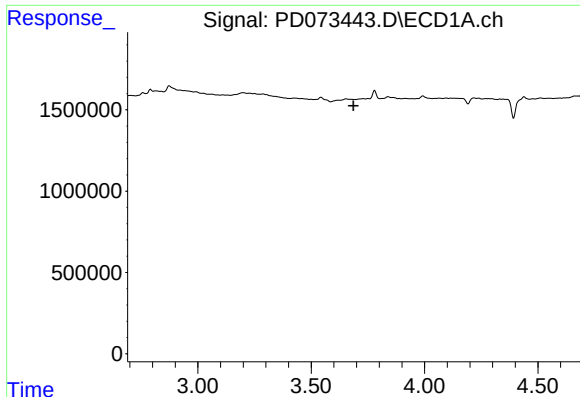


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 3.687 min
Response: 0
Conc: N.D.

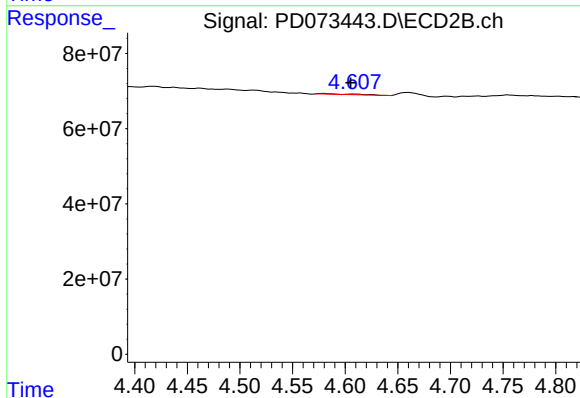


#23 Chlordane-1

R.T.: 4.608 min
Delta R.T.: 0.003 min
Response: 2631830
Conc: 1.04 ng/ml

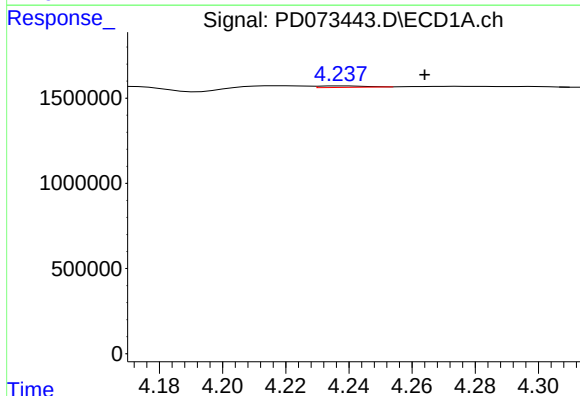


#24 Chlordane-2

R.T.: 4.238 min
Delta R.T.: -0.026 min
Response: 89542
Conc: 0.90 ng/ml

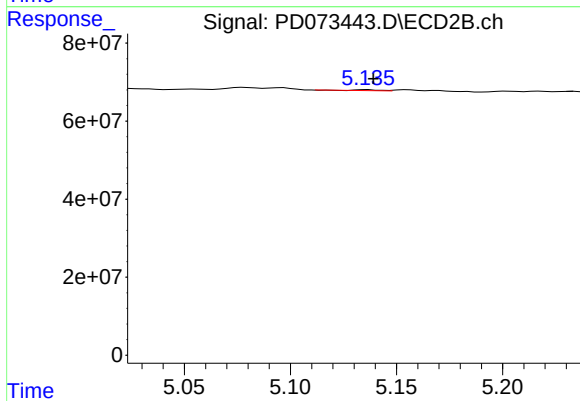


#24 Chlordane-2

R.T.: 5.136 min
Delta R.T.: -0.003 min
Response: 1656439
Conc: 0.99 ng/ml

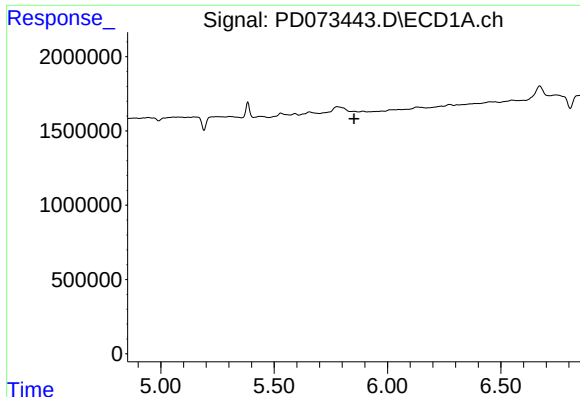


#27 Chlorine-5

R.T.: 0.000 min
Exp R.T.: 5.853 min
Response: 0
Conc: N.D.

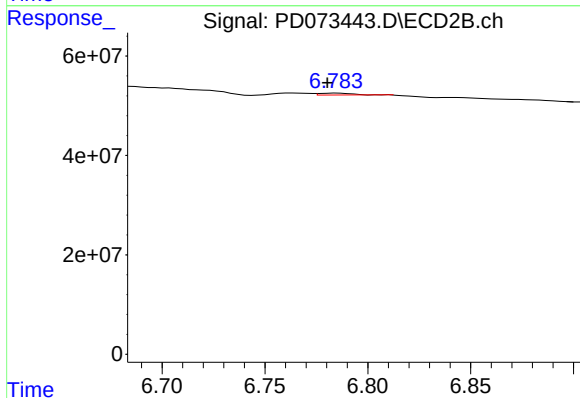


#27 Chlorine-5

R.T.: 6.784 min
Delta R.T.: 0.004 min
Response: 1775400
Conc: 1.50 ng/ml

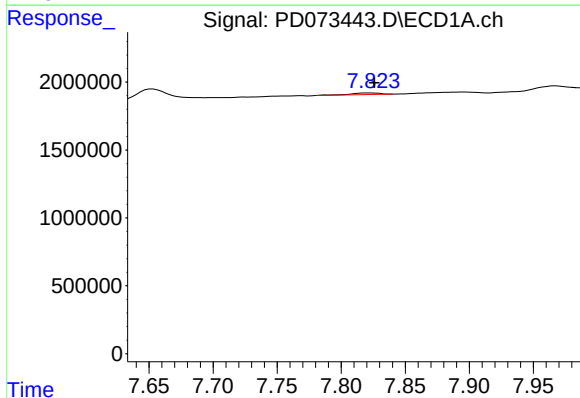

#28 Decachlorobiphenyl

R.T.: 7.825 min
Delta R.T.: -0.001 min
Response: 197528
Conc: 0.08 ng/ml

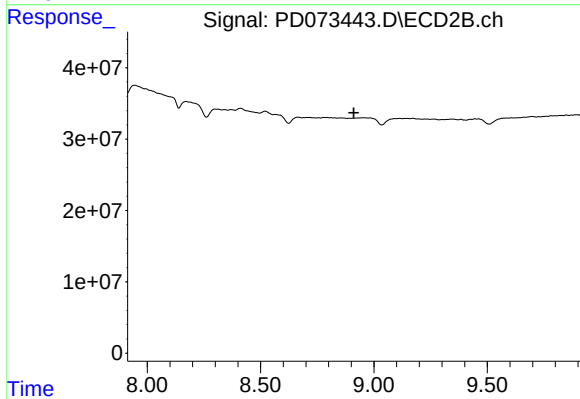

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.911 min
Response: 0
Conc: N.D.