

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122323\
 Data File : PD080298.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2023 23:35
 Operator : AR\AJ
 Sample : 05823-01 10X
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AW7

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/21/2023
 Supervised By :Ankita Jodhani 12/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 02:55:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121723CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 02:51:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.567	2.800	30199905	53732201	21.183	21.775
27) SA Decachlor...	9.110	7.939	40485431	65261656	22.721	24.075
Target Compounds						
17) MA 4,4'-DDT	7.042	6.047	968733	1288302	0.563m	0.464m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122323\
Data File : PD080298.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2023 23:35
Operator : AR\AJ
Sample : 05823-01 10X
Misc :
ALS Vial : 50 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 02:55:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121723CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 02:51:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

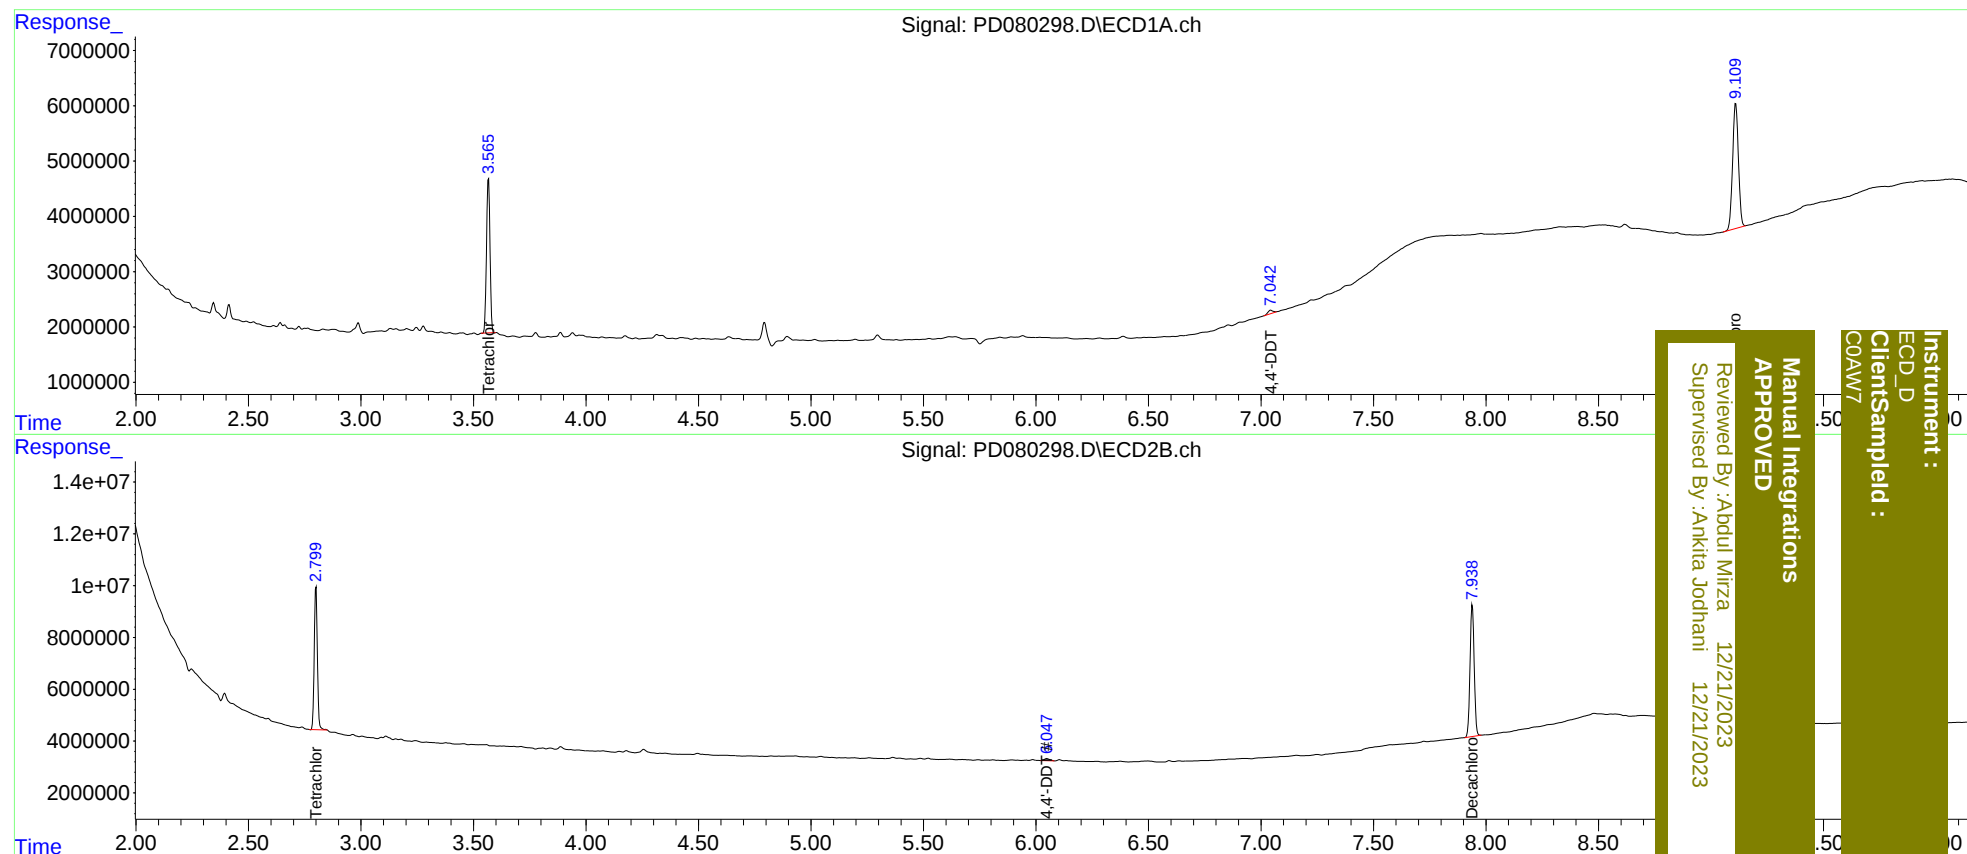

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 12/21/2023
Supervised By: Ankita Jodhani 12/21/2023

Instrument :
ECD_D
ClientSampled :
COAW7