

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD122323\  
 Data File : PD080298.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 20 Dec 2023 23:35  
 Operator : AR\AJ  
 Sample : 05823-01 10X  
 Misc :  
 ALS Vial : 50 Sample Multiplier: 1

**Instrument :**  
 ECD\_D  
**ClientSampleId :**  
 C0AW7

**Manual Integrations**  
**APPROVED**  
 Reviewed By :Abdul Mirza 12/21/2023  
 Supervised By :Ankita Jodhani 12/21/2023

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Dec 21 02:55:22 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD121723CLP-TCLP.M  
 Quant Title : GC Extractables  
 QLast Update : Sat Dec 16 02:51:51 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm


Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
-----						
System Monitoring Compounds						
1) SA Tetrachlo...	3.567	2.800	30199905	53732201	21.183	21.775
27) SA Decachlor...	9.110	7.939	40485431	65261656	22.721	24.075
Target Compounds						
17) MA 4,4'-DDT	7.042	6.047	968733	1288302	0.563m	0.464m
-----						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD122323\  
 Data File : PD080298.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 20 Dec 2023 23:35  
 Operator : AR\AJ  
 Sample : 05823-01 10X  
 Misc :  
 ALS Vial : 50 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Dec 21 02:55:22 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD121723CLP-TCLP.M  
 Quant Title : GC Extractables  
 QLast Update : Sat Dec 16 02:51:51 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

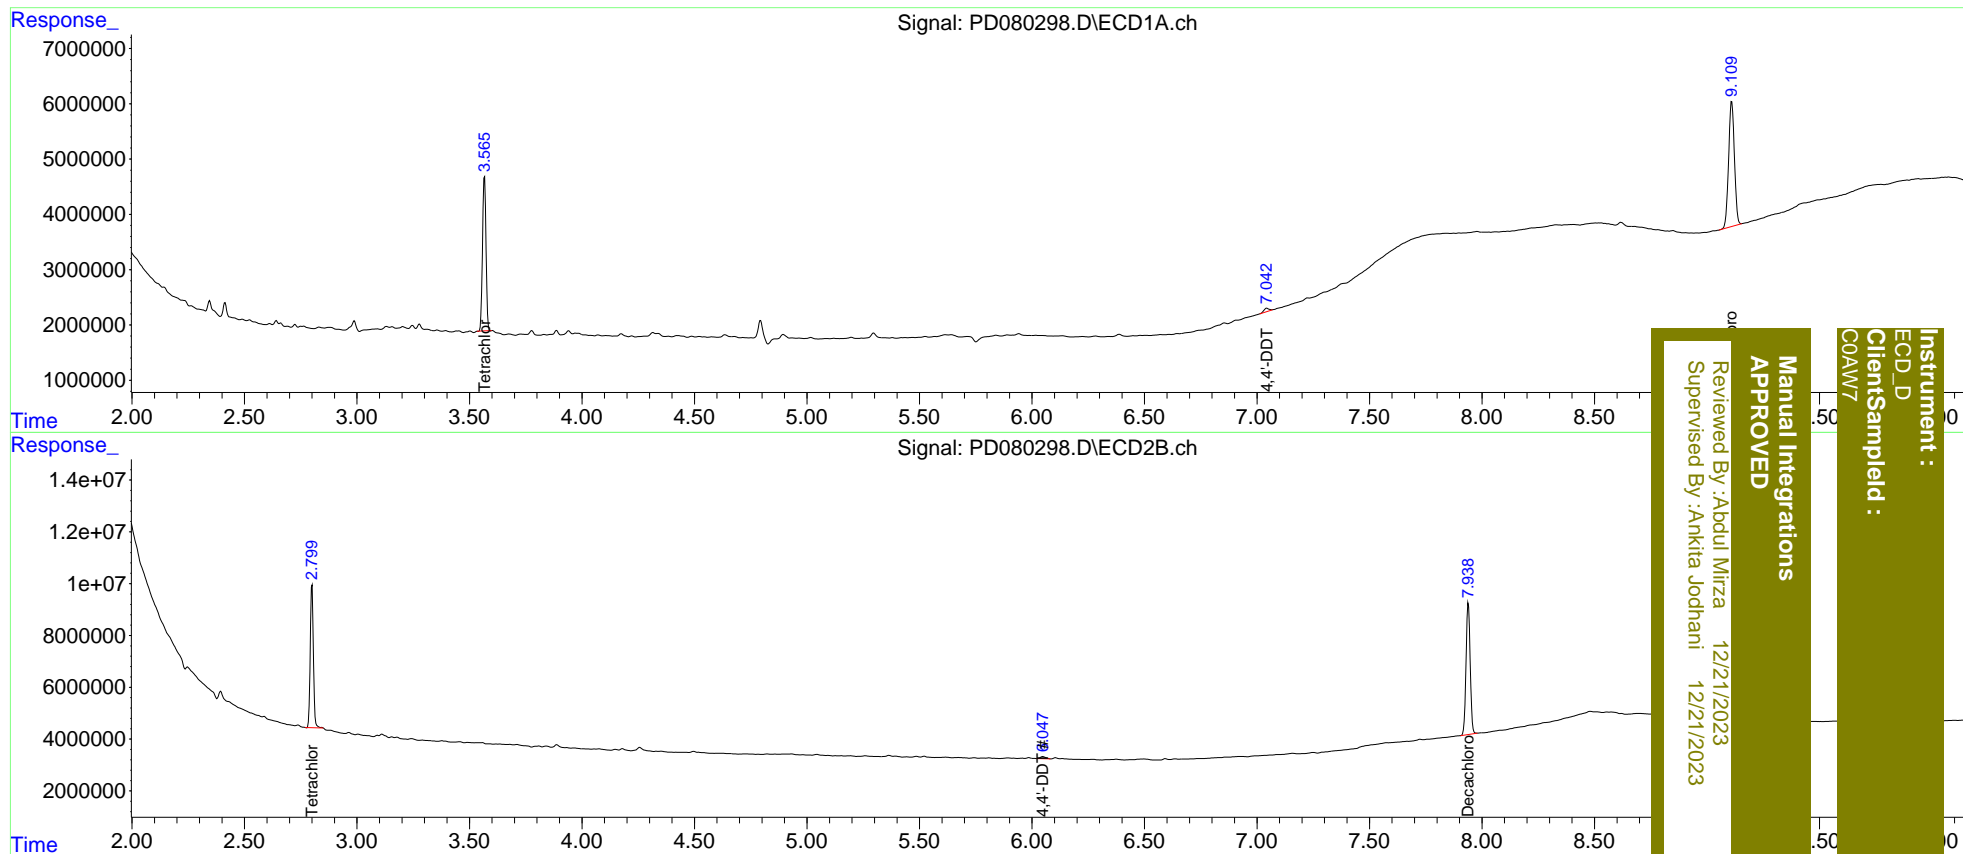

Instrument : ECD\_D  
 ClientSampled : COAW7  
 Manual Integrations APPROVED  
 Reviewed By :Abdul Mirza 12/21/2023  
 Supervised By :Ankita Jodhani 12/21/2023