

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122323\
 Data File : PD080300.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Dec 2023 00:02
 Operator : AR\AJ
 Sample : 05823-03MSD 10X
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AW7MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 02:56:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121723CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 02:51:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.568	2.800	29105298	52064969	20.416	21.099
2)	SA Decachlor...	9.111	7.940	39208486	63105566	22.004	23.279
Target Compounds							
2)	A alpha-BHC	4.024	3.302	128.8E6	213.6E6	53.068	54.418
3)	MA gamma-BHC...	4.357	3.631	115.4E6	192.1E6	49.929	52.251
4)	MA Heptachlor	4.950	3.973	116.4E6	183.5E6	48.582	50.704
5)	MB Aldrin	5.293	4.253	111.8E6	181.3E6	50.539	52.016
6)	B beta-BHC	4.551	3.927	48171829	80658280	48.476	47.284
7)	B delta-BHC	4.800	4.157	120.9E6	202.8E6	52.332	52.925
8)	B Heptachlo...	5.719	4.755	106.2E6	172.8E6	50.767	52.415
9)	A Endosulfan I	6.105	5.125	100.8E6	158.8E6	49.292	50.523
10)	B trans-Chl...	5.975	5.005	104.1E6	170.0E6	51.482	52.683
11)	B cis-Chlor...	6.055	5.069	105.6E6	170.8E6	51.233	51.525
12)	B 4,4'-DDE	6.225	5.258	202.1E6	339.0E6	105.336	110.056
13)	MA Dieldrin	6.381	5.389	220.5E6	366.1E6	102.533	105.485
14)	MA Endrin	6.611	5.664	183.7E6	323.9E6	102.544	108.003
15)	B Endosulfa...	6.829	5.956	186.1E6	311.3E6	100.788	107.974
16)	A 4,4'-DDD	6.743	5.811	165.7E6	287.0E6	103.394	108.651
17)	MA 4,4'-DDT	7.057	6.062	172.8E6	284.0E6	100.442	102.160
18)	B Endrin al...	6.959	6.136	133.5E6	220.1E6	92.561	98.094
19)	B Endosulfa...	7.194	6.358	175.4E6	290.1E6	99.594	107.458
20)	A Methoxychlor	7.531	6.636	427.6E6	683.6E6	477.738	493.344
21)	B Endrin ke...	7.680	6.864	189.5E6	336.3E6	99.197	108.369

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD122323\
Data File : PD080300.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Dec 2023 00:02
Operator : AR\AJ
Sample : 05823-03MSD 10X
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 02:56:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121723CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 02:51:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

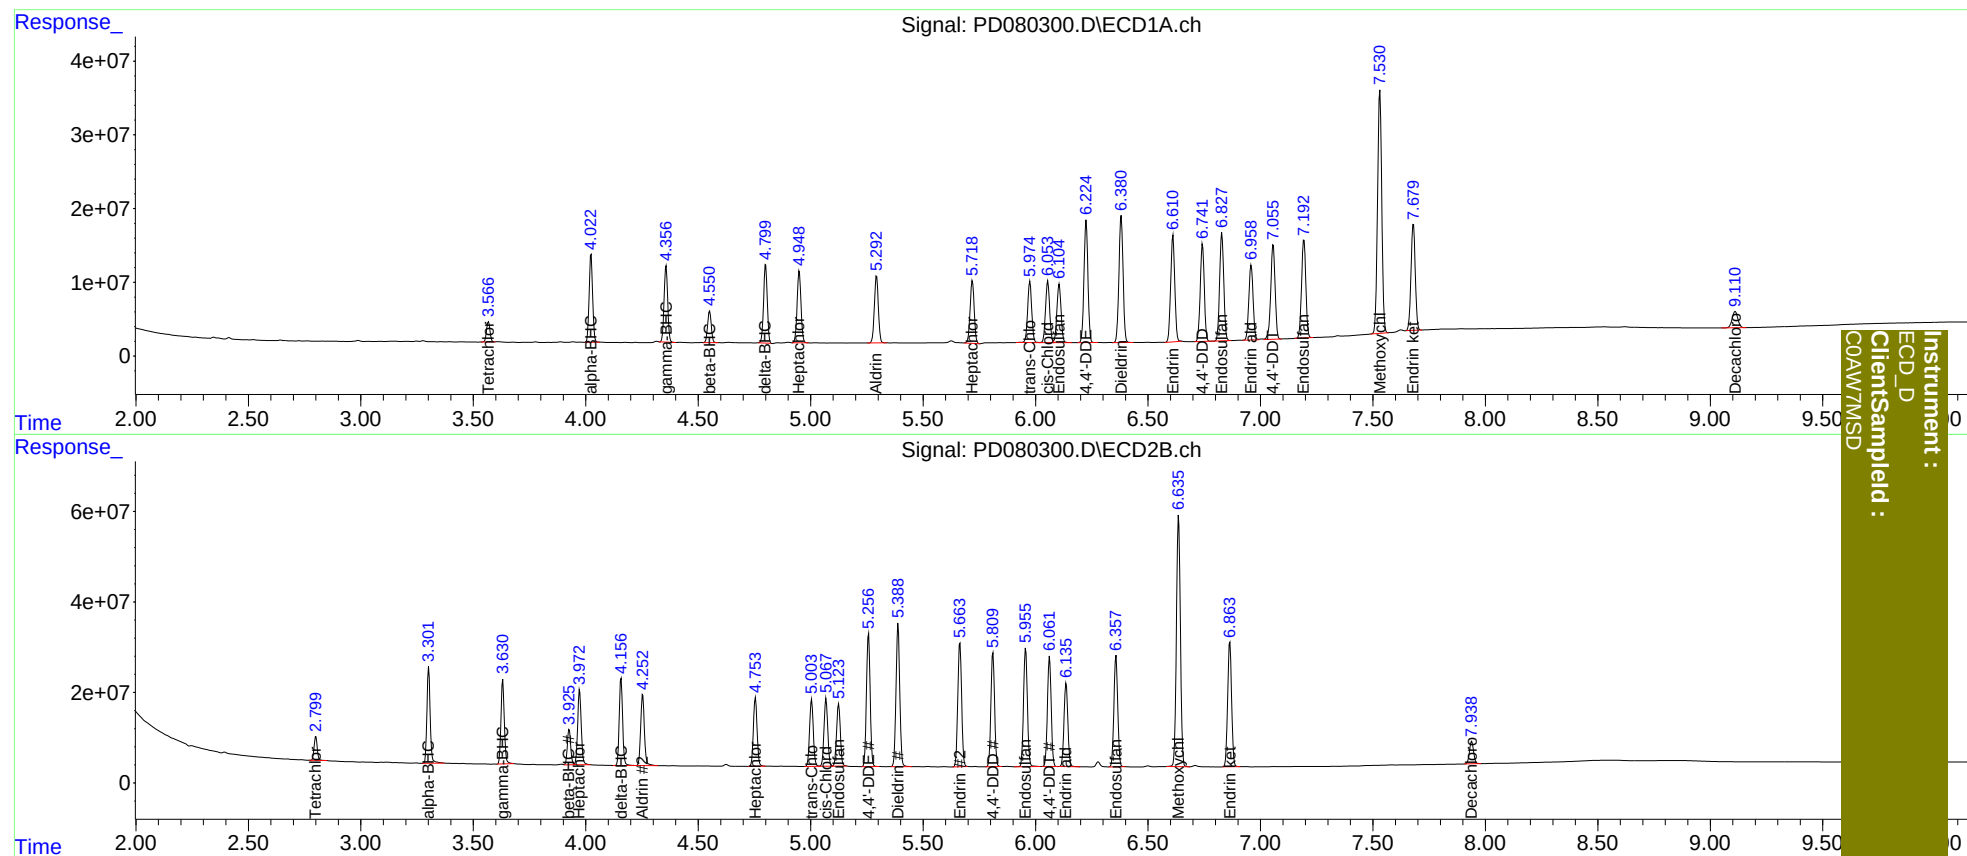

Instrument :
ECD_D
ClientSampled :
COAW/MSD